

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120822\
 Data File : FF011783.D
 Signal(s) : FID2B.ch
 Acq On : 08 Dec 2022 09:27
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 08 16:05:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
 Quant Title :
 QLast Update : Tue Dec 06 04:24:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.774	2552927	18.486 ug/ml
12)	N-OCTACOSANE	17.230	2369000	19.219 ug/ml
13)	N-TRIACONTANE	18.115	188707	1.558 ug/ml
14)	N-DOTRIACONTANE	18.948	249106	2.070 ug/ml
15)	N-TETRATRIACONTANE	19.731	207136	1.748 ug/ml
16)	N-HEXATRIACONTANE	20.470	145594	1.252 ug/ml
17)	N-OCTATRIACONTANE	21.211	93482	0.774 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120822\
Data File : FF011783.D
Signal(s) : FID2B.ch
Acq On : 08 Dec 2022 09:27
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 08 16:05:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

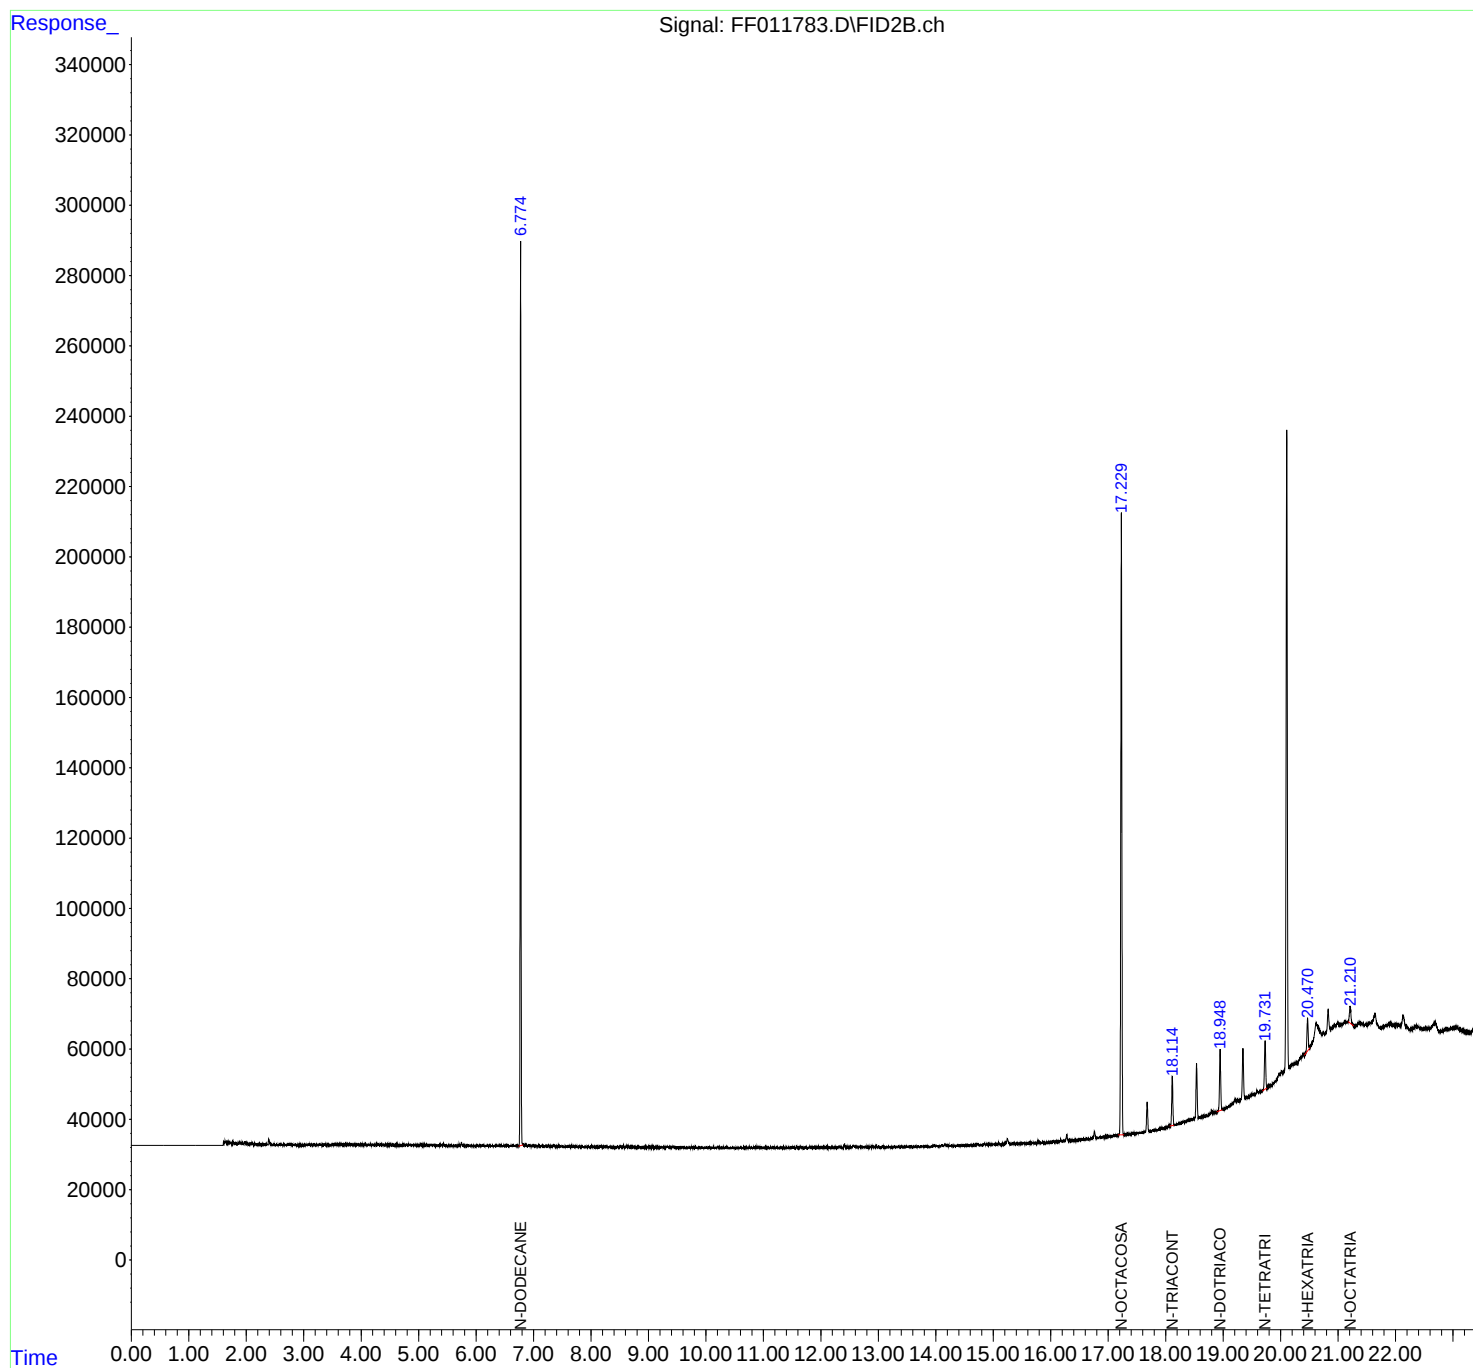


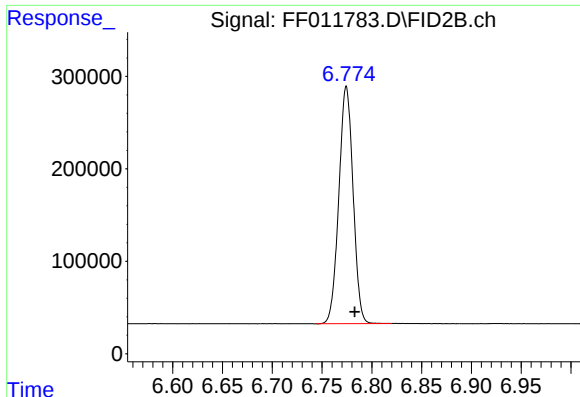

#3 N-DODECANE


R.T.: 6.774 min
Delta R.T.: -0.008 min
Response: 2552927
Conc: 18.49 ug/ml

Instrument :
FID_F
ClientSampleId :

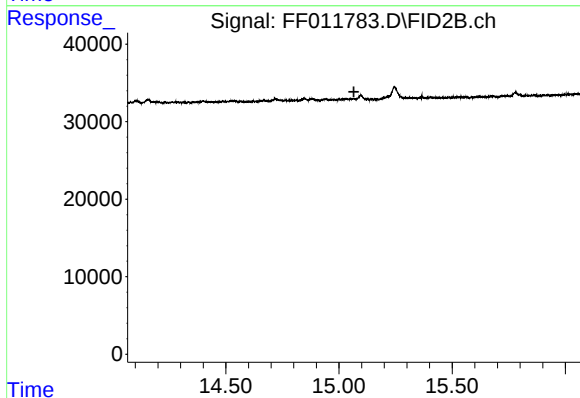


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.066 min
Response: 0
Conc: N.D.

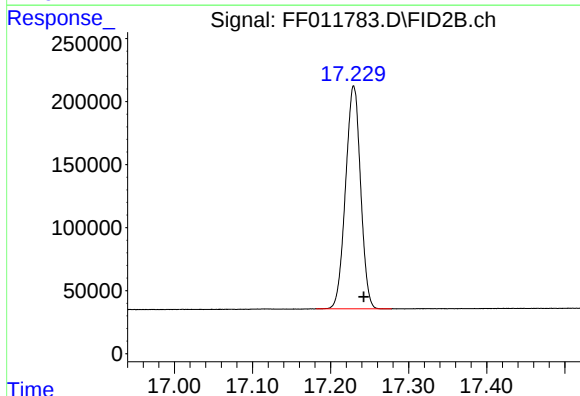


#12 N-OCTACOSANE

R.T.: 17.230 min
Delta R.T.: -0.013 min
Response: 2369000
Conc: 19.22 ug/ml

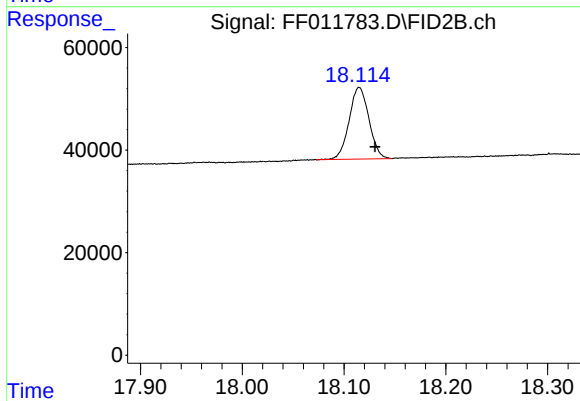

#13 N-TRIACONTANE


R.T.: 18.115 min
Delta R.T.: -0.015 min
Response: 188707
Conc: 1.56 ug/ml

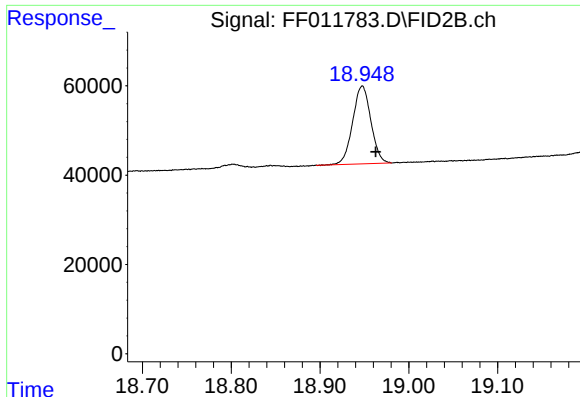

#14 N-DOTRIACONTANE


R.T.: 18.948 min
Delta R.T.: -0.015 min
Response: 249106
Conc: 2.07 ug/ml

Instrument :
FID_F
ClientSampleId :

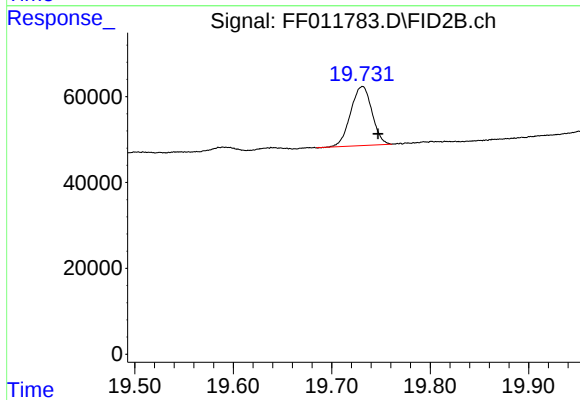


#15 N-TETRATRIACONTANE

R.T.: 19.731 min
Delta R.T.: -0.016 min
Response: 207136
Conc: 1.75 ug/ml

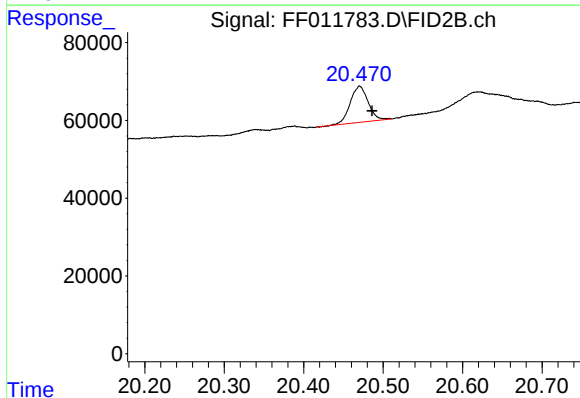

#16 N-HEXATRIACONTANE

R.T.: 20.470 min
Delta R.T.: -0.016 min
Response: 145594
Conc: 1.25 ug/ml

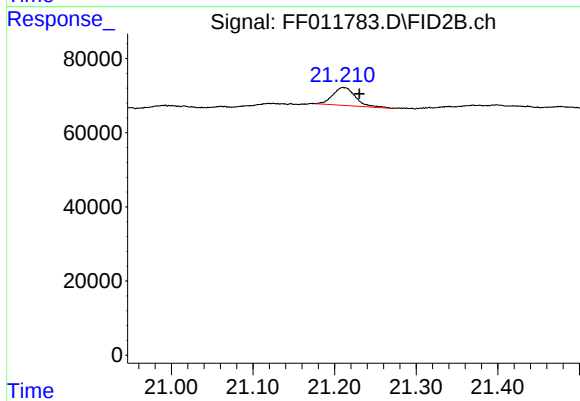

#17 N-OCTATRIACONTANE

R.T.: 21.211 min
Delta R.T.: -0.020 min
Response: 93482
Conc: 0.77 ug/ml