

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120822\
 Data File : FF011784.D
 Signal(s) : FID2B.ch
 Acq On : 08 Dec 2022 09:56
 Operator : YP\AJ
 Sample : N5908-01 20X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 08 16:05:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
 Quant Title :
 QLast Update : Tue Dec 06 04:24:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.054	615329	5.389 ug/ml
Target Compounds			
5) N-HEXADECANE	10.235	66355	0.479 ug/ml
6) N-OCTADECANE	11.673	157962	1.135 ug/ml
7) N-EICOSANE	12.948	795617	5.877 ug/ml
8) N-DOCOSANE	14.189	312927	2.362 ug/ml
10) N-TETRACOSANE	15.272	144179	1.097 ug/ml
11) N-HEXACOSANE	16.268	29767	0.235 ug/ml
12) N-OCTACOSANE	17.234	69426	0.563 ug/ml
15) N-TETRATRIACONTANE	19.727	66932	0.565 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120822\
Data File : FF011784.D
Signal(s) : FID2B.ch
Acq On : 08 Dec 2022 09:56
Operator : YP\AJ
Sample : N5908-01 20X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 08 16:05:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

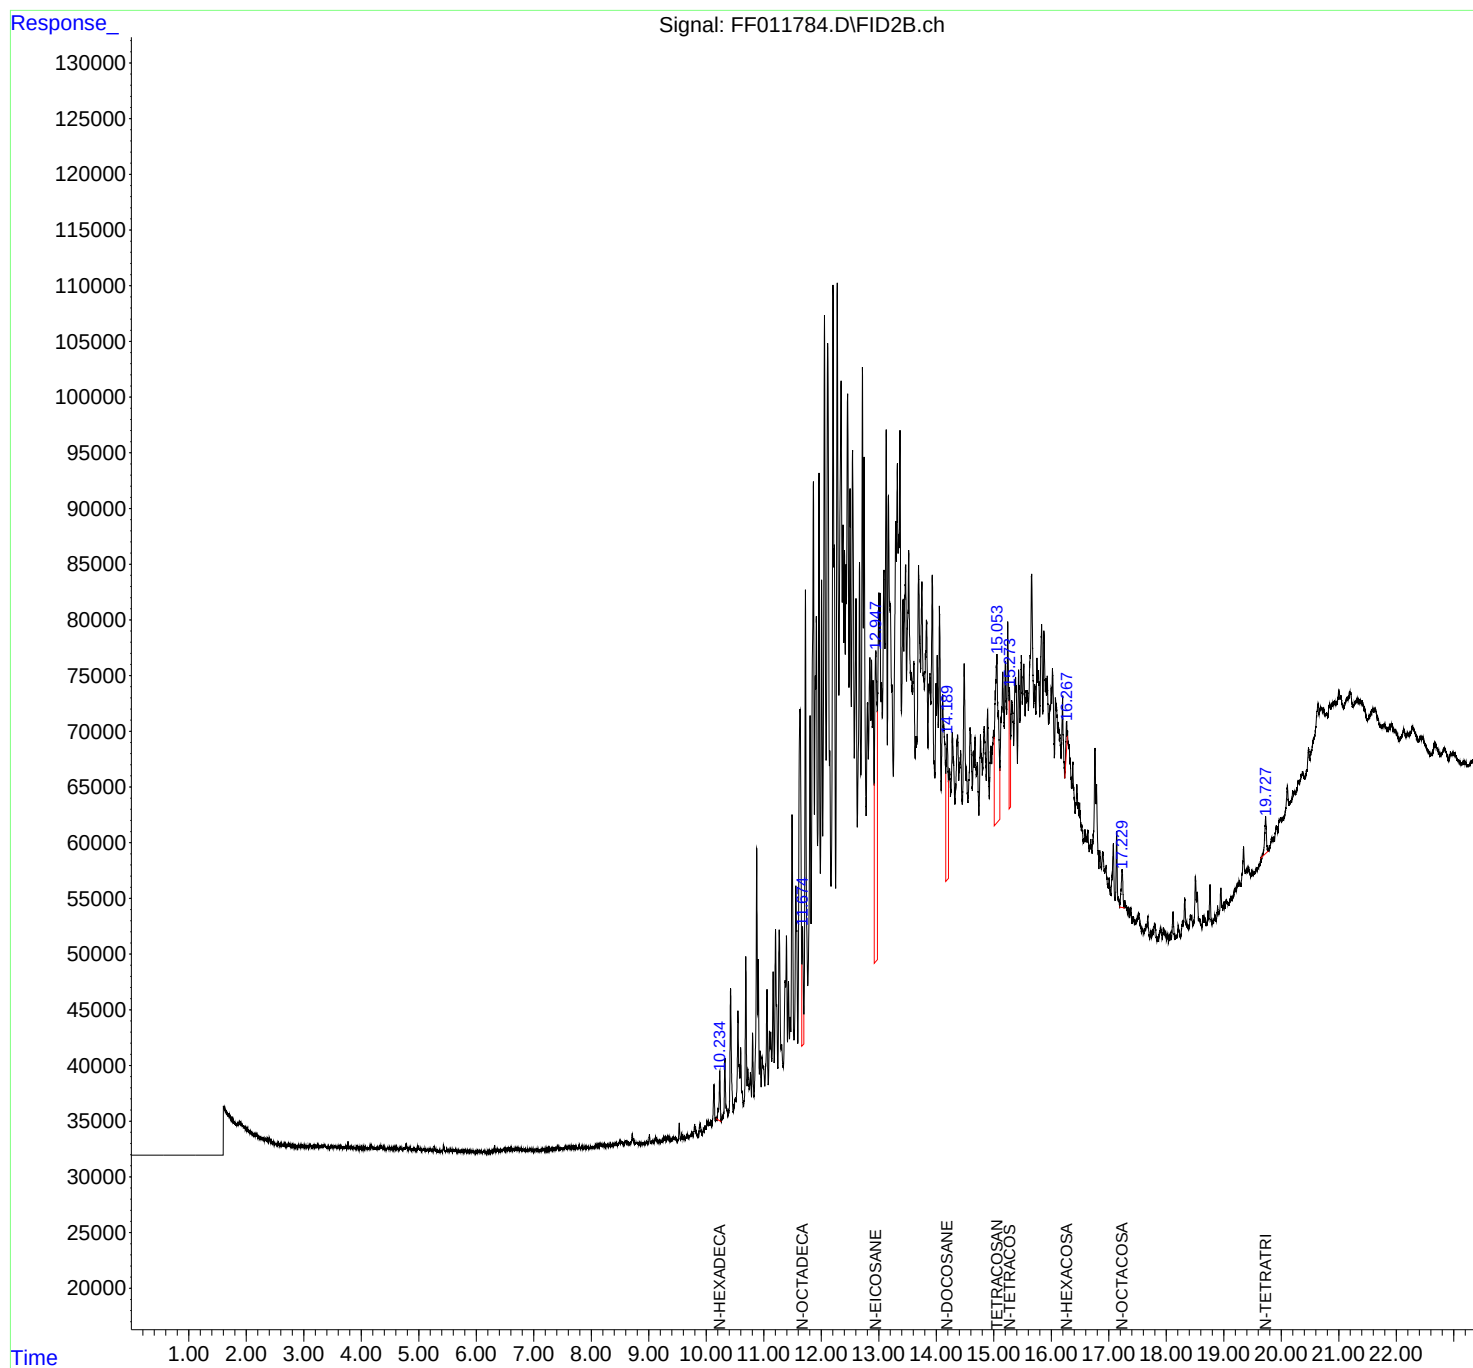


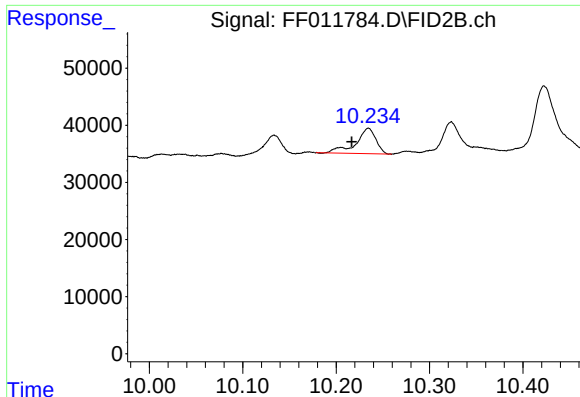

#5 N-HEXADECANE


R.T.: 10.235 min
Delta R.T.: 0.018 min
Response: 66355
Conc: 0.48 ug/ml

Instrument :
FID_F
ClientSampleId :

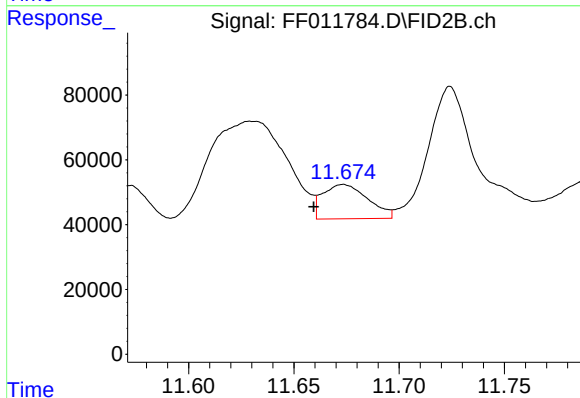


#6 N-OCTADECANE

R.T.: 11.673 min
Delta R.T.: 0.014 min
Response: 157962
Conc: 1.14 ug/ml

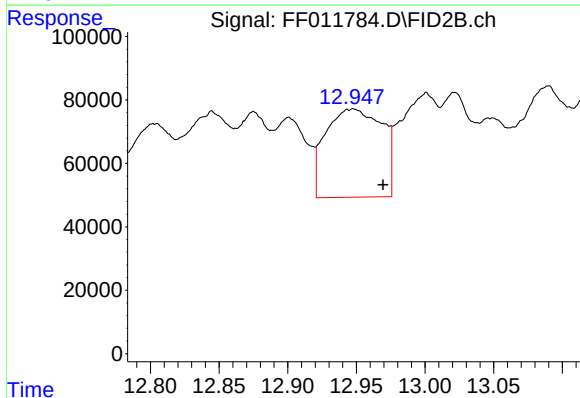


#7 N-EICOSANE

R.T.: 12.948 min
Delta R.T.: -0.022 min
Response: 795617
Conc: 5.88 ug/ml

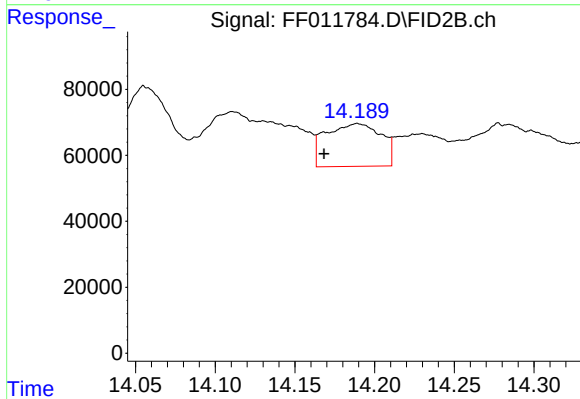

#8 N-DOCOSANE


R.T.: 14.189 min
Delta R.T.: 0.021 min
Response: 312927
Conc: 2.36 ug/ml

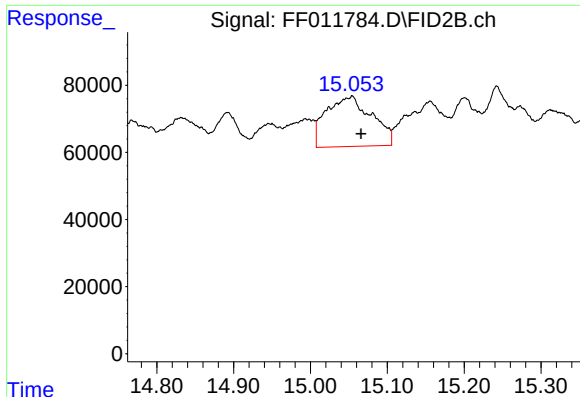

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.054 min
Delta R.T.: -0.011 min
Response: 615329
Conc: 5.39 ug/ml

Instrument :
FID_F
ClientSampleId :

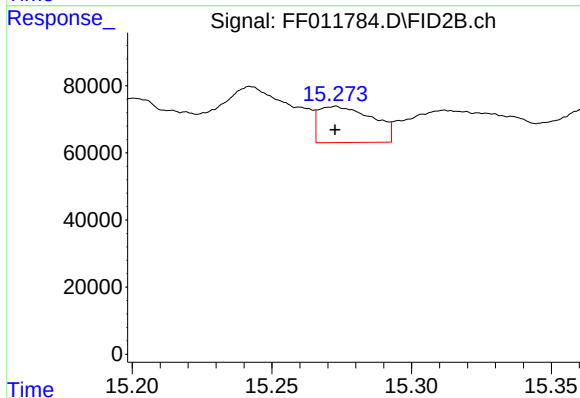


#10 N-TETRACOSANE

R.T.: 15.272 min
Delta R.T.: 0.000 min
Response: 144179
Conc: 1.10 ug/ml

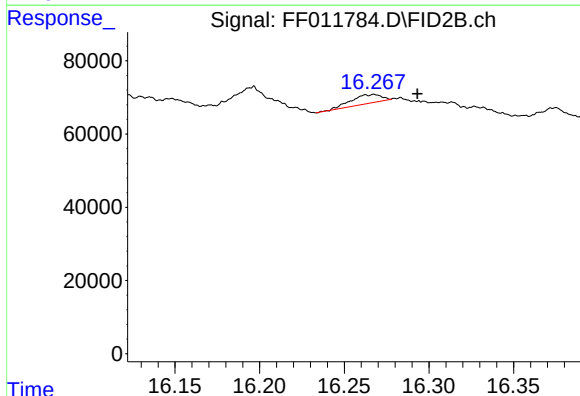


#11 N-HEXACOSANE

R.T.: 16.268 min
Delta R.T.: -0.026 min
Response: 29767
Conc: 0.23 ug/ml

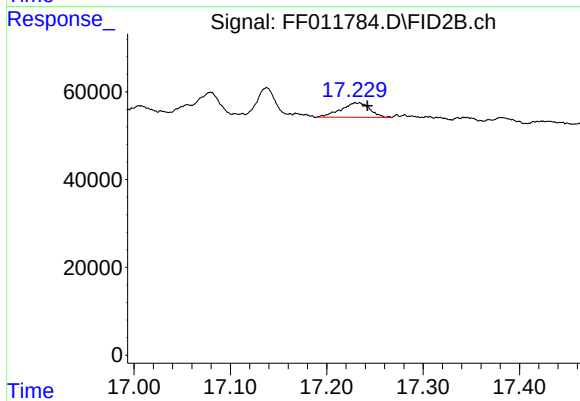

#12 N-OCTACOSANE

R.T.: 17.234 min
Delta R.T.: -0.009 min
Response: 69426
Conc: 0.56 ug/ml

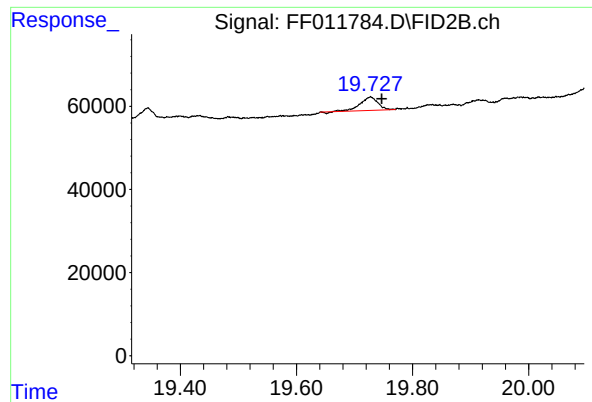

#15 N-TETRATRIACONTANE

R.T.: 19.727 min
Delta R.T.: -0.020 min
Response: 66932
Conc: 0.56 ug/ml

Instrument :

FID_F

ClientSampleId :