

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120822\
Data File : FF011784.D
Signal(s) : FID2B.ch
Acq On : 08 Dec 2022 09:56
Operator : YP\AJ
Sample : N5908-01 20X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SP25-12-20221206-6.5-7.0

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/09/2022
Supervised By :Ankita Jodhani 12/09/2022

Integration File: Sample.e
Quant Time: Dec 08 16:05:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.053	258613	2.265 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120822\
Data File : FF011784.D
Signal(s) : FID2B.ch
Acq On : 08 Dec 2022 09:56
Operator : YP\AJ
Sample : N5908-01 20X
Misc :
ALS Vial : 56 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
SP25-12-20221206-6.5-7.0


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/09/2022
Supervised By :Ankita Jodhani 12/09/2022

Integration File: Sample.e
Quant Time: Dec 08 16:05:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

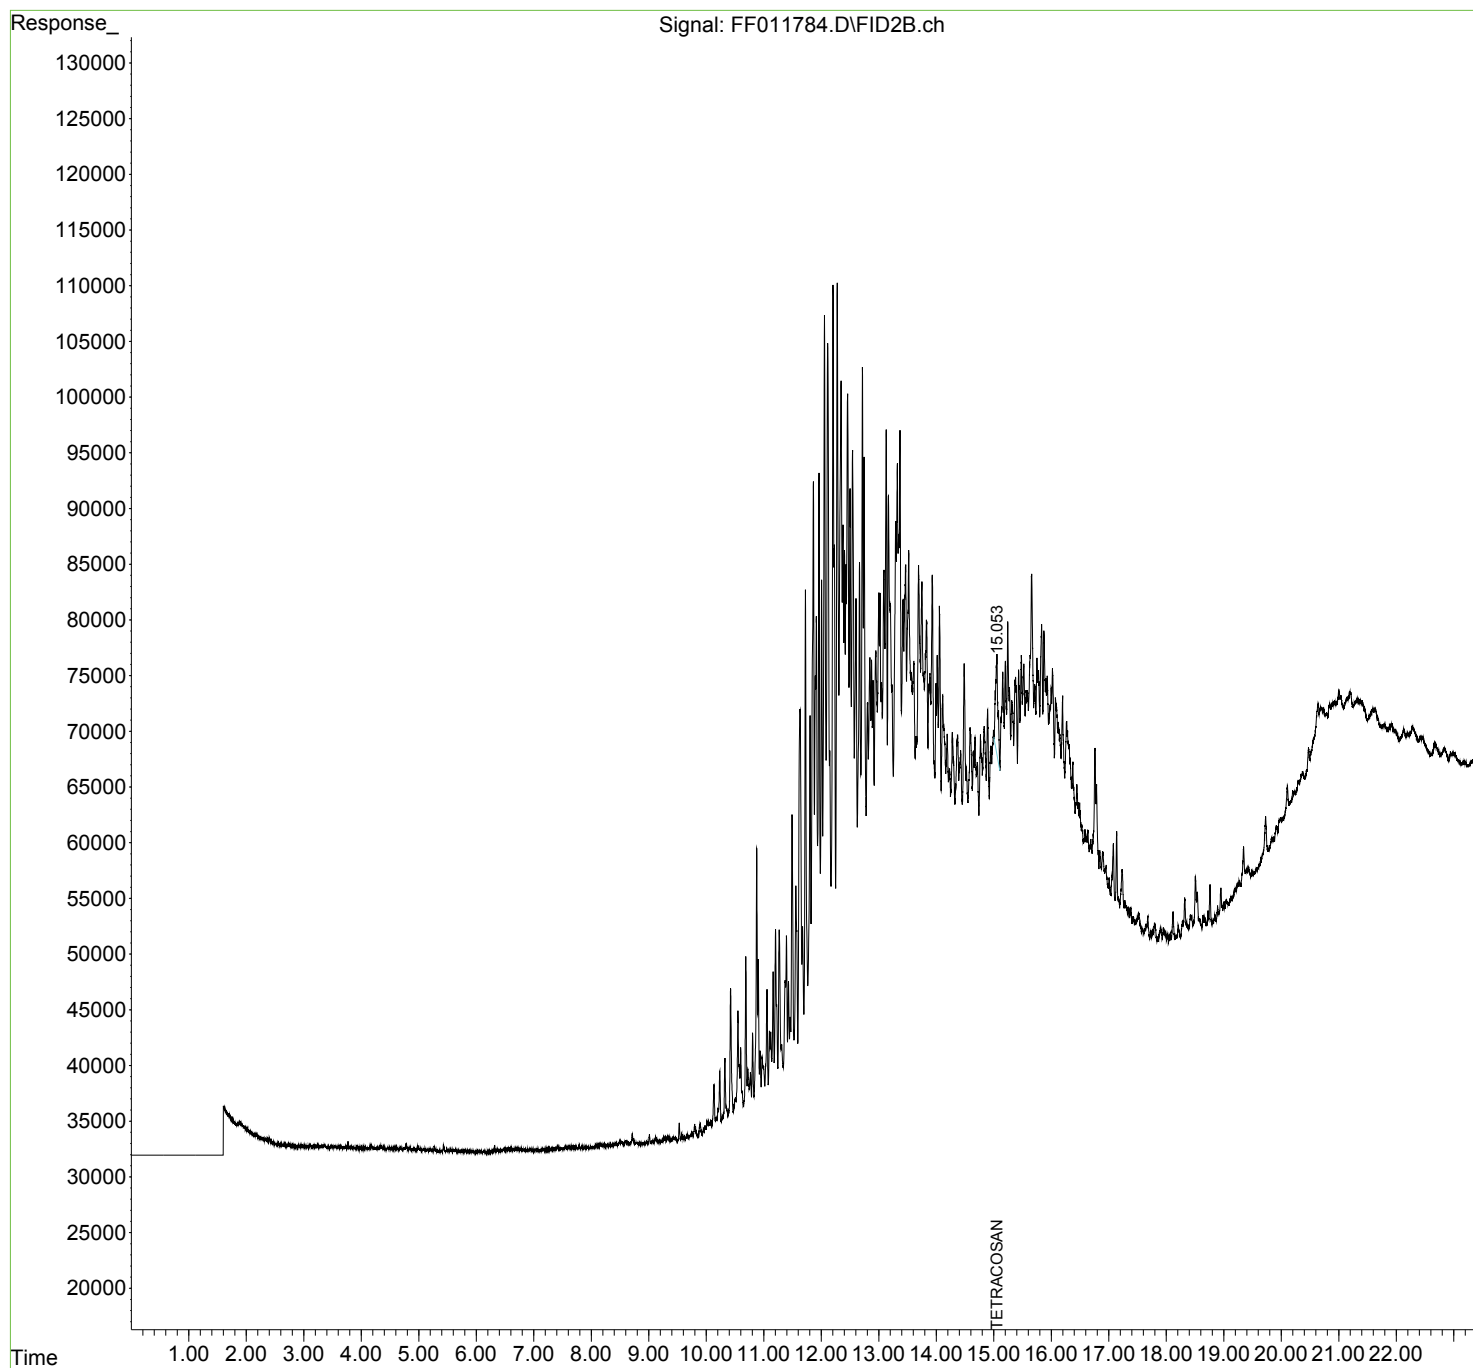

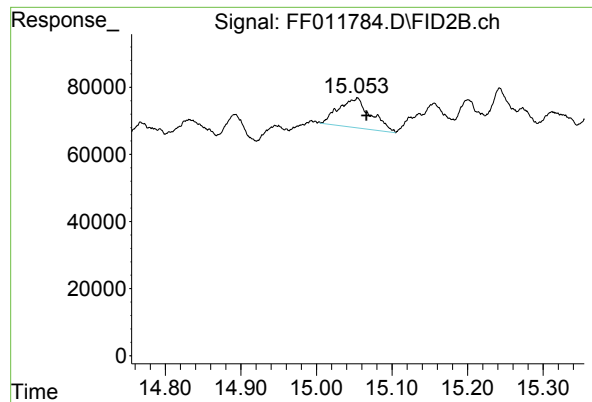

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.053 min
Delta R.T.: -0.013 min
Response: 258613
Conc: 2.26 ug/ml

Instrument :
FID_F
ClientSampleId :
SP25-12-20221206-6.5-7.0

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/09/2022
Supervised By :Ankita Jodhani 12/09/2022