

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120920\
Data File : FF007940.D
Signal(s) : FID2B.ch
Acq On : 09 Dec 2020 15:48
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 10 00:35:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120220.M
Quant Title :
QLast Update : Thu Dec 03 09:08:10 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.711	2296837	18.167 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.780	83484	0.659 ug/ml
14) N-DOTRIACONTANE	18.617	388273	3.503 ug/ml
16) N-HEXATRIACONTANE	20.148	112609	1.734 ug/ml
18) N-TETRACONTANE	21.891f	415186	7.402 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120920\
Data File : FF007940.D
Signal(s) : FID2B.ch
Acq On : 09 Dec 2020 15:48
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 10 00:35:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120220.M
Quant Title :
QLast Update : Thu Dec 03 09:08:10 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

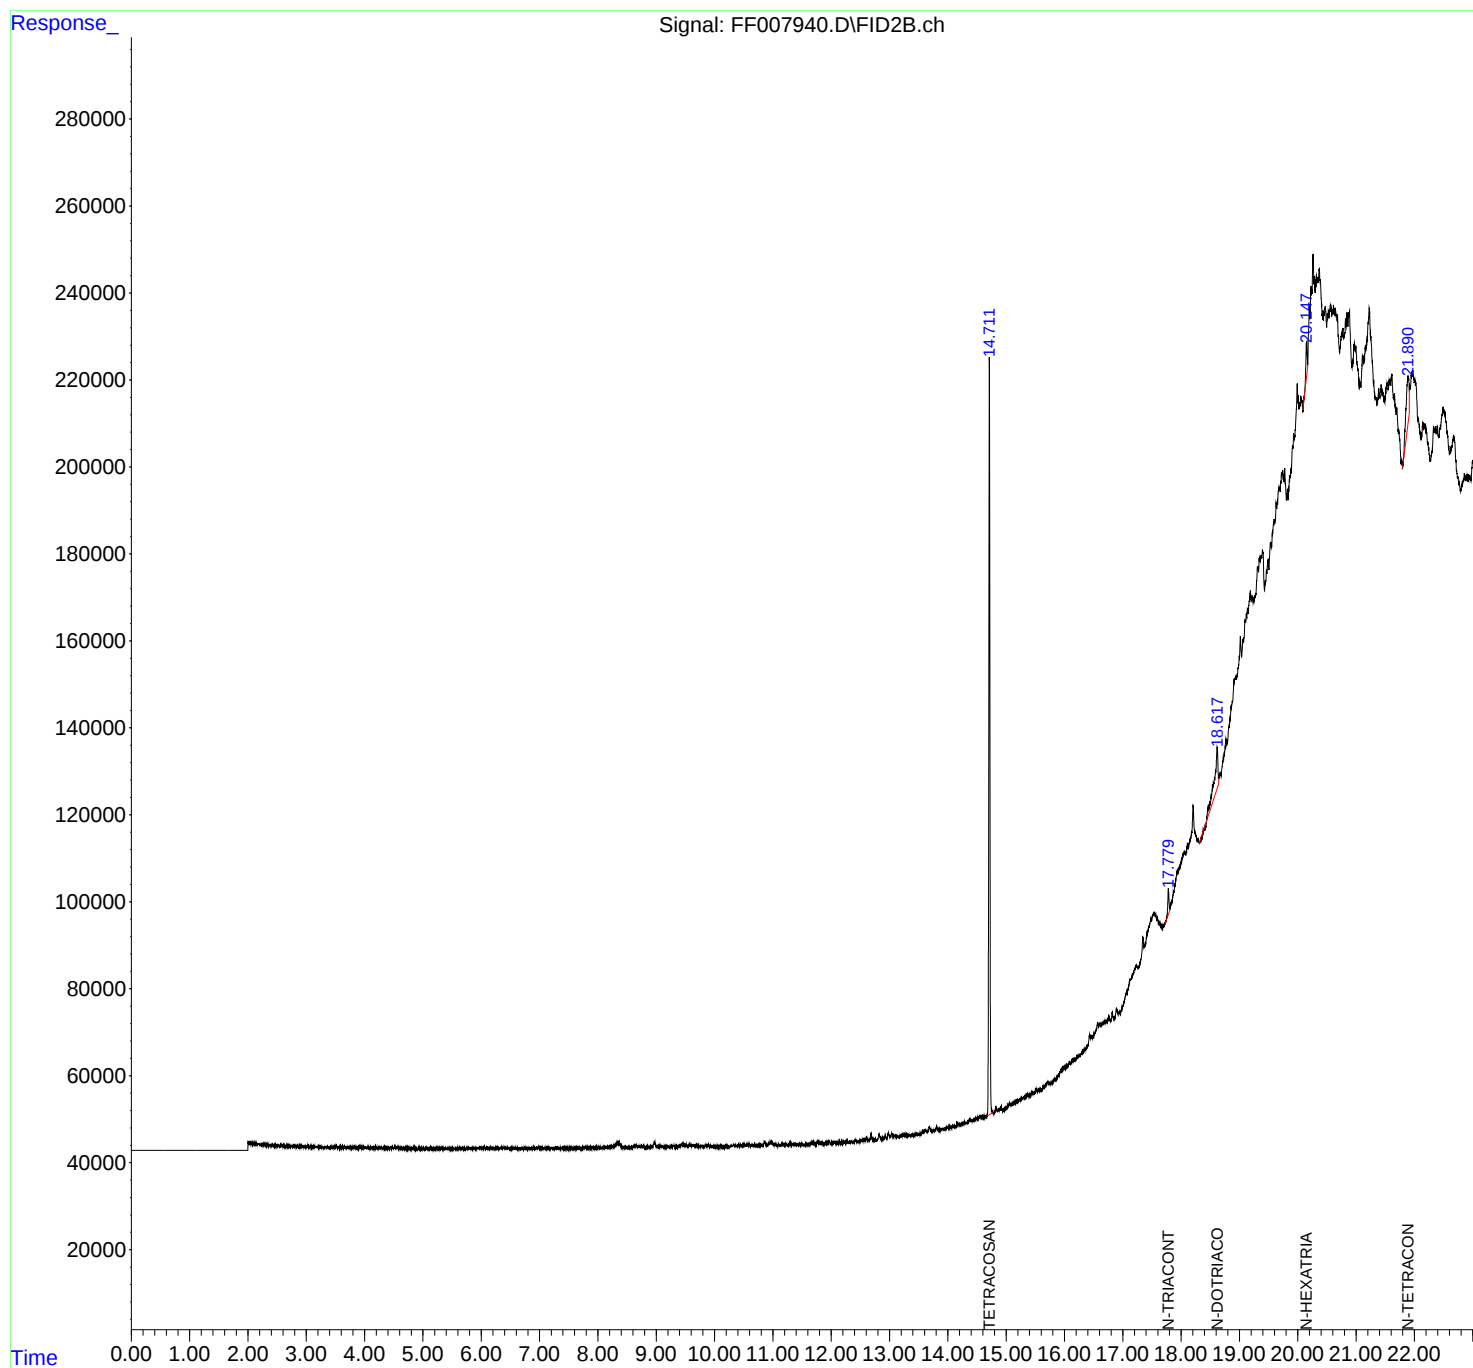

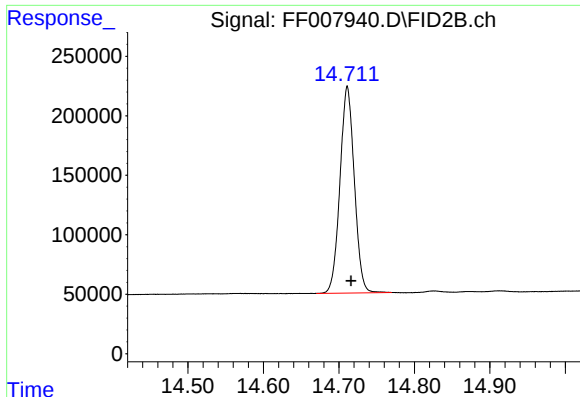


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.711 min
Delta R.T.: -0.005 min
Response: 2296837
Conc: 18.17 ug/ml

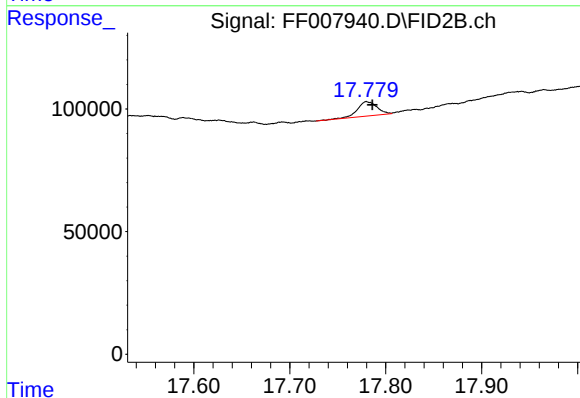


#13 N-TRIACONTANE

R.T.: 17.780 min
Delta R.T.: -0.006 min
Response: 83484
Conc: 0.66 ug/ml

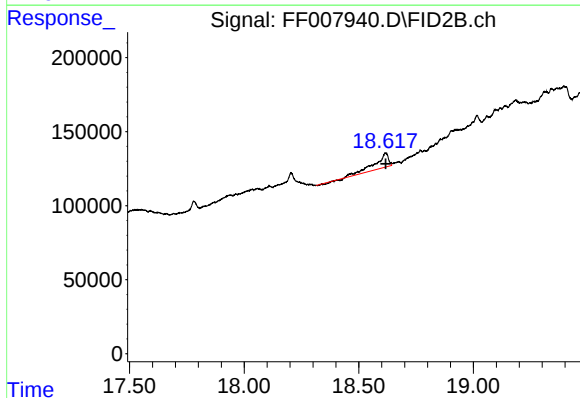


#14 N-DOTRIACONTANE

R.T.: 18.617 min
Delta R.T.: -0.001 min
Response: 388273
Conc: 3.50 ug/ml

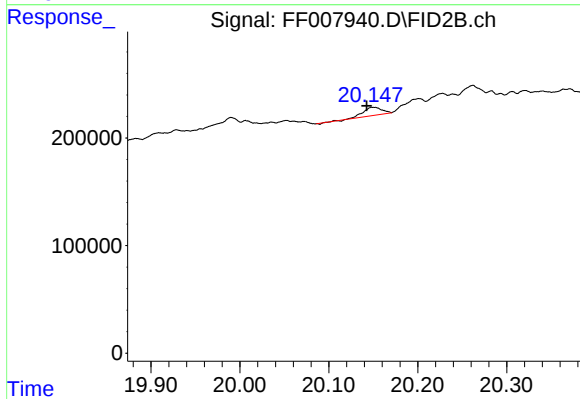

#16 N-HEXATRIACONTANE

R.T.: 20.148 min
Delta R.T.: 0.006 min
Response: 112609
Conc: 1.73 ug/ml

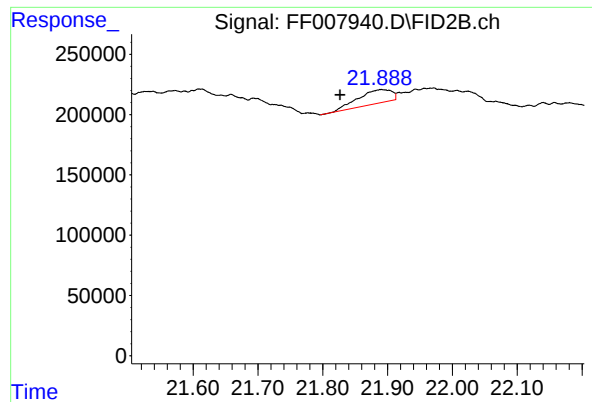

#18 N-TETRACONTANE

R.T.: 21.891 min
Delta R.T.: 0.064 min
Response: 415186
Conc: 7.40 ug/ml