

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121018\
Data File : FF002954.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2018 11:50
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 11 00:56:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.380	3475422	21.886 ug/ml
10) N-TETRACOSANE	14.817	133408	0.923 ug/ml
12) N-OCTACOSANE	16.820	3105903	23.181 ug/ml
13) N-TRIACONTANE	17.710	243336	1.899 ug/ml
14) N-DOTRIACONTANE	18.547	336528	2.818 ug/ml
15) N-TETRATRIACONTANE	19.335	241510	2.131 ug/ml
16) N-HEXATRIACONTANE	20.080	135583	1.257 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121018\
Data File : FF002954.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2018 11:50
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 11 00:56:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

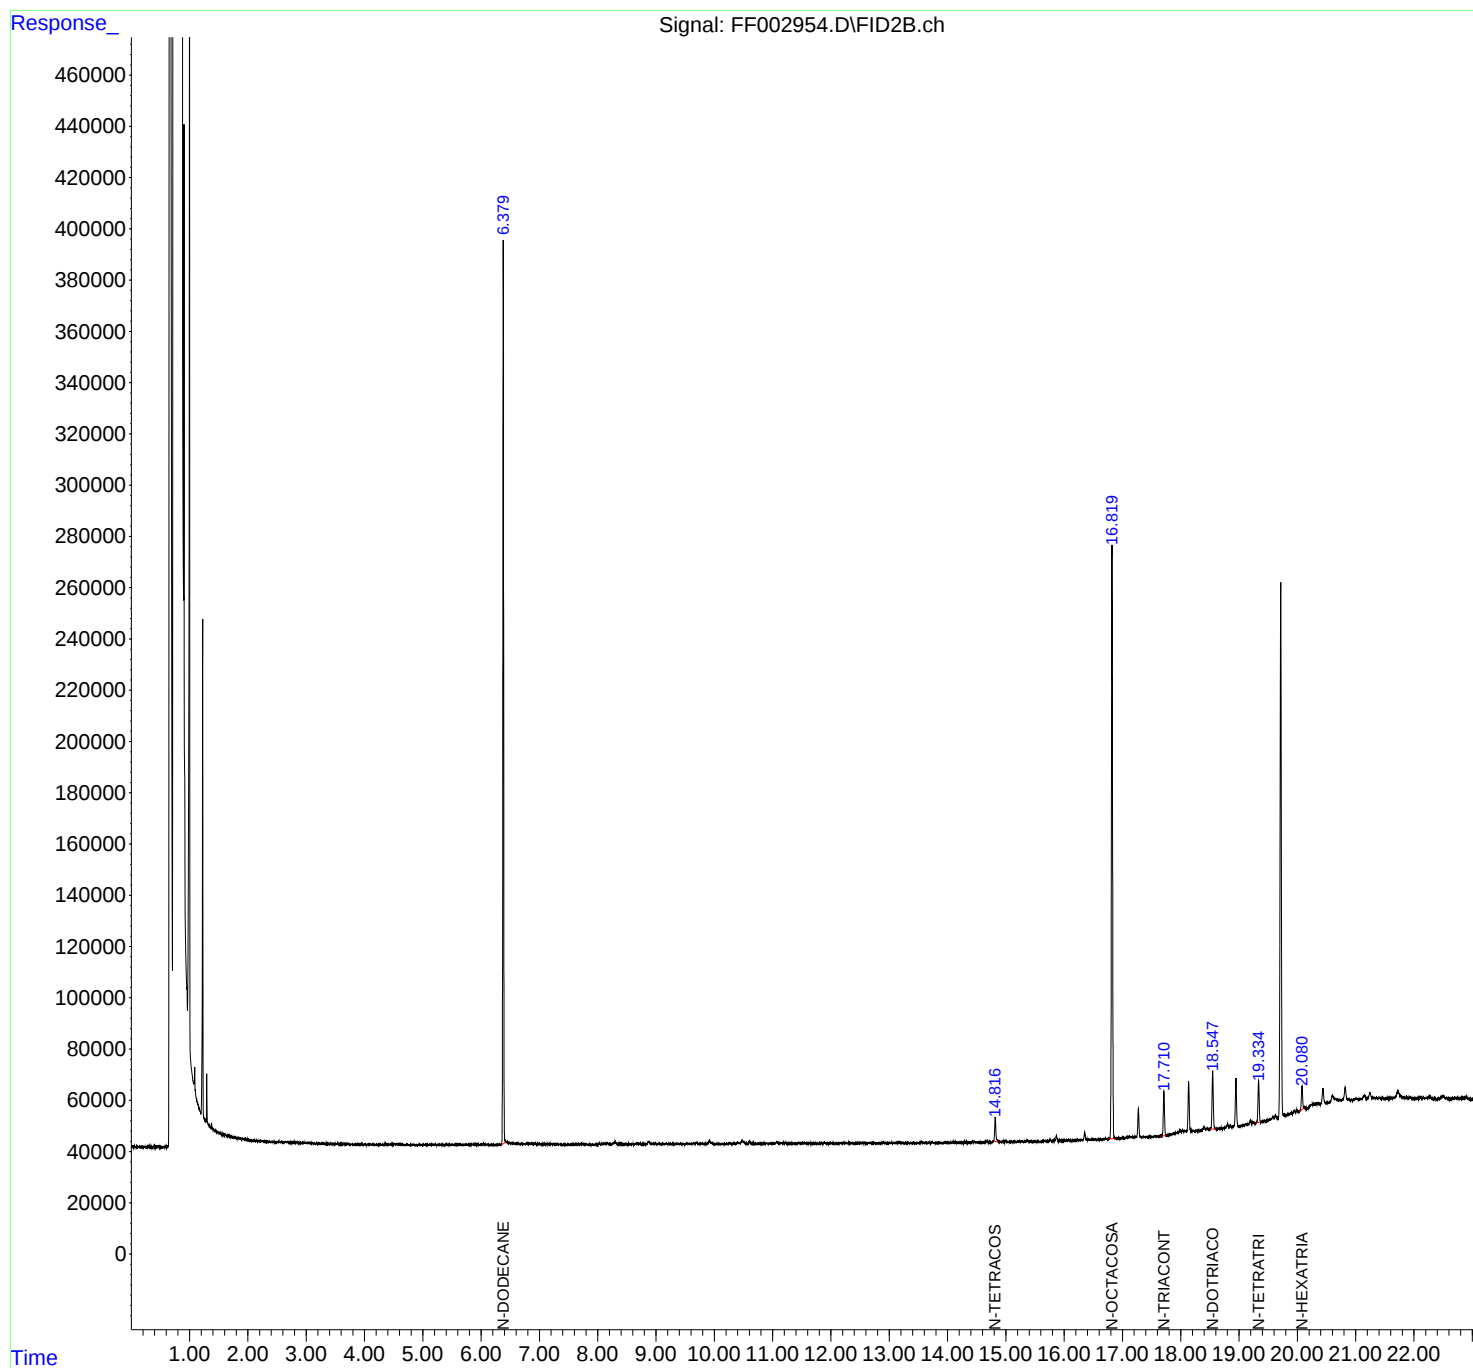


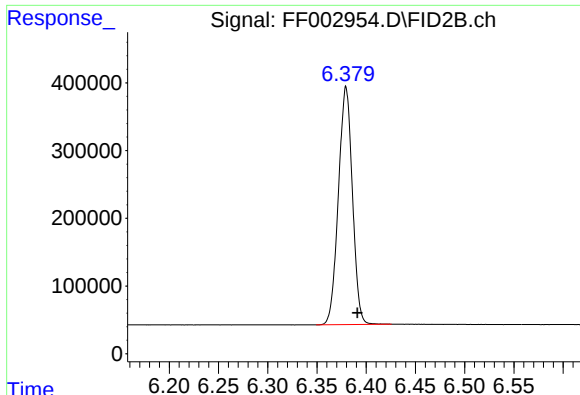

#3 N-DODECANE


R.T.: 6.380 min
Delta R.T.: -0.011 min
Response: 3475422
Conc: 21.89 ug/ml

Instrument :
FID_F
ClientSampleId :

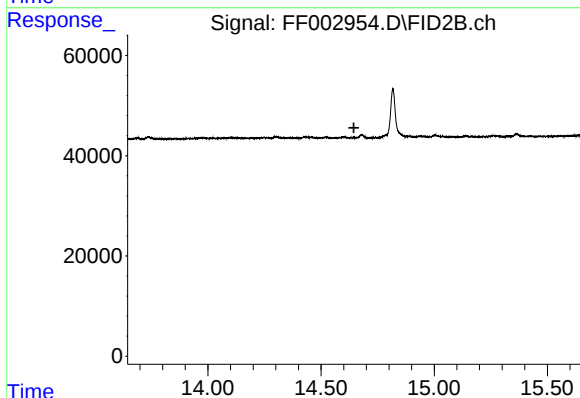


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.645 min
Response: 0
Conc: N.D.

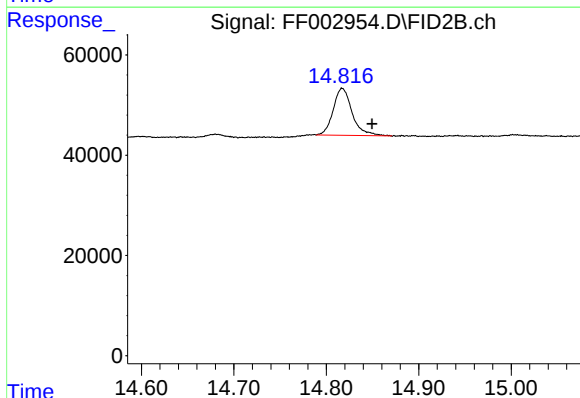


#10 N-TETRACOSANE

R.T.: 14.817 min
Delta R.T.: -0.032 min
Response: 133408
Conc: 0.92 ug/ml

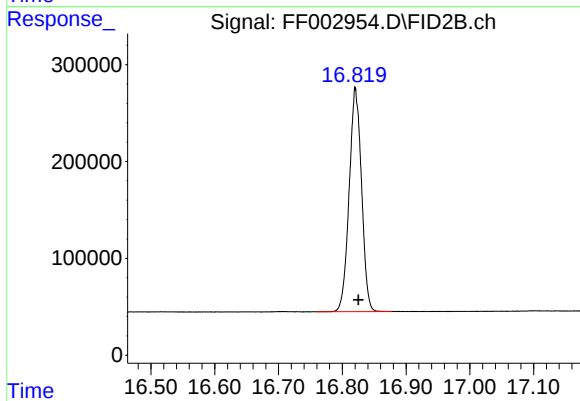

#12 N-OCTACOSANE


R.T.: 16.820 min
Delta R.T.: -0.005 min
Response: 3105903
Conc: 23.18 ug/ml

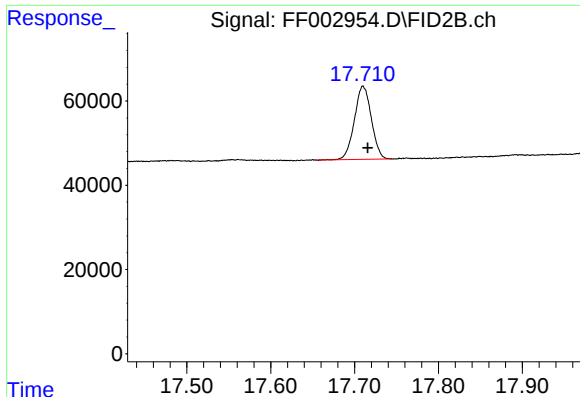

#13 N-TRIACONTANE


R.T.: 17.710 min
Delta R.T.: -0.005 min
Response: 243336
Conc: 1.90 ug/ml

Instrument :
FID_F
ClientSampleId :

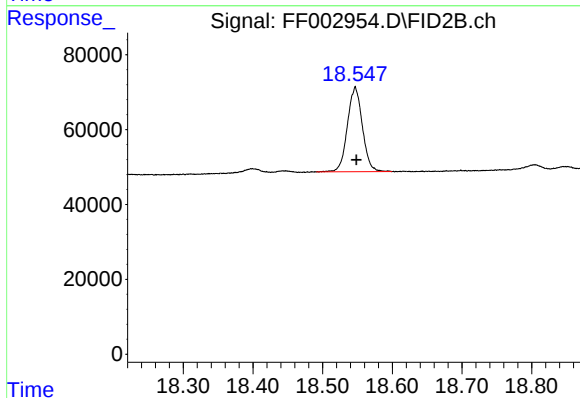


#14 N-DOTRIACONTANE

R.T.: 18.547 min
Delta R.T.: -0.002 min
Response: 336528
Conc: 2.82 ug/ml

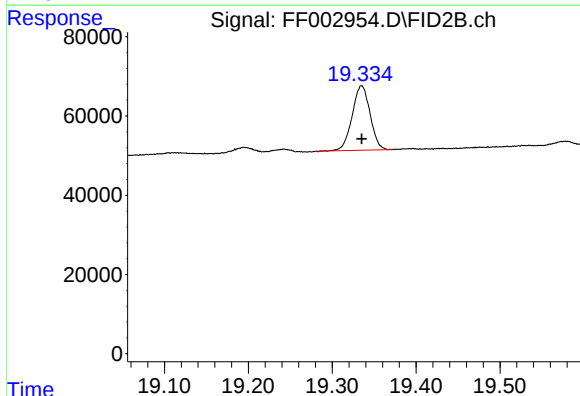

#15 N-TETRATRIACONTANE

R.T.: 19.335 min
Delta R.T.: 0.000 min
Response: 241510
Conc: 2.13 ug/ml

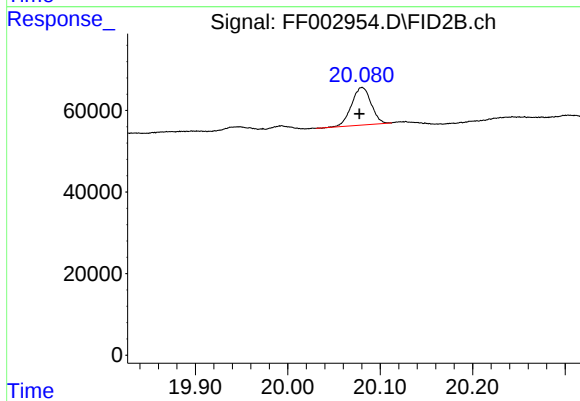

#16 N-HEXATRIACONTANE

R.T.: 20.080 min
Delta R.T.: 0.003 min
Response: 135583
Conc: 1.26 ug/ml