

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121018\
Data File : FF002955.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2018 12:37
Operator : AJ\SJ
Sample : J6261-01 500X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 11 00:57:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

4)	N-TETRADECANE	8.175	85967	0.536 ug/ml
5)	N-HEXADECANE	9.779	115915	0.724 ug/ml
6)	N-OCTADECANE	11.223	373323	2.357 ug/ml
7)	N-EICOSANE	12.537	121248	0.786 ug/ml
10)	N-TETRACOSANE	14.817	126511	0.875 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121018\
Data File : FF002955.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2018 12:37
Operator : AJ\SJ
Sample : J6261-01 500X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 11 00:57:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

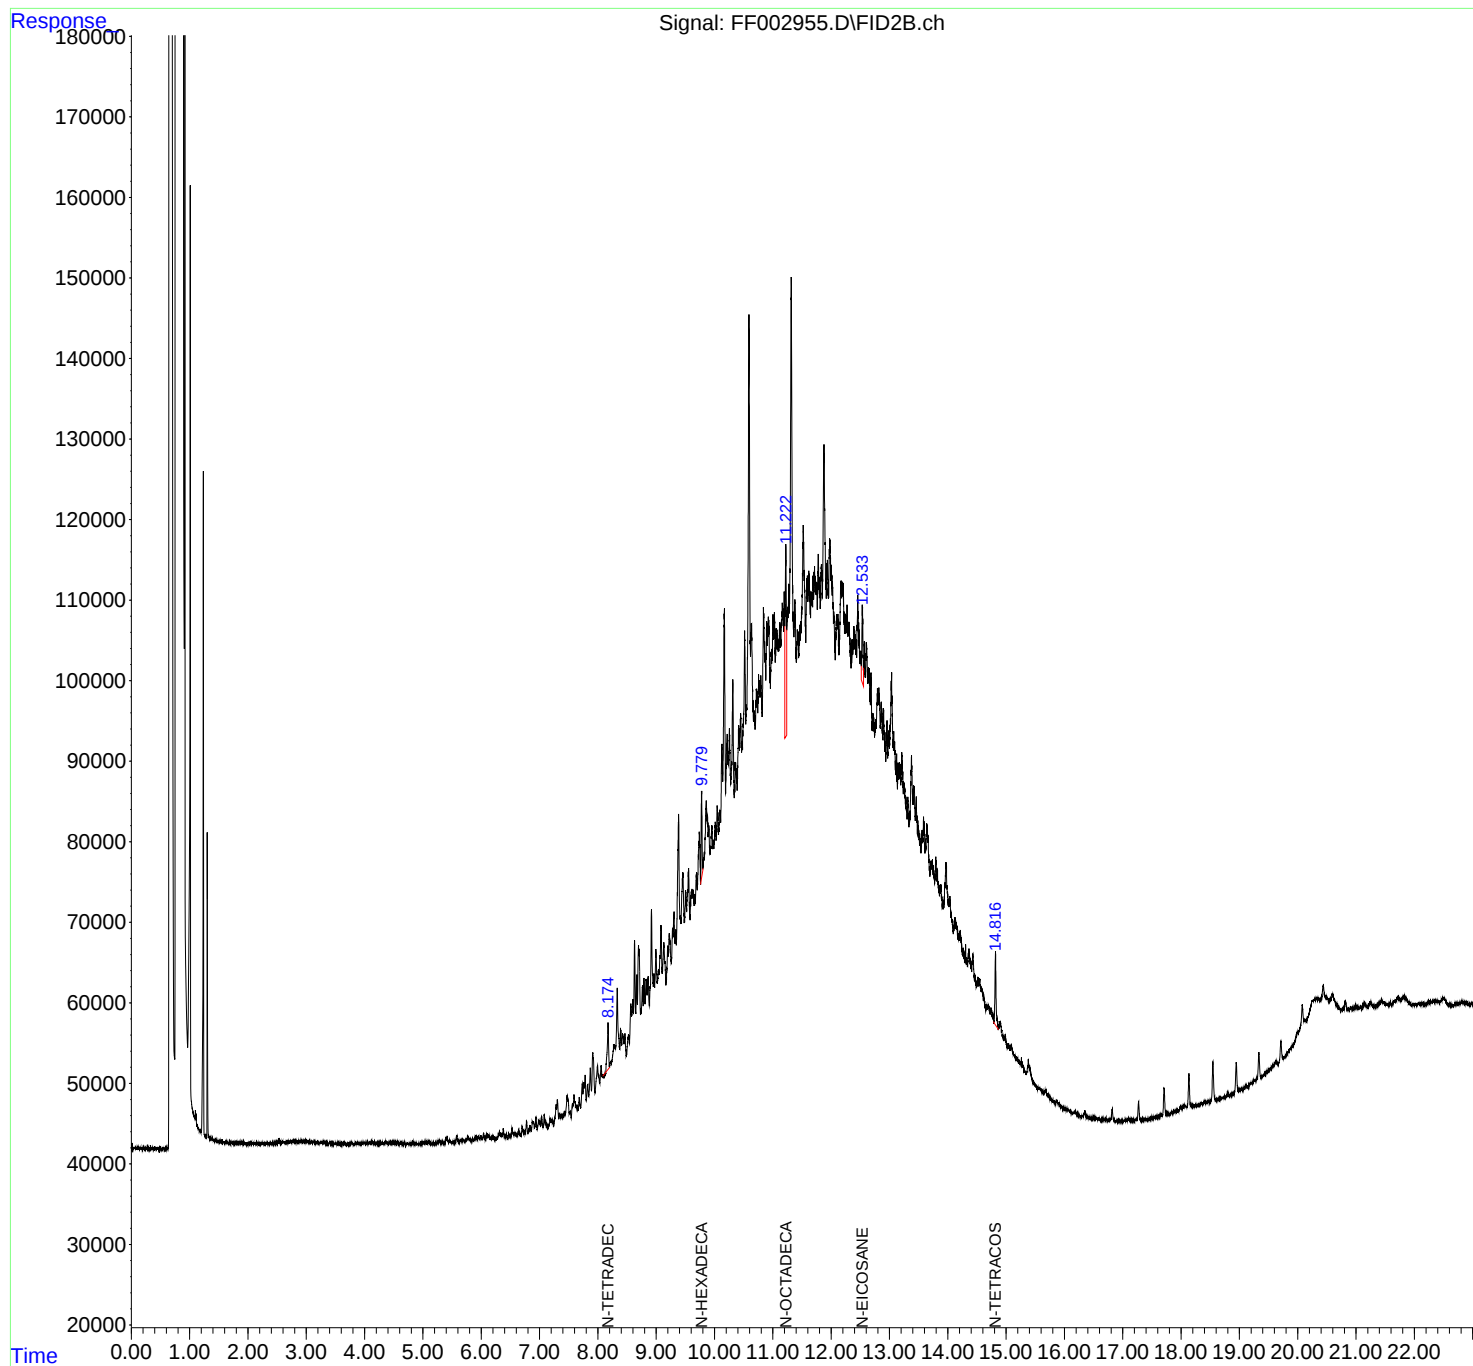


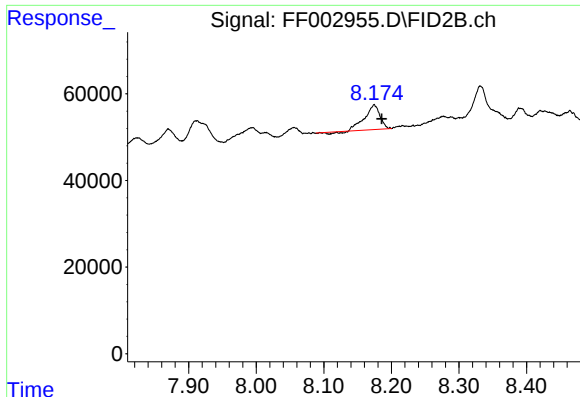

#4 N-TETRADECANE


R.T.: 8.175 min
Delta R.T.: -0.011 min
Response: 85967
Conc: 0.54 ug/ml

Instrument :
FID_F
ClientSampleId :

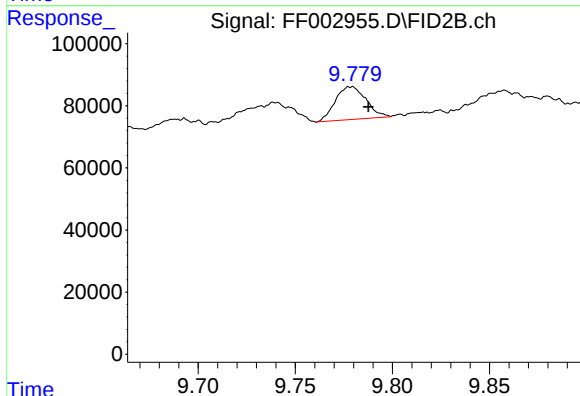


#5 N-HEXADECANE

R.T.: 9.779 min
Delta R.T.: -0.009 min
Response: 115915
Conc: 0.72 ug/ml

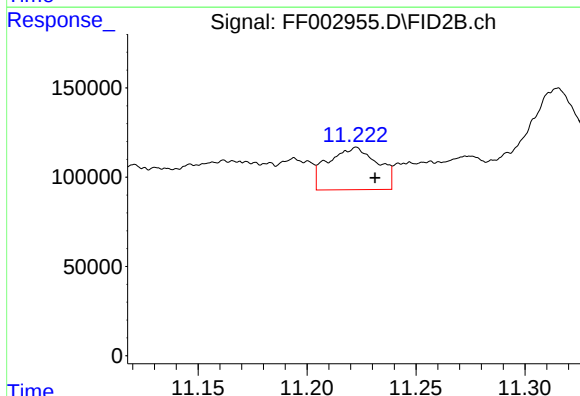


#6 N-OCTADECANE

R.T.: 11.223 min
Delta R.T.: -0.009 min
Response: 373323
Conc: 2.36 ug/ml

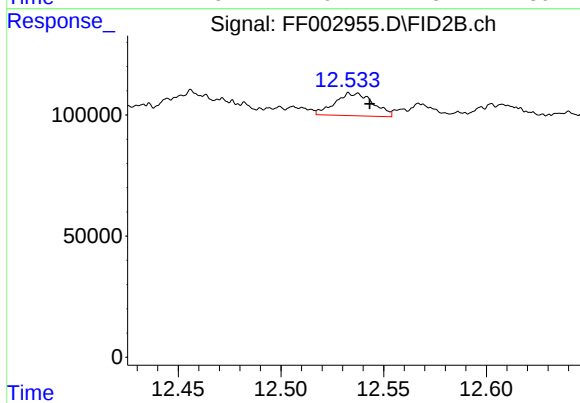

#7 N-EICOSANE


R.T.: 12.537 min
Delta R.T.: -0.007 min
Response: 121248
Conc: 0.79 ug/ml

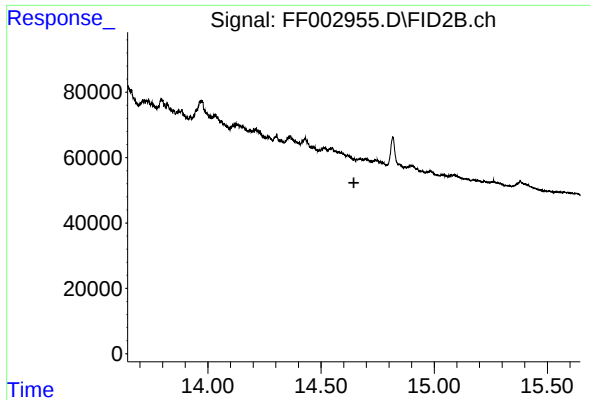

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.645 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

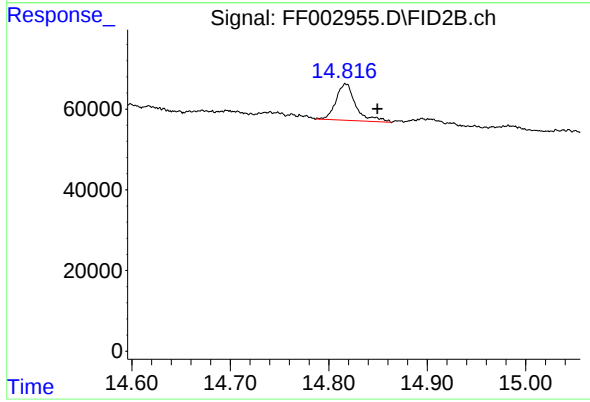

#10 N-TETRACOSANE

R.T.: 14.817 min
Delta R.T.: -0.032 min
Response: 126511
Conc: 0.88 ug/ml