

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121018\
 Data File : FF002959.D
 Signal(s) : FID2B.ch
 Acq On : 10 Dec 2018 16:04
 Operator : AJ\SJ
 Sample : J6316-01
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 11 00:57:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.642	2053911	15.821 ug/ml
Target Compounds			
2) N-DECANE	4.432f	73909	0.472 ug/ml
3) N-DODECANE	6.390	1217963	7.670 ug/ml
4) N-TETRADECANE	8.156	292982	1.828 ug/ml
7) N-EICOSANE	12.538	149800	0.971 ug/ml
8) N-DOCOSANE	13.755	533389	3.567 ug/ml
10) N-TETRACOSANE	14.814	1862888	12.891 ug/ml
11) N-HEXACOSANE	15.869	199343	1.428 ug/ml
12) N-OCTACOSANE	16.817	495137	3.695 ug/ml
13) N-TRIACONTANE	17.713	407189	3.178 ug/ml
14) N-DOTRIACONTANE	18.544	206834	1.732 ug/ml
16) N-HEXATRIACONTANE	20.079	64657	0.599 ug/ml
18) N-TETRACONTANE	21.705	84362	0.803 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121018\
Data File : FF002959.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2018 16:04
Operator : AJ\SJ
Sample : J6316-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 11 00:57:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

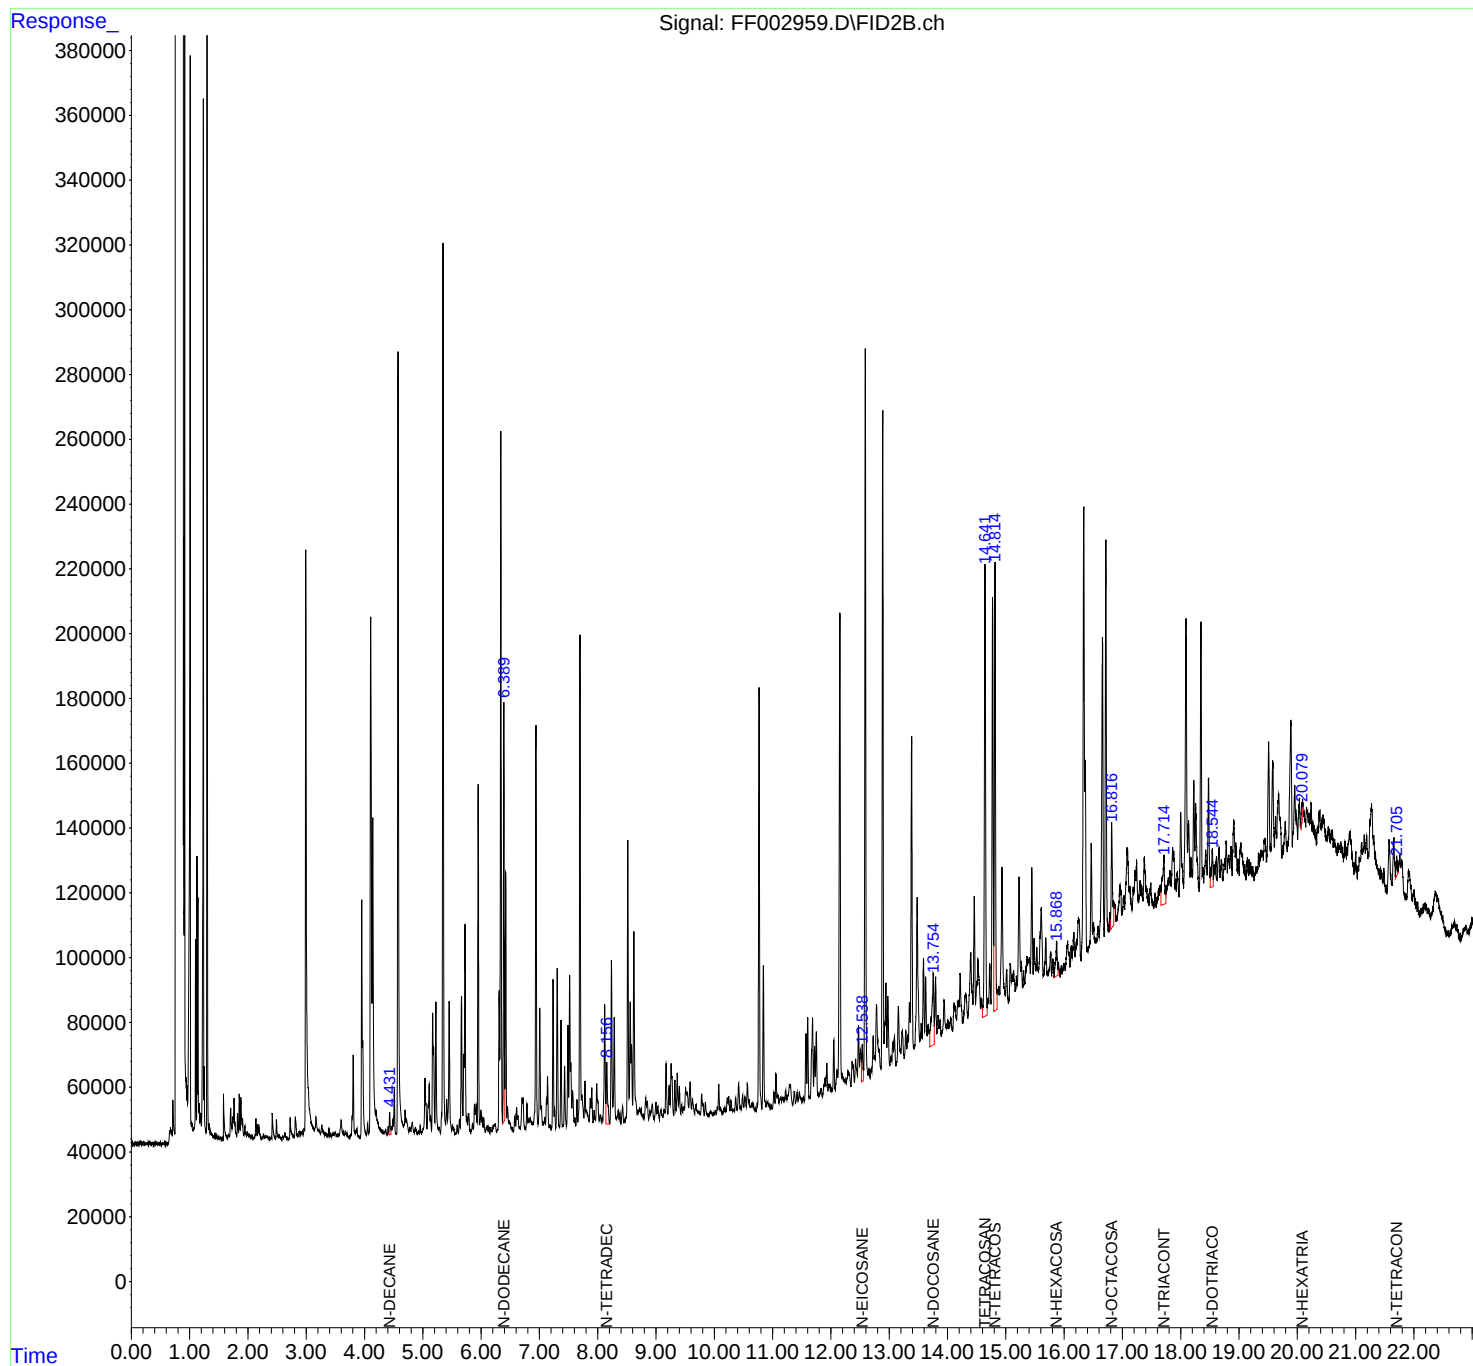


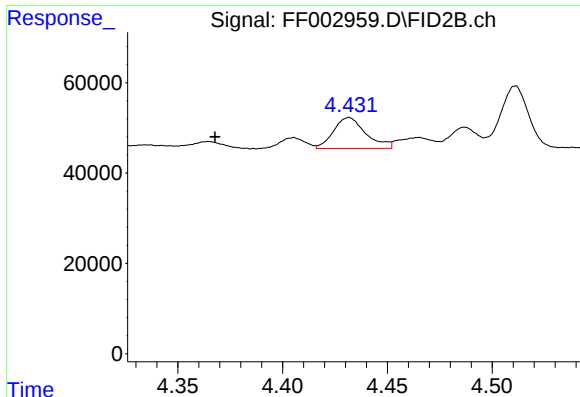

#2 N-DECANE


R.T.: 4.432 min
Delta R.T.: 0.064 min
Response: 73909
Conc: 0.47 ug/ml

Instrument :
FID_F
ClientSampleId :

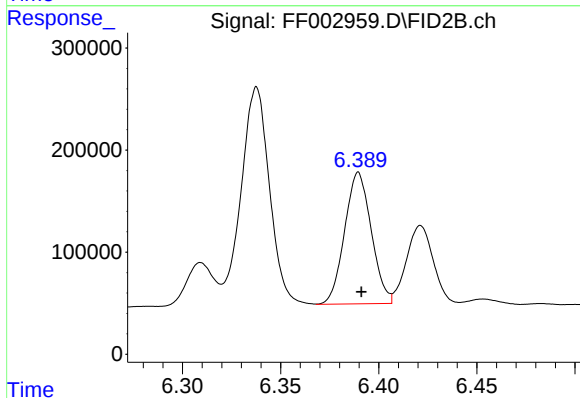


#3 N-DODECANE

R.T.: 6.390 min
Delta R.T.: -0.001 min
Response: 1217963
Conc: 7.67 ug/ml

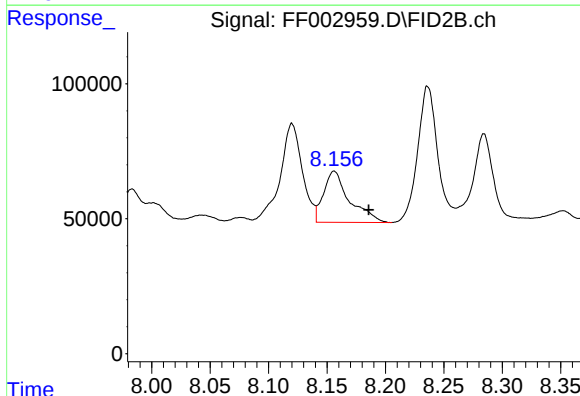


#4 N-TETRADECANE

R.T.: 8.156 min
Delta R.T.: -0.029 min
Response: 292982
Conc: 1.83 ug/ml

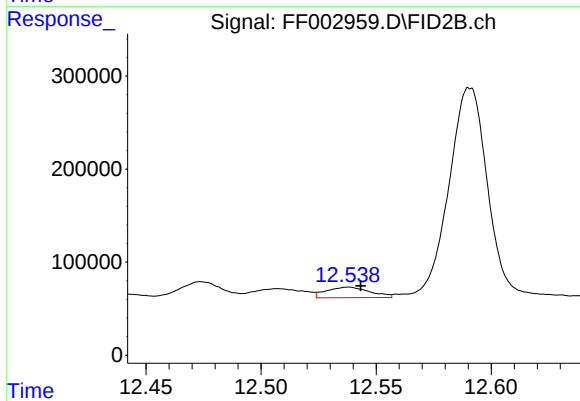

#7 N-EICOSANE


R.T.: 12.538 min
Delta R.T.: -0.005 min
Response: 149800
Conc: 0.97 ug/ml

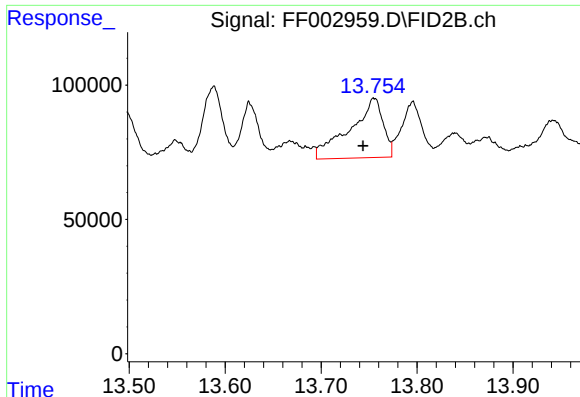

#8 N-DOCOSANE


R.T.: 13.755 min
Delta R.T.: 0.012 min
Response: 533389
Conc: 3.57 ug/ml

Instrument :
FID_F
ClientSampleId :

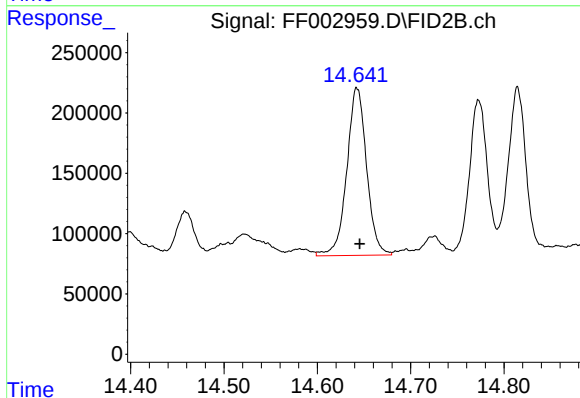


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.642 min
Delta R.T.: -0.003 min
Response: 2053911
Conc: 15.82 ug/ml

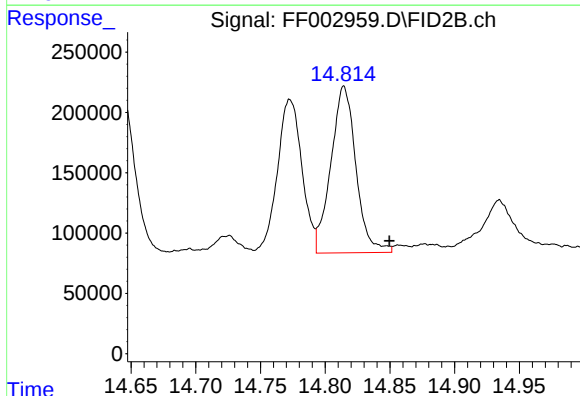


#10 N-TETRACOSANE

R.T.: 14.814 min
Delta R.T.: -0.035 min
Response: 1862888
Conc: 12.89 ug/ml

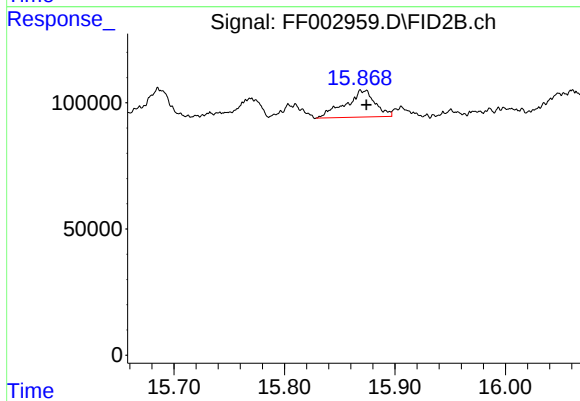

#11 N-HEXACOSANE


R.T.: 15.869 min
Delta R.T.: -0.005 min
Response: 199343
Conc: 1.43 ug/ml

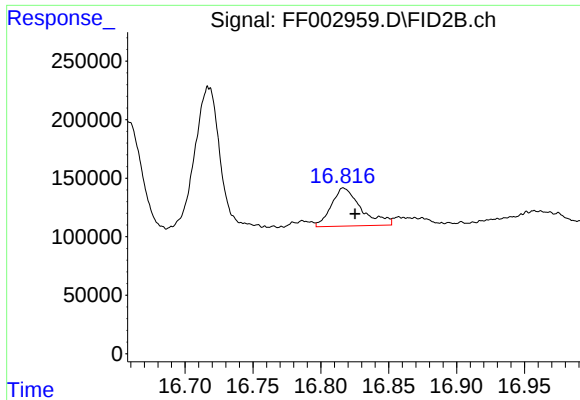

#12 N-OCTACOSANE


R.T.: 16.817 min
Delta R.T.: -0.008 min
Response: 495137
Conc: 3.70 ug/ml

Instrument :
FID_F
ClientSampleId :

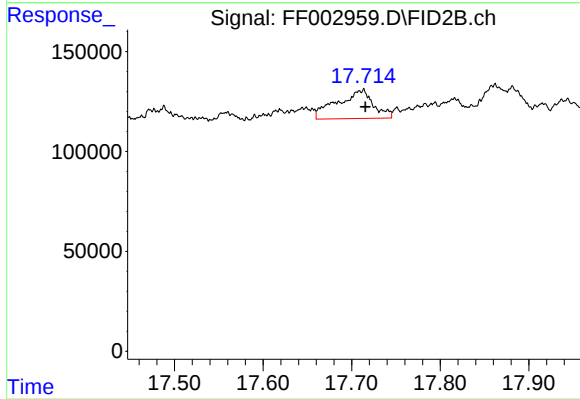


#13 N-TRIACONTANE

R.T.: 17.713 min
Delta R.T.: -0.002 min
Response: 407189
Conc: 3.18 ug/ml

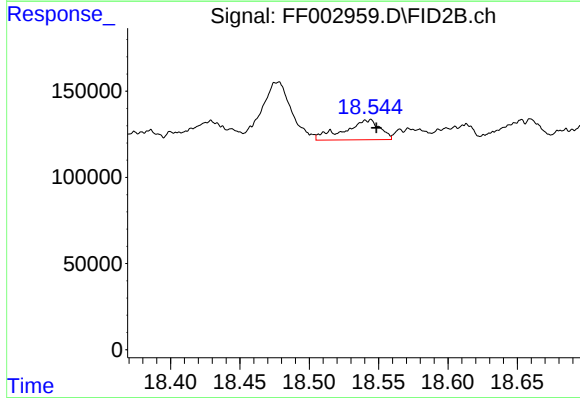


#14 N-DOTRIACONTANE

R.T.: 18.544 min
Delta R.T.: -0.005 min
Response: 206834
Conc: 1.73 ug/ml

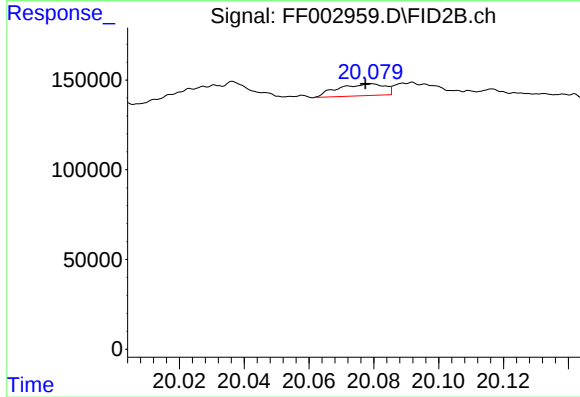

#16 N-HEXATRIACONTANE

R.T.: 20.079 min
Delta R.T.: 0.002 min
Response: 64657
Conc: 0.60 ug/ml

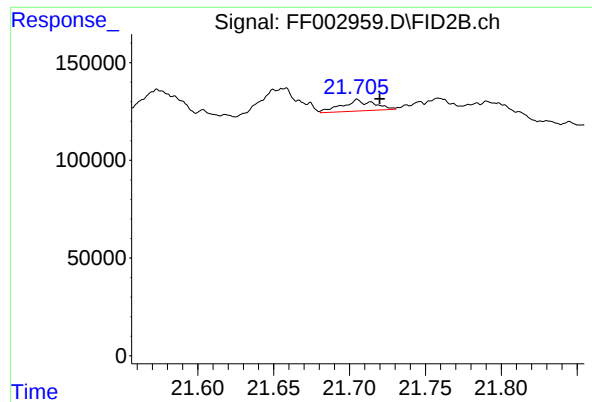

#18 N-TETRACONTANE

R.T.: 21.705 min
Delta R.T.: -0.015 min
Response: 84362
Conc: 0.80 ug/ml

Instrument :
FID_F
ClientSampleId :