

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121018\
 Data File : FF002960.D
 Signal(s) : FID2B.ch
 Acq On : 10 Dec 2018 16:35
 Operator : AJ\SJ
 Sample : J6316-05
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 11 00:57:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.642	1719433	13.244 ug/ml
Target Compounds			
3) N-DODECANE	6.390	251221	1.582 ug/ml
4) N-TETRADECANE	8.237f	872905	5.446 ug/ml
5) N-HEXADECANE	9.795	314126	1.962 ug/ml
7) N-EICOSANE	12.537	146579	0.950 ug/ml
8) N-DOCOSANE	13.753	456579	3.053 ug/ml
10) N-TETRACOSANE	14.815	1755123	12.145 ug/ml
11) N-HEXACOSANE	15.872	246815	1.768 ug/ml
12) N-OCTACOSANE	16.820	929351	6.936 ug/ml
13) N-TRIACONTANE	17.717	2704929	21.110 ug/ml
14) N-DOTRIACONTANE	18.546	1132090	9.480 ug/ml
15) N-TETRATRIACONTANE	19.372	450090	3.971 ug/ml
18) N-TETRACONTANE	21.726	103975	0.989 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121018\
Data File : FF002960.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2018 16:35
Operator : AJ\SJ
Sample : J6316-05
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 11 00:57:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

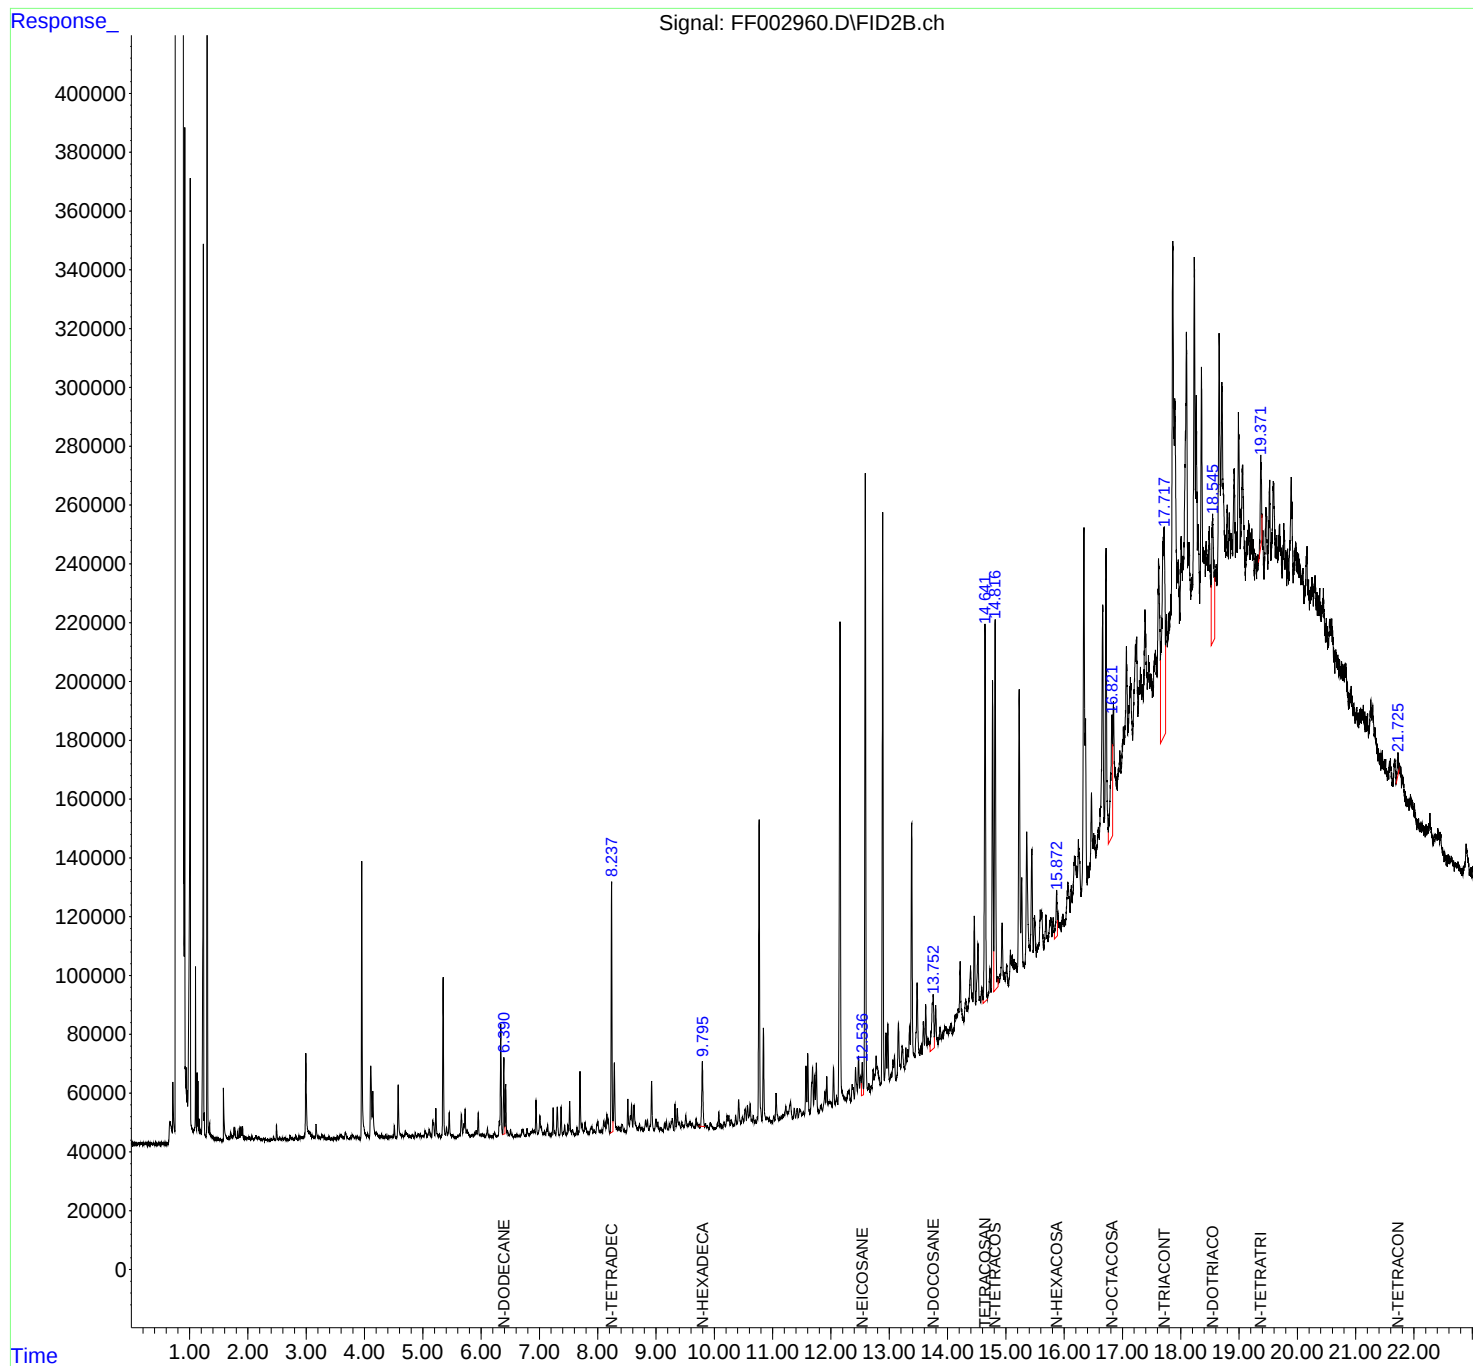


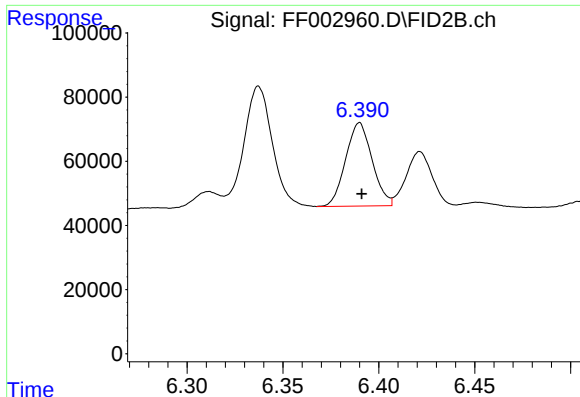

#3 N-DODECANE


R.T.: 6.390 min
Delta R.T.: -0.001 min
Response: 251221
Conc: 1.58 ug/ml

Instrument :
FID_F
ClientSampleId :

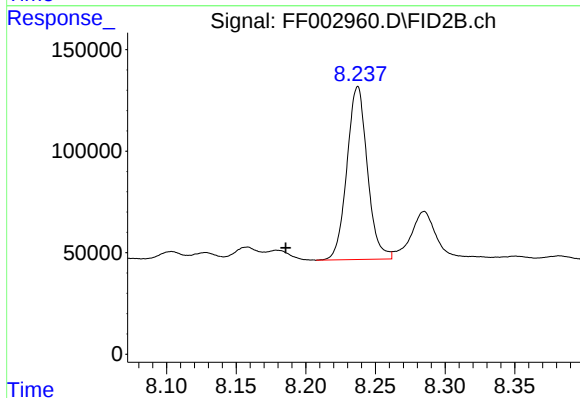


#4 N-TETRADECANE

R.T.: 8.237 min
Delta R.T.: 0.052 min
Response: 872905
Conc: 5.45 ug/ml

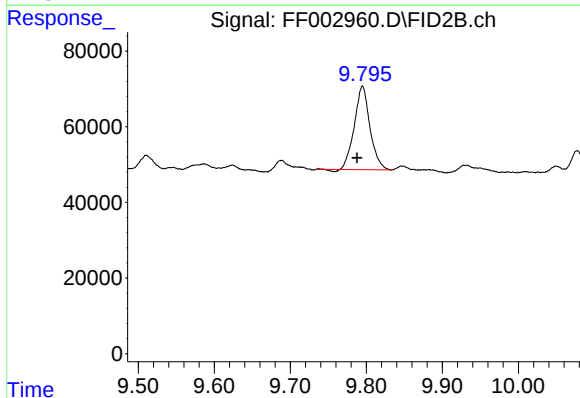


#5 N-HEXADECANE

R.T.: 9.795 min
Delta R.T.: 0.007 min
Response: 314126
Conc: 1.96 ug/ml

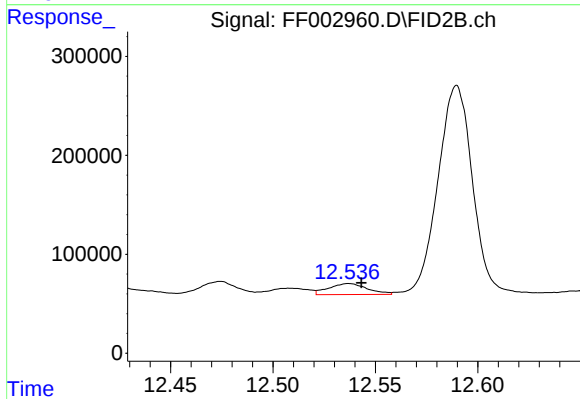

#7 N-EICOSANE


R.T.: 12.537 min
Delta R.T.: -0.006 min
Response: 146579
Conc: 0.95 ug/ml

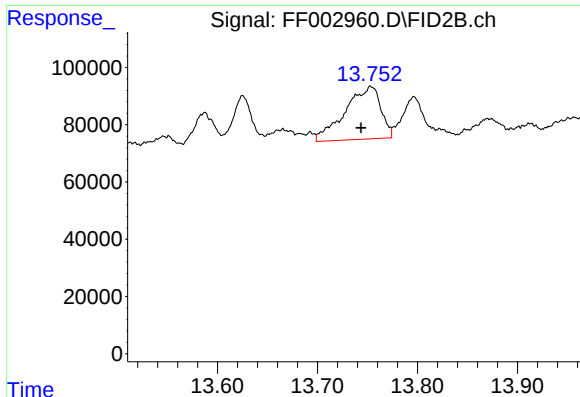

#8 N-DOCOSANE


R.T.: 13.753 min
Delta R.T.: 0.010 min
Response: 456579
Conc: 3.05 ug/ml

Instrument :
FID_F
ClientSampleId :

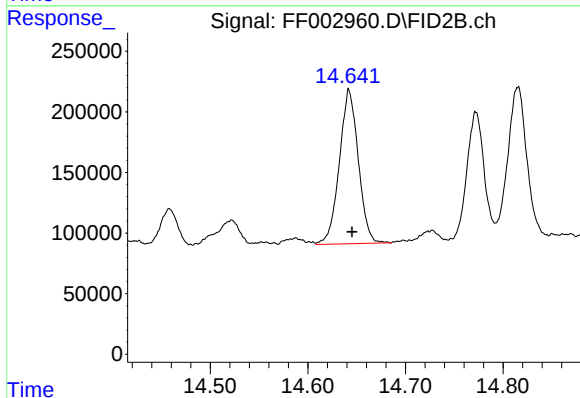


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.642 min
Delta R.T.: -0.003 min
Response: 1719433
Conc: 13.24 ug/ml

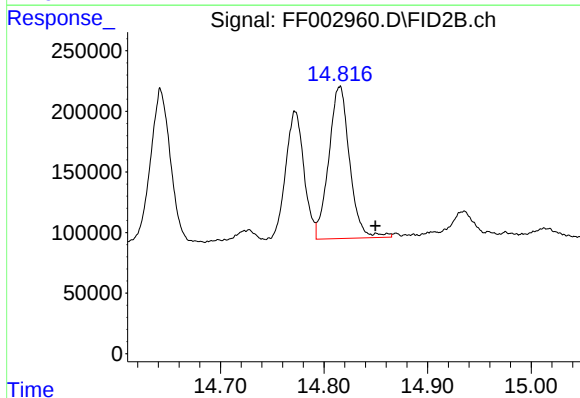


#10 N-TETRACOSANE

R.T.: 14.815 min
Delta R.T.: -0.034 min
Response: 1755123
Conc: 12.14 ug/ml

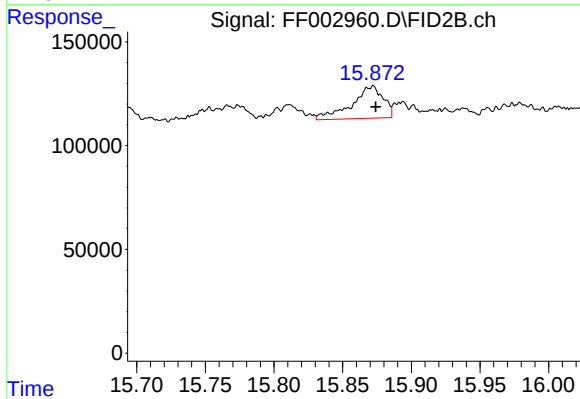

#11 N-HEXACOSANE


R.T.: 15.872 min
Delta R.T.: -0.002 min
Response: 246815
Conc: 1.77 ug/ml

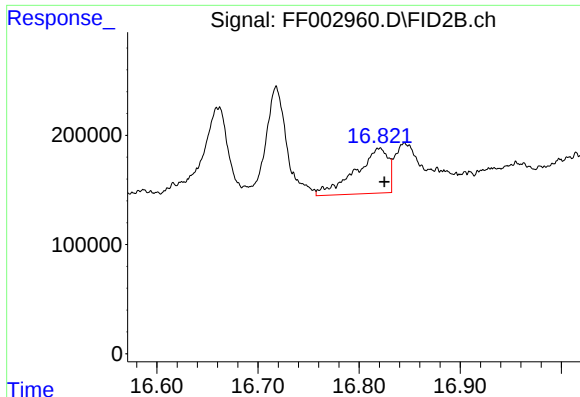

#12 N-OCTACOSANE


R.T.: 16.820 min
Delta R.T.: -0.005 min
Response: 929351
Conc: 6.94 ug/ml

Instrument :
FID_F
ClientSampleId :

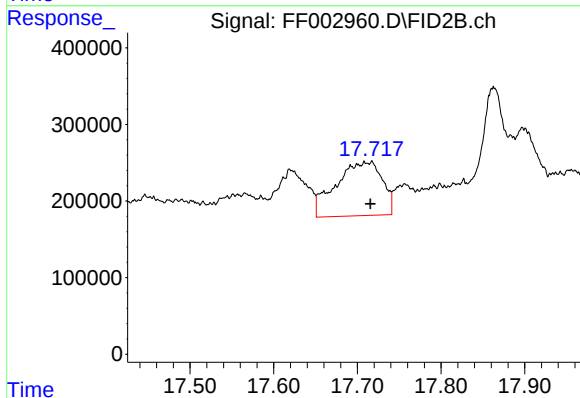


#13 N-TRIACONTANE

R.T.: 17.717 min
Delta R.T.: 0.002 min
Response: 2704929
Conc: 21.11 ug/ml

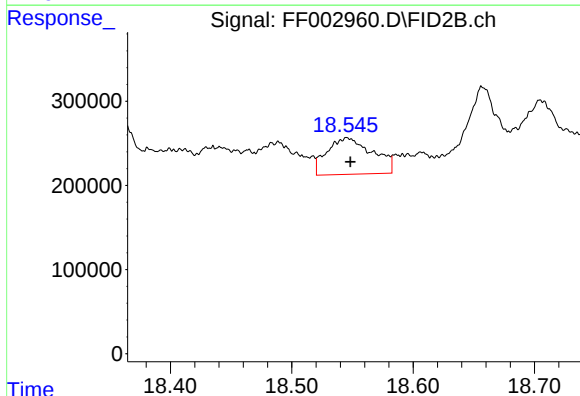


#14 N-DOTRIACONTANE

R.T.: 18.546 min
Delta R.T.: -0.003 min
Response: 1132090
Conc: 9.48 ug/ml

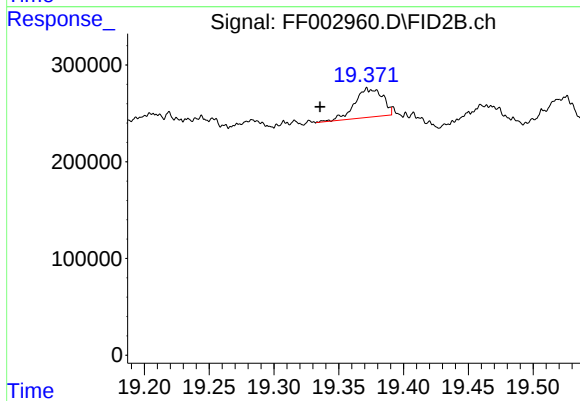

#15 N-TETRATRIACONTANE

R.T.: 19.372 min
Delta R.T.: 0.037 min
Response: 450090
Conc: 3.97 ug/ml

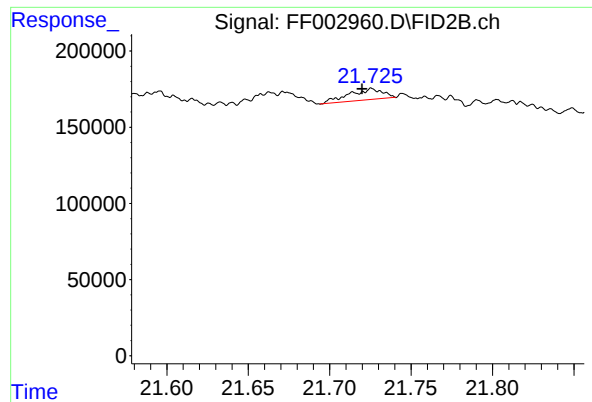

#18 N-TETRACONTANE

R.T.: 21.726 min
Delta R.T.: 0.006 min
Response: 103975
Conc: 0.99 ug/ml

Instrument :
FID_F
ClientSampleId :