

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121018\
 Data File : FF002962.D
 Signal(s) : FID2B.ch
 Acq On : 10 Dec 2018 17:36
 Operator : AJ\SJ
 Sample : J6316-13
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 11 00:58:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.650	4709935	36.279 ug/ml
Target Compounds			
3) N-DODECANE	6.372	681592	4.292 ug/ml
4) N-TETRADECANE	8.218	207459	1.294 ug/ml
5) N-HEXADECANE	9.792	4354768	27.193 ug/ml
6) N-OCTADECANE	11.201	404251	2.552 ug/ml
7) N-EICOSANE	12.554	1210867	7.851 ug/ml
8) N-DOCOSANE	13.769	5248996	35.103 ug/ml
10) N-TETRACOSANE	14.850	16531707	114.394 ug/ml
11) N-HEXACOSANE	15.890	848322	6.078 ug/ml
12) N-OCTACOSANE	16.843	3465940	25.868 ug/ml
13) N-TRIACONTANE	17.727	1063782	8.302 ug/ml
14) N-DOTRIACONTANE	18.549	568229	4.758 ug/ml
15) N-TETRATRIACONTANE	19.338	28621	0.253 ug/ml
16) N-HEXATRIACONTANE	20.064	427297	3.960 ug/ml
18) N-TETRACONTANE	21.693	716024	6.812 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121018\
Data File : FF002962.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2018 17:36
Operator : AJ\SJ
Sample : J6316-13
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 11 00:58:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

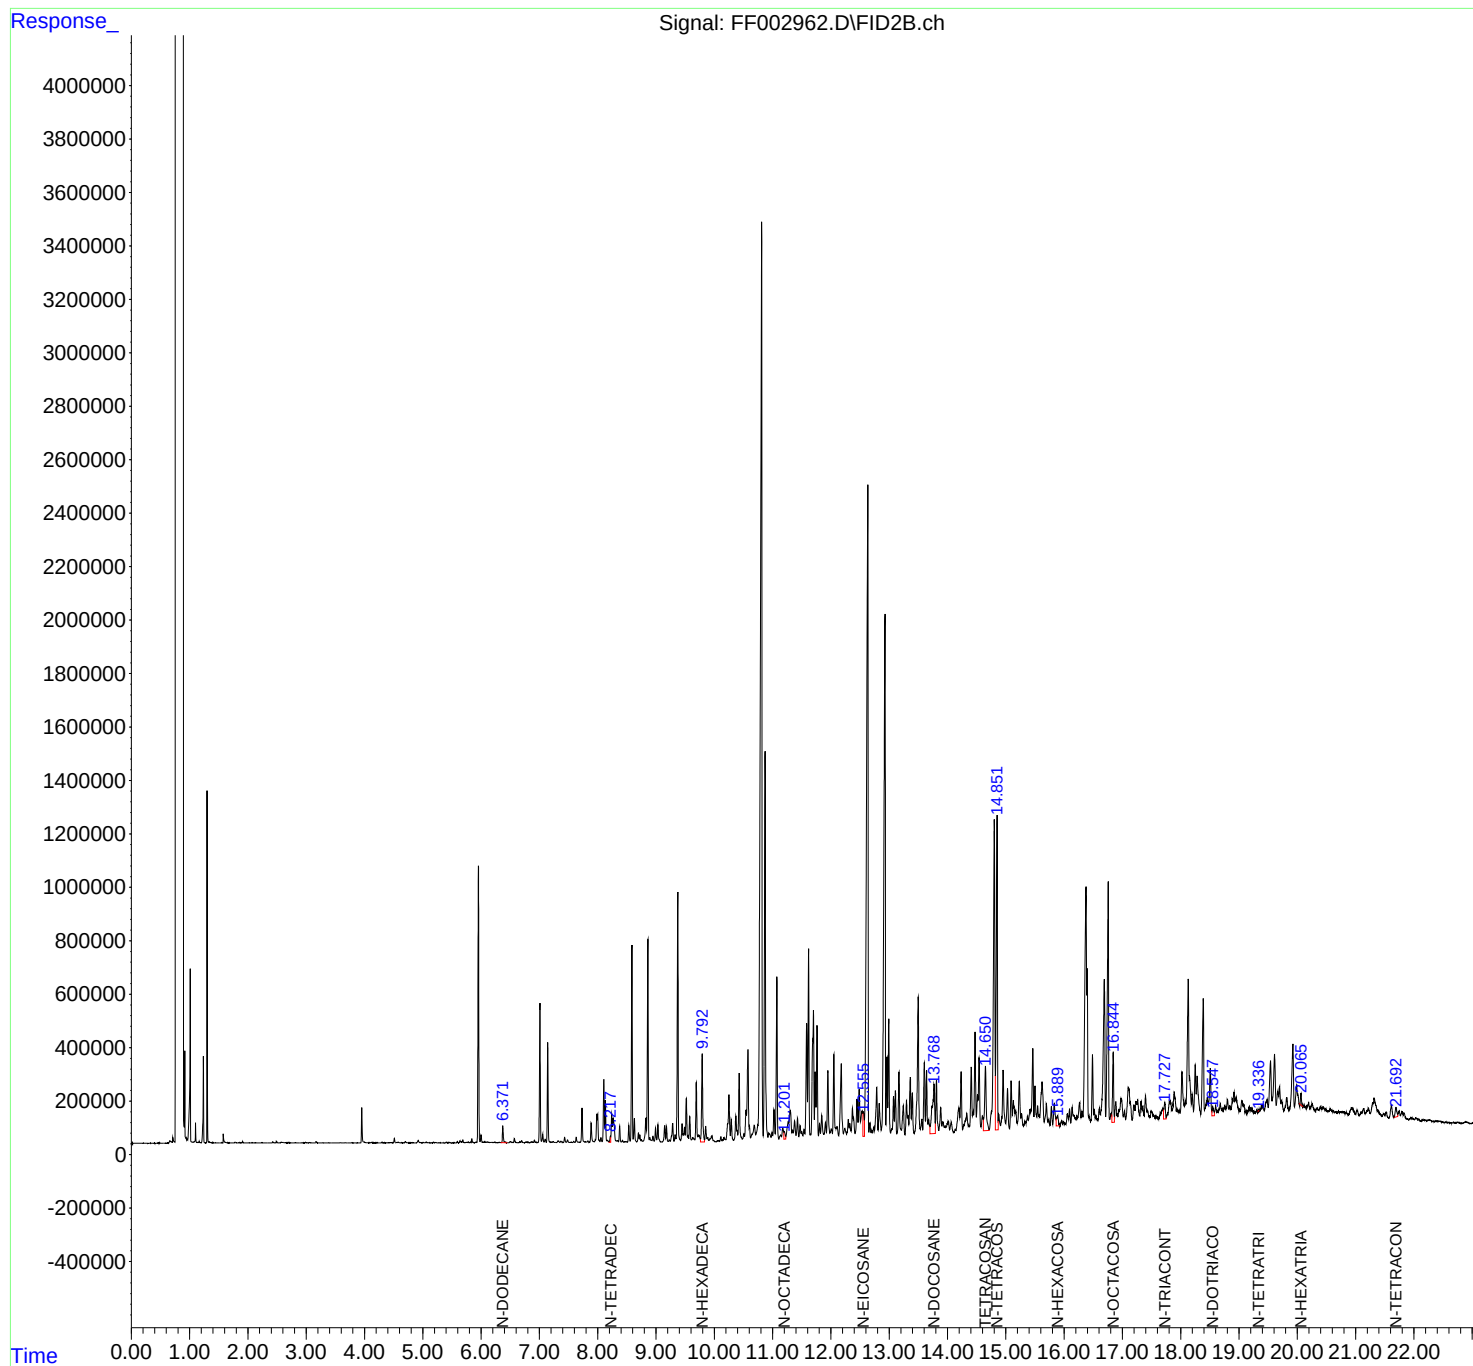


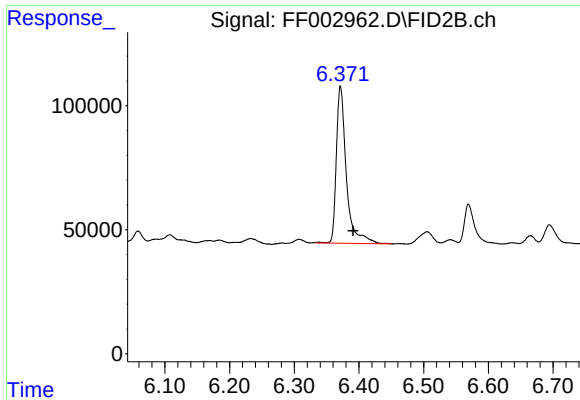

#3 N-DODECANE


R.T.: 6.372 min
Delta R.T.: -0.019 min
Response: 681592
Conc: 4.29 ug/ml

Instrument :
FID_F
ClientSampleId :

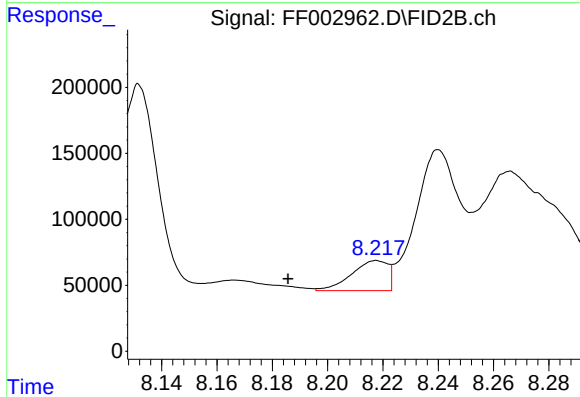


#4 N-TETRADECANE

R.T.: 8.218 min
Delta R.T.: 0.032 min
Response: 207459
Conc: 1.29 ug/ml

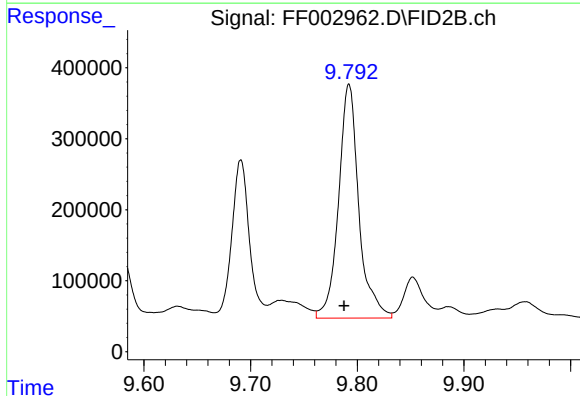


#5 N-HEXADECANE

R.T.: 9.792 min
Delta R.T.: 0.005 min
Response: 4354768
Conc: 27.19 ug/ml

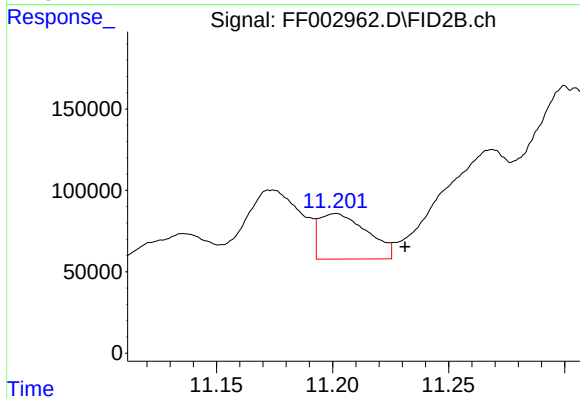

#6 N-OCTADECANE


R.T.: 11.201 min
Delta R.T.: -0.030 min
Response: 404251
Conc: 2.55 ug/ml

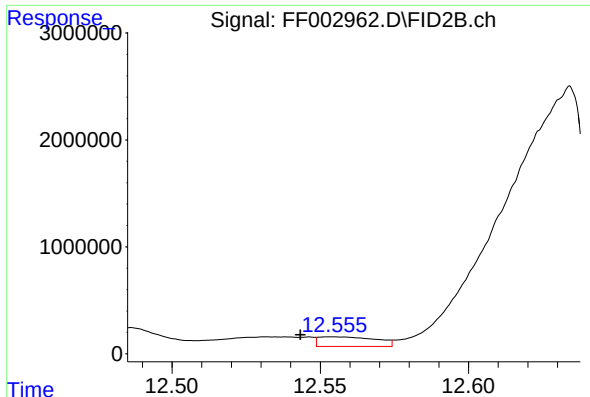

#7 N-EICOSANE


R.T.: 12.554 min
Delta R.T.: 0.011 min
Response: 1210867
Conc: 7.85 ug/ml

Instrument :
FID_F
ClientSampleId :

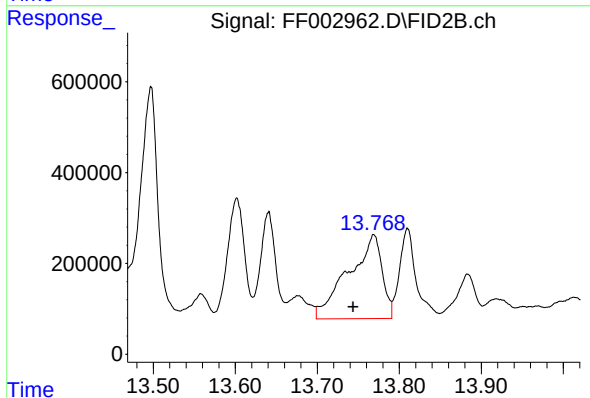


#8 N-DOCOSANE

R.T.: 13.769 min
Delta R.T.: 0.025 min
Response: 5248996
Conc: 35.10 ug/ml

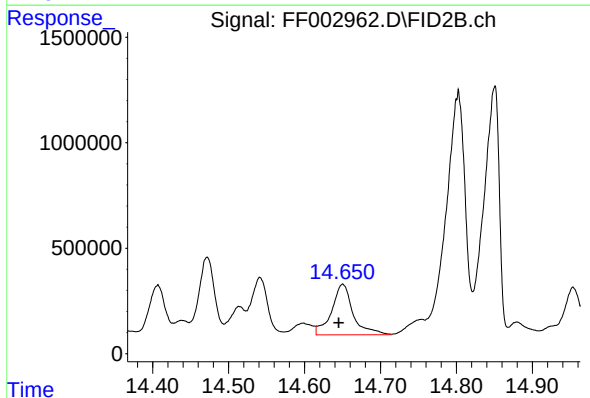


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.650 min
Delta R.T.: 0.005 min
Response: 4709935
Conc: 36.28 ug/ml

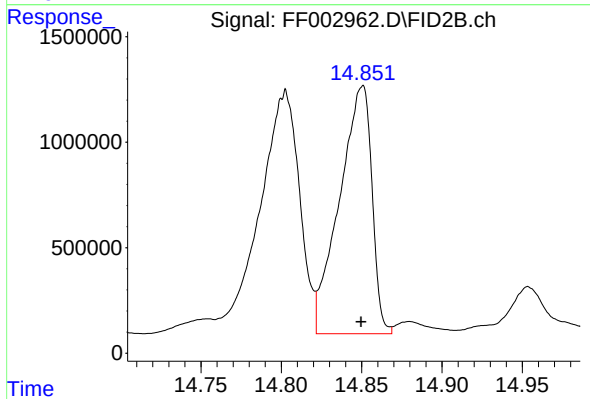

#10 N-TETRACOSANE


R.T.: 14.850 min
Delta R.T.: 0.000 min
Response: 16531707
Conc: 114.39 ug/ml

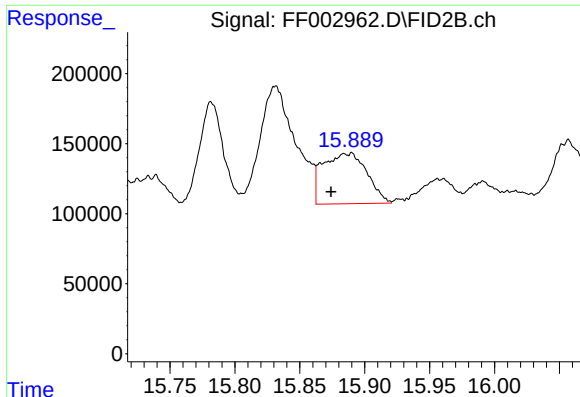

#11 N-HEXACOSANE


R.T.: 15.890 min
Delta R.T.: 0.016 min
Response: 848322
Conc: 6.08 ug/ml

Instrument :
FID_F
ClientSampleId :

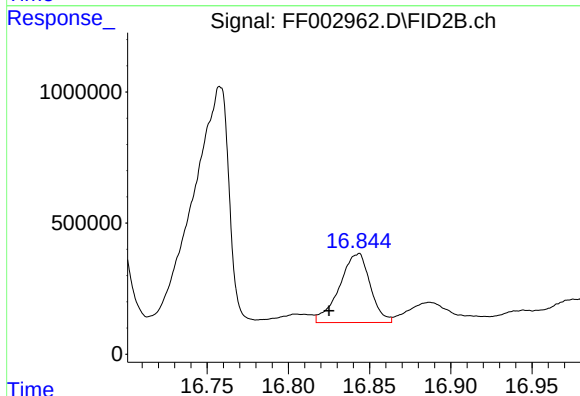


#12 N-OCTACOSANE

R.T.: 16.843 min
Delta R.T.: 0.018 min
Response: 3465940
Conc: 25.87 ug/ml

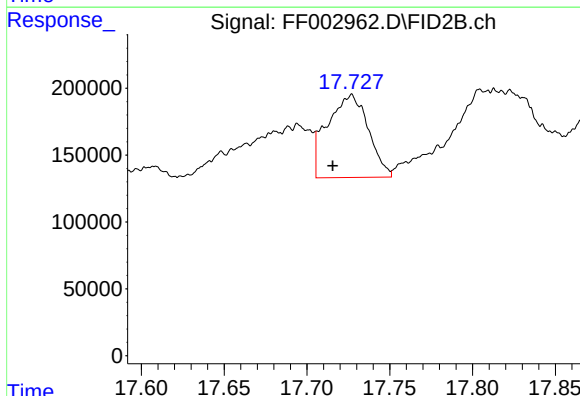


#13 N-TRIACONTANE

R.T.: 17.727 min
Delta R.T.: 0.011 min
Response: 1063782
Conc: 8.30 ug/ml

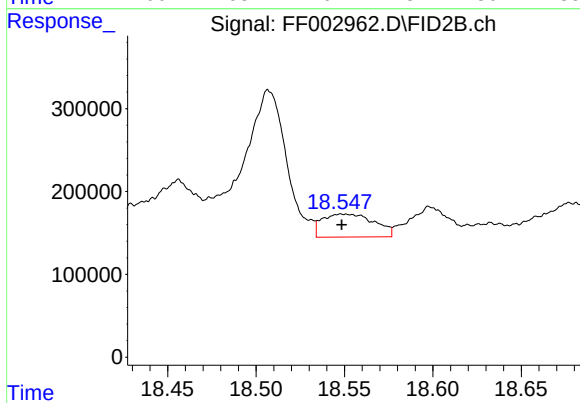

#14 N-DOTRIACONTANE

R.T.: 18.549 min
Delta R.T.: 0.000 min
Response: 568229
Conc: 4.76 ug/ml

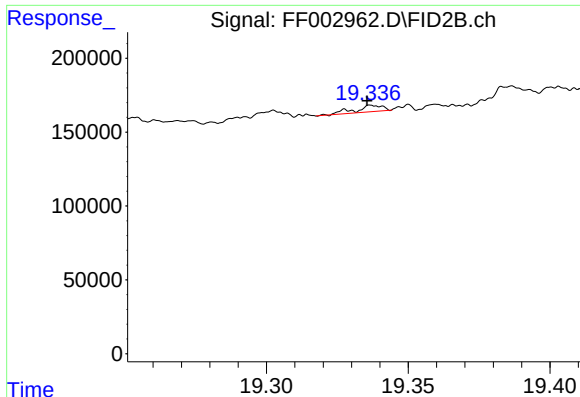

#15 N-TETRATRIACONTANE


R.T.: 19.338 min

Delta R.T.: 0.002 min

Response: 28621

Conc: 0.25 ug/ml

Instrument :
FID_F
ClientSampleId :

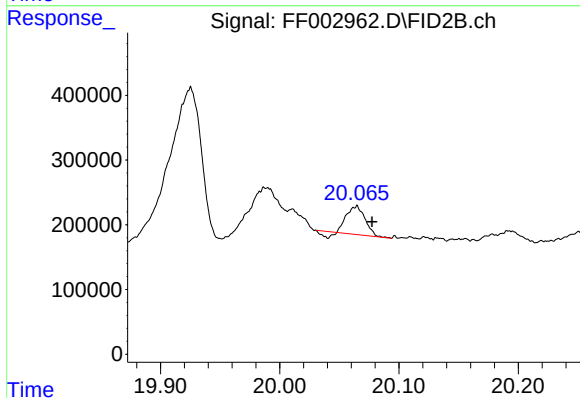


#16 N-HEXATRIACONTANE

R.T.: 20.064 min

Delta R.T.: -0.013 min

Response: 427297

Conc: 3.96 ug/ml

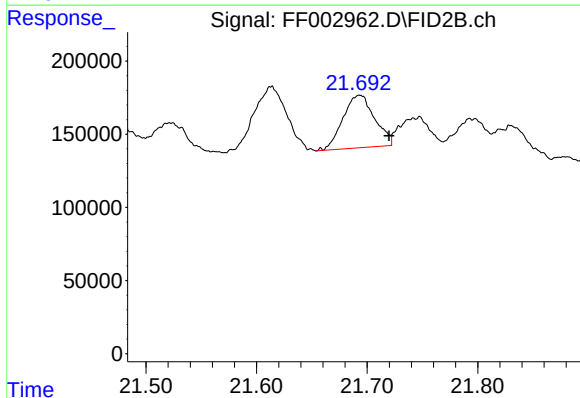

#18 N-TETRACONTANE

R.T.: 21.693 min

Delta R.T.: -0.027 min

Response: 716024

Conc: 6.81 ug/ml