

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121018\
Data File : FF002963.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2018 18:07
Operator : AJ\SJ
Sample : J6316-17
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 11 00:58:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.643	1348076	10.384 ug/ml
Target Compounds			
4) N-TETRADECANE	8.238f	411653	2.568 ug/ml
7) N-EICOSANE	12.590	617283	4.002 ug/ml
10) N-TETRACOSANE	14.813	513433	3.553 ug/ml
12) N-OCTACOSANE	16.818	184434	1.377 ug/ml
13) N-TRIACONTANE	17.711	174988	1.366 ug/ml
14) N-DOTRIACONTANE	18.540	323781	2.711 ug/ml
18) N-TETRACONTANE	21.710	82970	0.789 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121018\
Data File : FF002963.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2018 18:07
Operator : AJ\SJ
Sample : J6316-17
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 11 00:58:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

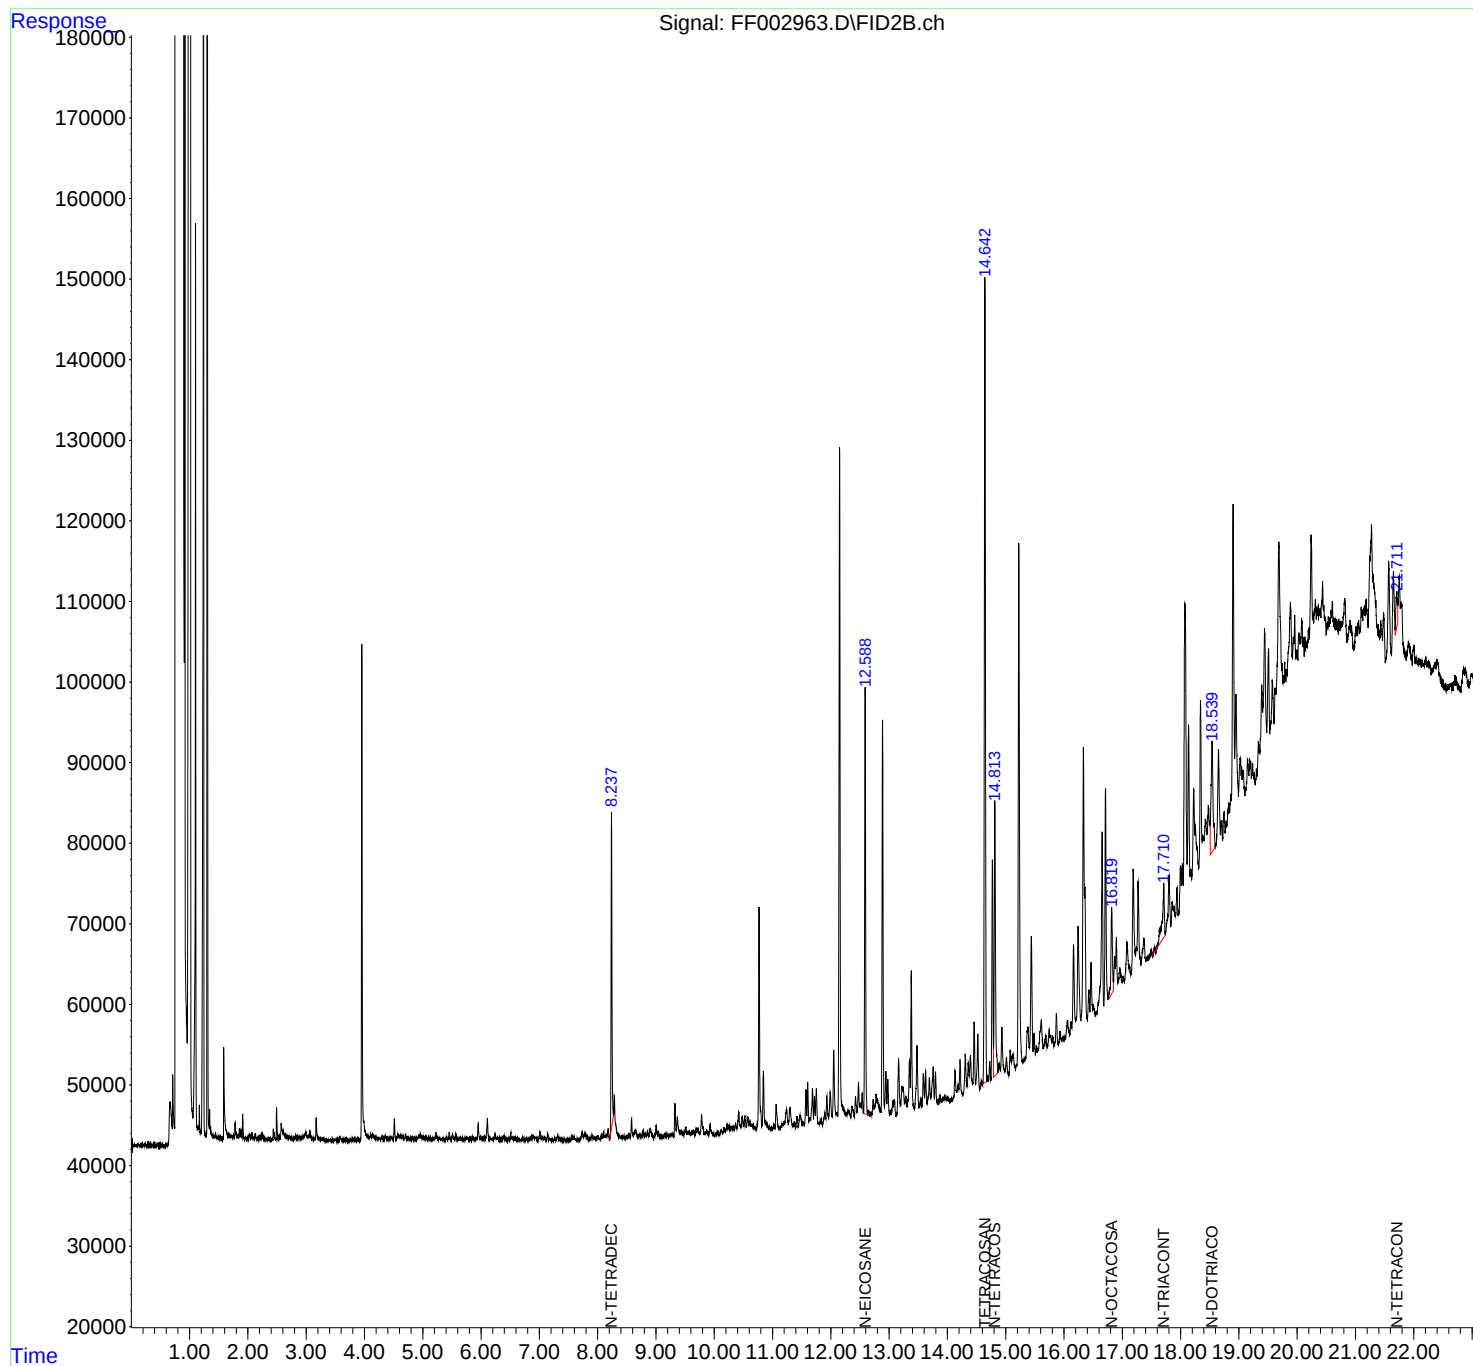


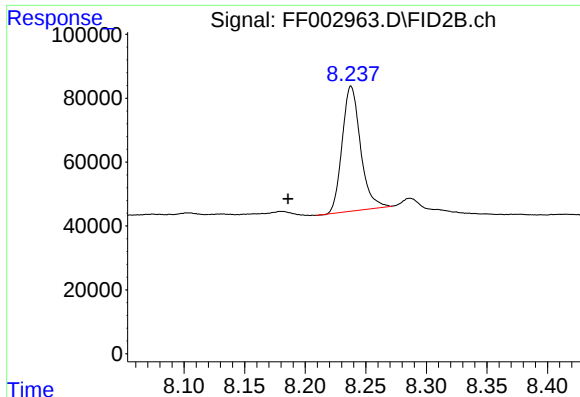

#4 N-TETRADECANE


R.T.: 8.238 min
Delta R.T.: 0.052 min
Response: 411653
Conc: 2.57 ug/ml

Instrument :
FID_F
ClientSampleId :

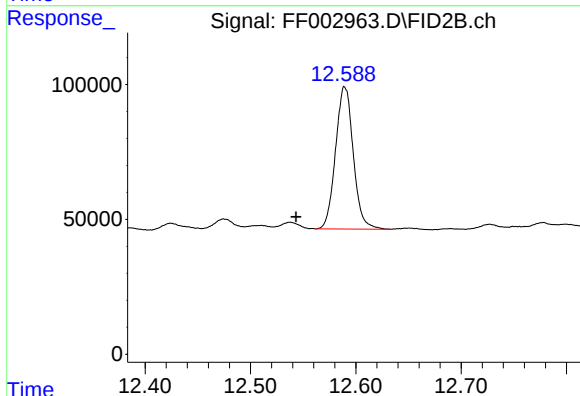


#7 N-EICOSANE

R.T.: 12.590 min
Delta R.T.: 0.046 min
Response: 617283
Conc: 4.00 ug/ml

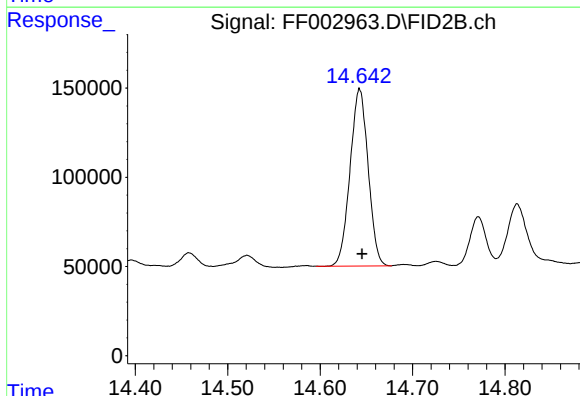


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.643 min
Delta R.T.: -0.003 min
Response: 1348076
Conc: 10.38 ug/ml

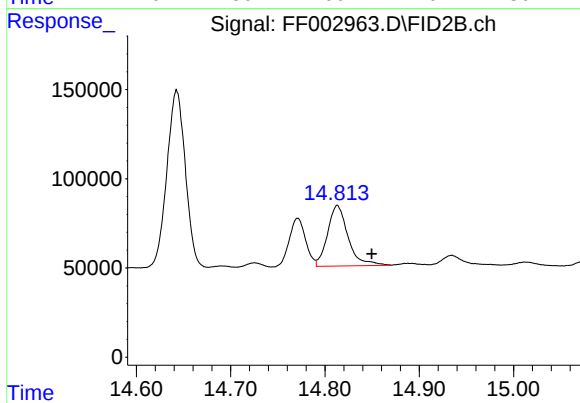

#10 N-TETRACOSANE


R.T.: 14.813 min
Delta R.T.: -0.036 min
Response: 513433
Conc: 3.55 ug/ml

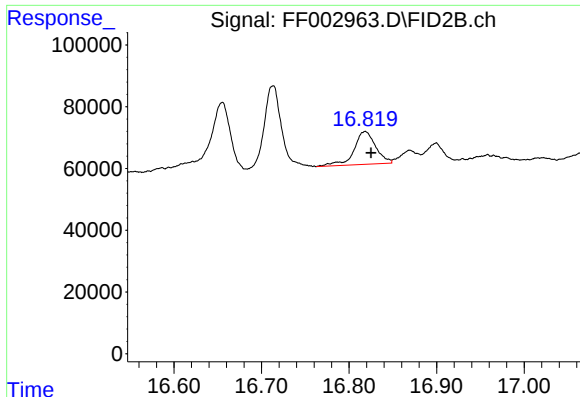

#12 N-OCTACOSANE


R.T.: 16.818 min
Delta R.T.: -0.007 min
Response: 184434
Conc: 1.38 ug/ml

Instrument :
FID_F
ClientSampleId :

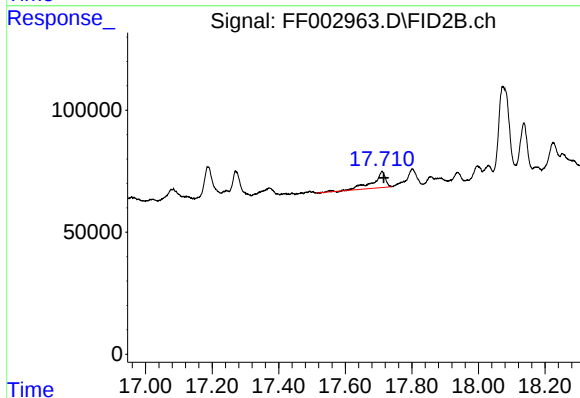


#13 N-TRIACONTANE

R.T.: 17.711 min
Delta R.T.: -0.005 min
Response: 174988
Conc: 1.37 ug/ml

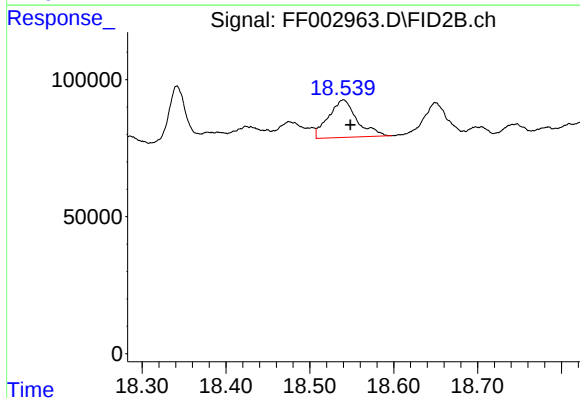

#14 N-DOTRIACONTANE

R.T.: 18.540 min
Delta R.T.: -0.008 min
Response: 323781
Conc: 2.71 ug/ml

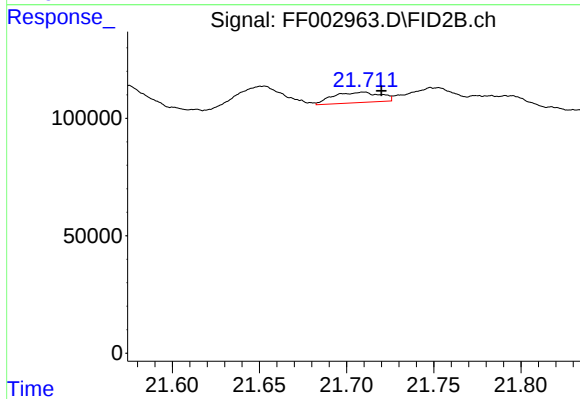

#18 N-TETRACONTANE

R.T.: 21.710 min
Delta R.T.: -0.010 min
Response: 82970
Conc: 0.79 ug/ml