

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121018\
 Data File : FF002966.D
 Signal(s) : FID2B.ch
 Acq On : 10 Dec 2018 19:39
 Operator : AJ\SJ
 Sample : J6316-05 2X
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 11 00:59:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.643	830369	6.396 ug/ml
Target Compounds			
3) N-DODECANE	6.391	119841	0.755 ug/ml
4) N-TETRADECANE	8.238f	391296	2.441 ug/ml
5) N-HEXADECANE	9.797	142402	0.889 ug/ml
7) N-EICOSANE	12.589	1170161	7.587 ug/ml
8) N-DOCOSANE	13.755	166892	1.116 ug/ml
10) N-TETRACOSANE	14.815	924918	6.400 ug/ml
11) N-HEXACOSANE	15.871	129292	0.926 ug/ml
12) N-OCTACOSANE	16.819	305398	2.279 ug/ml
13) N-TRIACONTANE	17.713	449443	3.508 ug/ml
14) N-DOTRIACONTANE	18.542	274664	2.300 ug/ml
15) N-TETRATRIACONTANE	19.368	143674	1.268 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121018\
Data File : FF002966.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2018 19:39
Operator : AJ\SJ
Sample : J6316-05 2X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 11 00:59:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

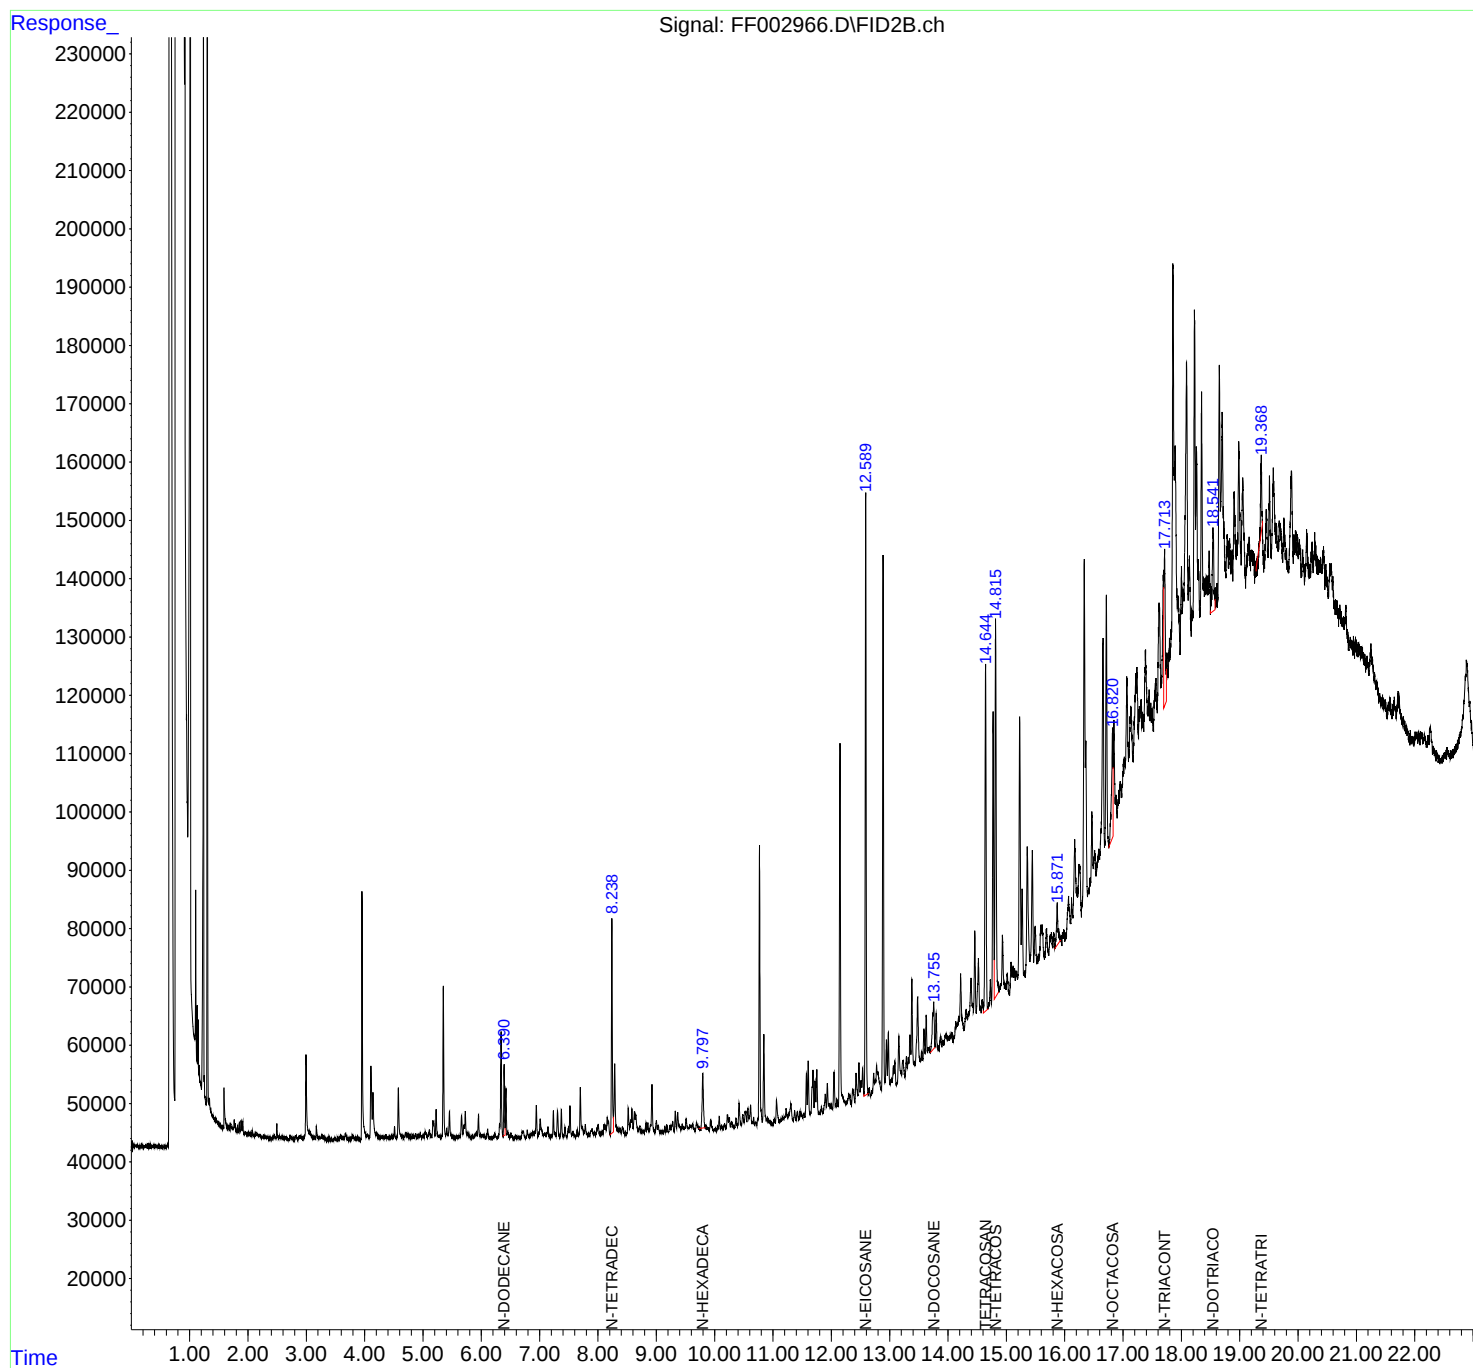


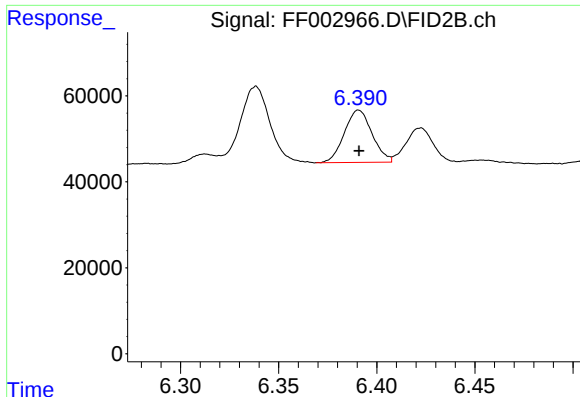

#3 N-DODECANE


R.T.: 6.391 min
Delta R.T.: 0.000 min
Response: 119841
Conc: 0.75 ug/ml

Instrument :
FID_F
ClientSampleId :

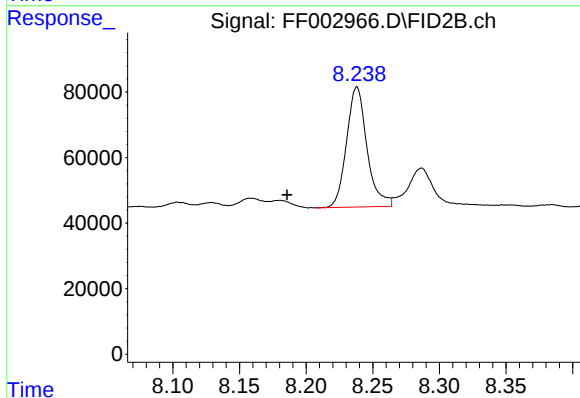


#4 N-TETRADECANE

R.T.: 8.238 min
Delta R.T.: 0.052 min
Response: 391296
Conc: 2.44 ug/ml

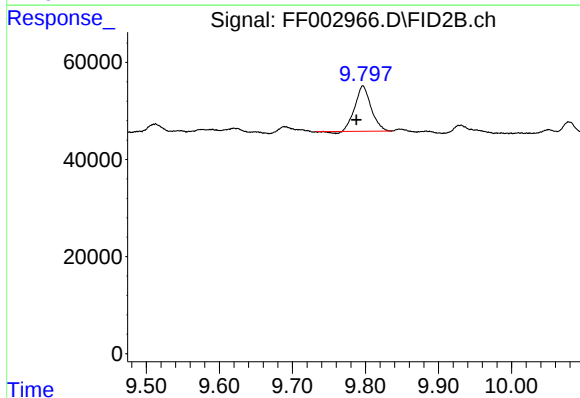


#5 N-HEXADECANE

R.T.: 9.797 min
Delta R.T.: 0.009 min
Response: 142402
Conc: 0.89 ug/ml

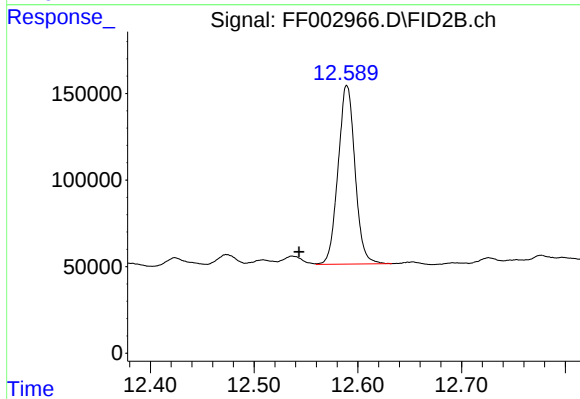

#7 N-EICOSANE


R.T.: 12.589 min
Delta R.T.: 0.046 min
Response: 1170161
Conc: 7.59 ug/ml

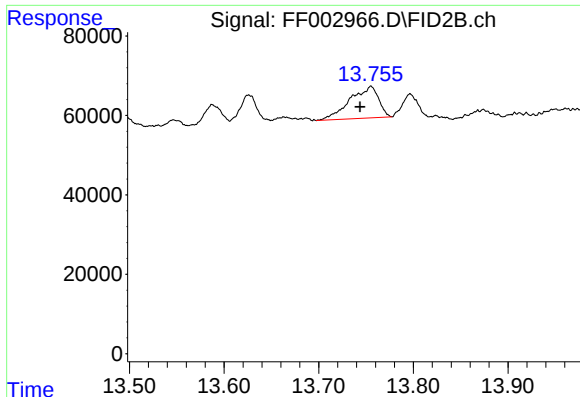

#8 N-DOCOSANE


R.T.: 13.755 min
Delta R.T.: 0.012 min
Response: 166892
Conc: 1.12 ug/ml

Instrument :
FID_F
ClientSampleId :

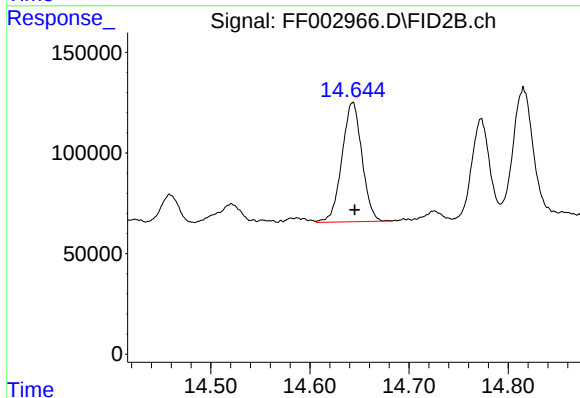


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.643 min
Delta R.T.: -0.002 min
Response: 830369
Conc: 6.40 ug/ml

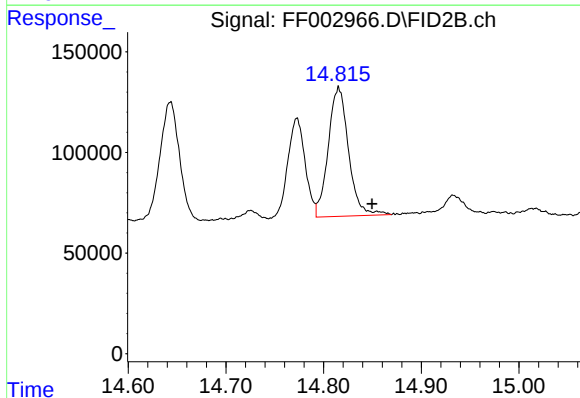


#10 N-TETRACOSANE

R.T.: 14.815 min
Delta R.T.: -0.034 min
Response: 924918
Conc: 6.40 ug/ml

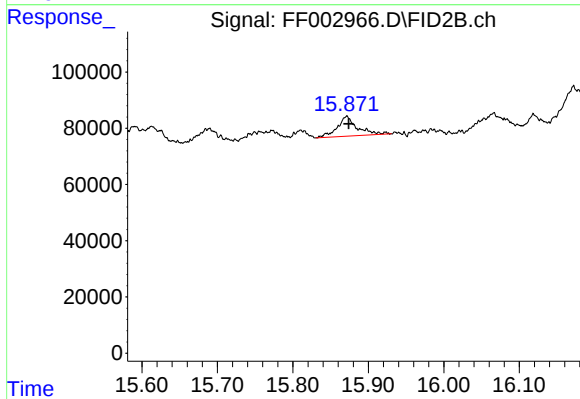

#11 N-HEXACOSANE


R.T.: 15.871 min
Delta R.T.: -0.003 min
Response: 129292
Conc: 0.93 ug/ml

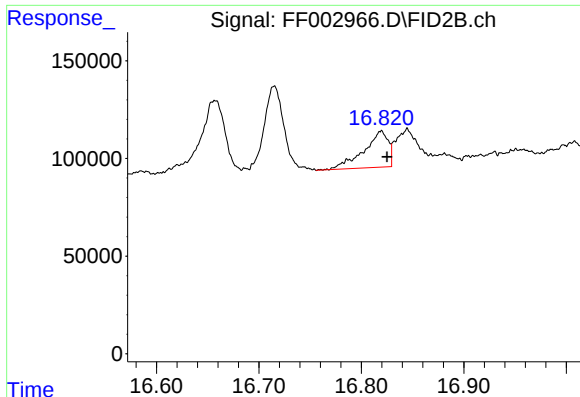

#12 N-OCTACOSANE


R.T.: 16.819 min
Delta R.T.: -0.006 min
Response: 305398
Conc: 2.28 ug/ml

Instrument :
FID_F
ClientSampleId :

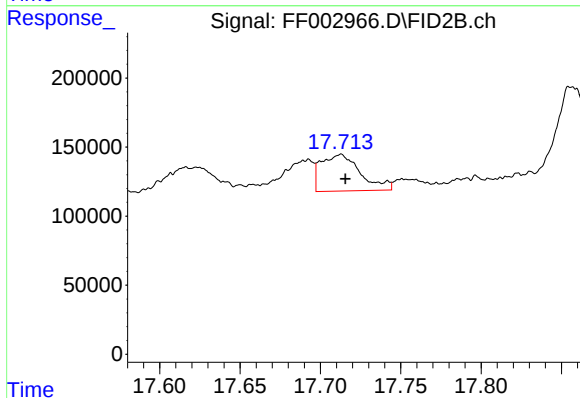


#13 N-TRIACONTANE

R.T.: 17.713 min
Delta R.T.: -0.003 min
Response: 449443
Conc: 3.51 ug/ml

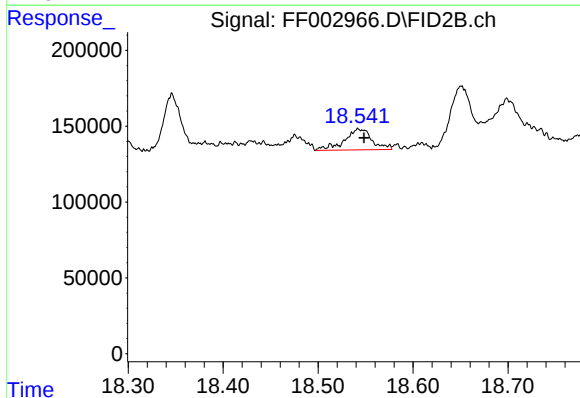

#14 N-DOTRIACONTANE

R.T.: 18.542 min
Delta R.T.: -0.006 min
Response: 274664
Conc: 2.30 ug/ml

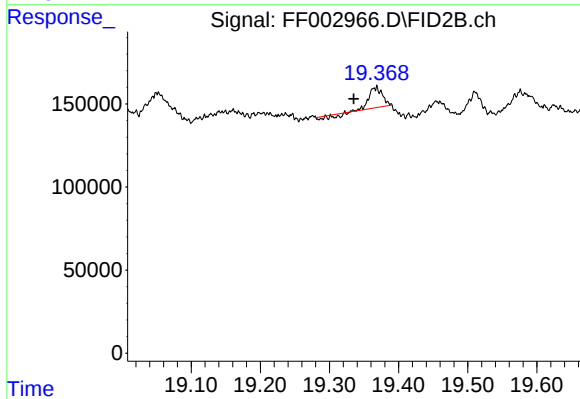

#15 N-TETRATRIACONTANE

R.T.: 19.368 min
Delta R.T.: 0.033 min
Response: 143674
Conc: 1.27 ug/ml