

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121018\
 Data File : FF002967.D
 Signal(s) : FID2B.ch
 Acq On : 10 Dec 2018 20:09
 Operator : AJ\SJ
 Sample : J6316-09 2X
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 11 00:59:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.642	734259	5.656 ug/ml
Target Compounds			
4) N-TETRADECANE	8.238f	220234	1.374 ug/ml
7) N-EICOSANE	12.538	157857	1.024 ug/ml
8) N-DOCOSANE	13.757	444706	2.974 ug/ml
10) N-TETRACOSANE	14.815	1702408	11.780 ug/ml
11) N-HEXACOSANE	15.873	140525	1.007 ug/ml
12) N-OCTACOSANE	16.817	467486	3.489 ug/ml
13) N-TRIACONTANE	17.710	149051	1.163 ug/ml
14) N-DOTRIACONTANE	18.544	135832	1.137 ug/ml
18) N-TETRACONTANE	21.751	268148	2.551 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121018\
Data File : FF002967.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2018 20:09
Operator : AJ\SJ
Sample : J6316-09 2X
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 11 00:59:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

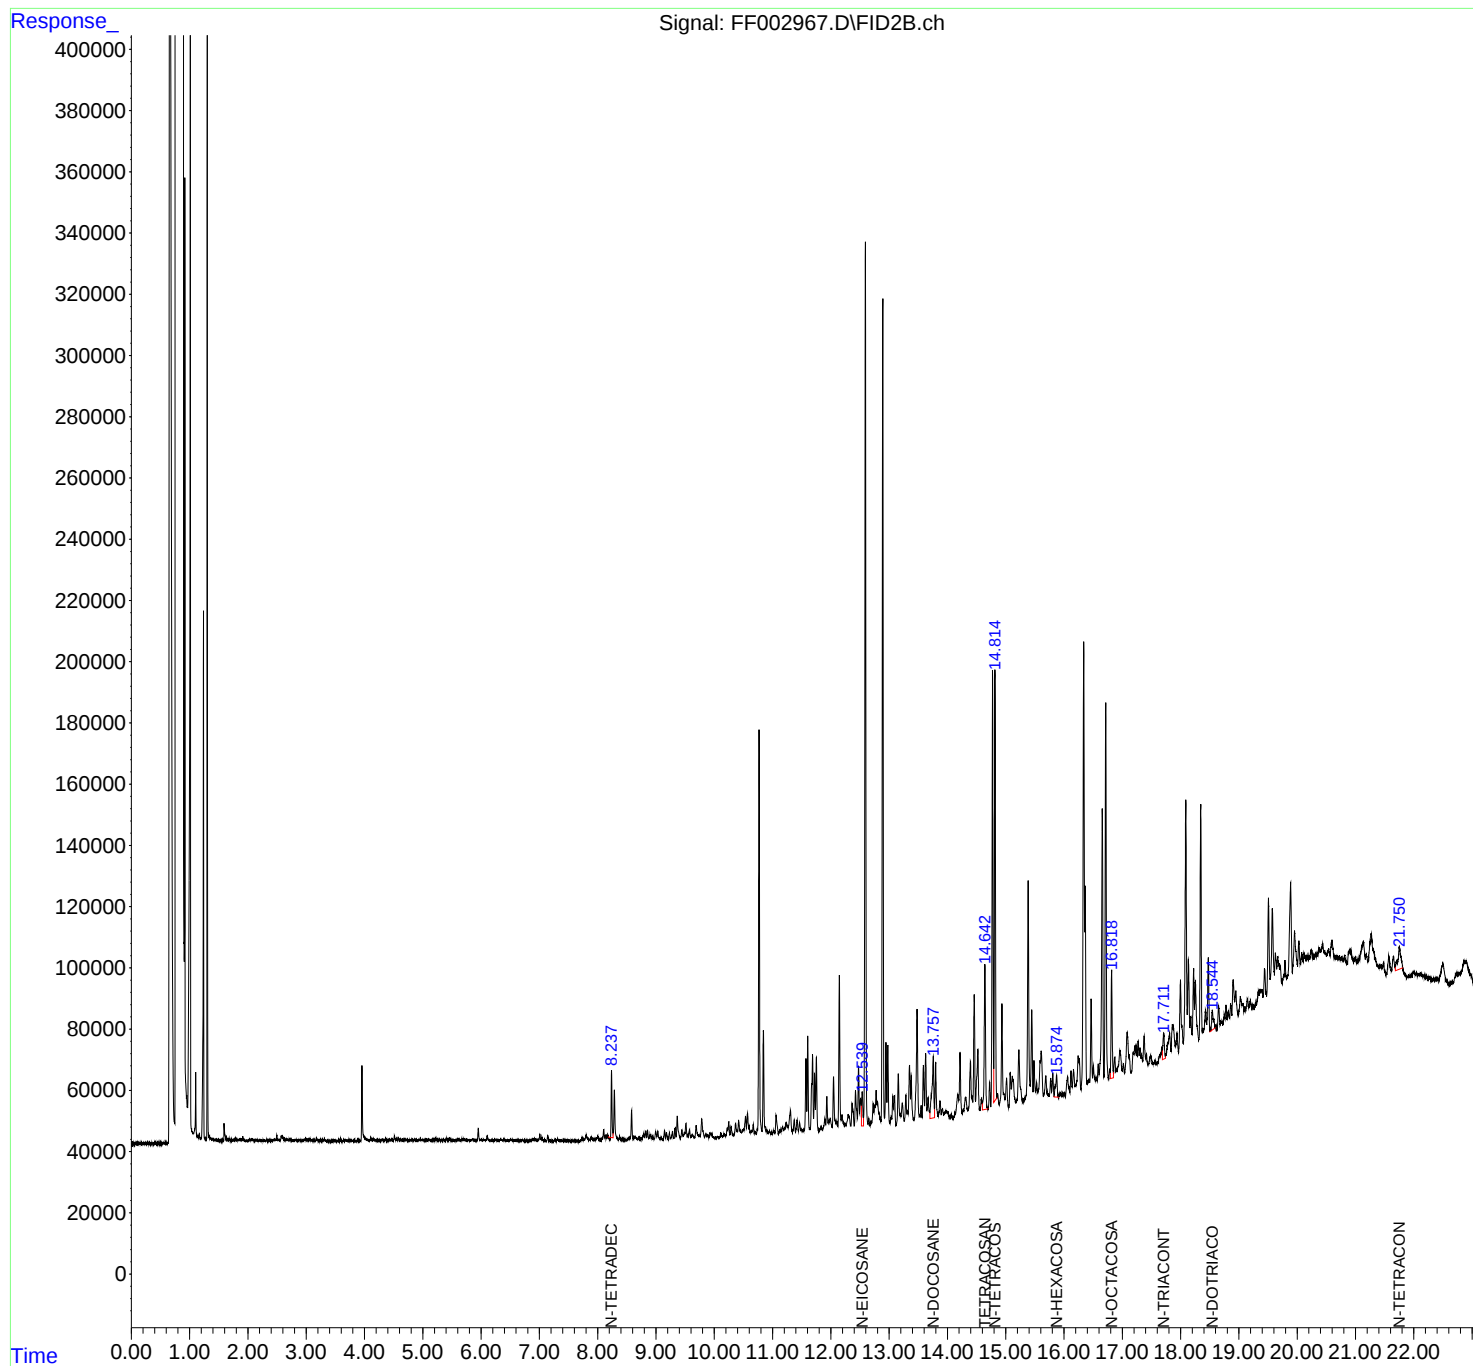


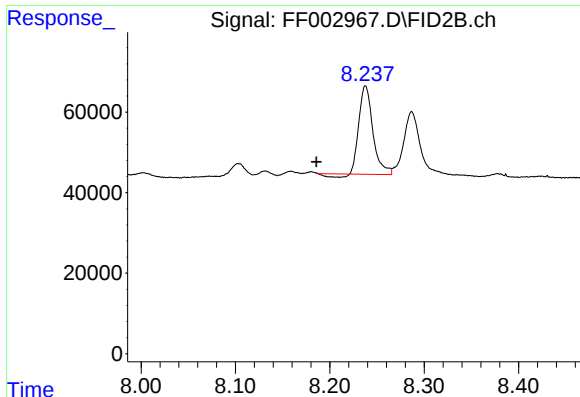

#4 N-TETRADECANE


R.T.: 8.238 min
Delta R.T.: 0.052 min
Response: 220234
Conc: 1.37 ug/ml

Instrument :
FID_F
ClientSampleId :

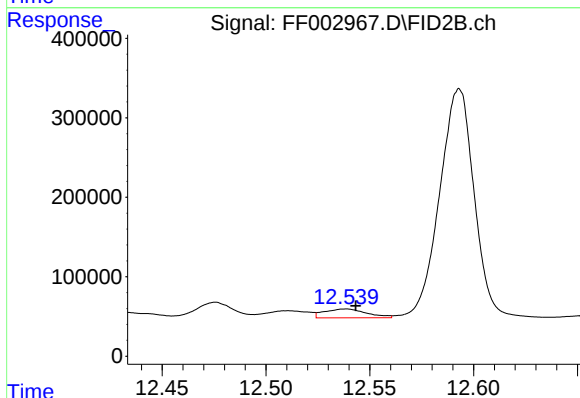


#7 N-EICOSANE

R.T.: 12.538 min
Delta R.T.: -0.005 min
Response: 157857
Conc: 1.02 ug/ml

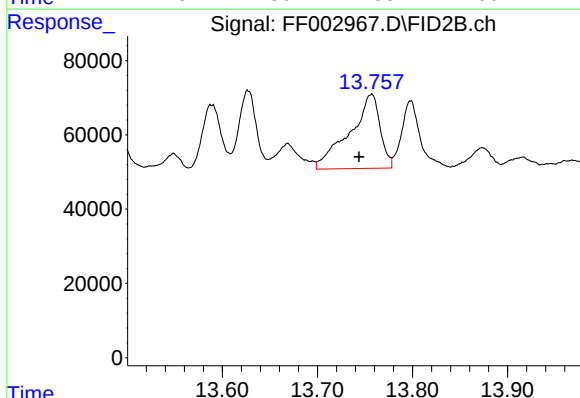


#8 N-DOCOSANE

R.T.: 13.757 min
Delta R.T.: 0.013 min
Response: 444706
Conc: 2.97 ug/ml

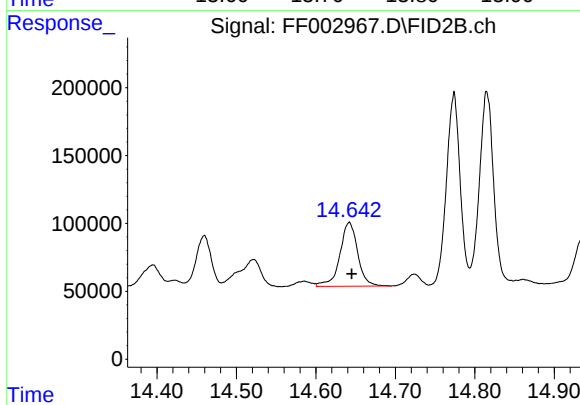

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.642 min
Delta R.T.: -0.003 min
Response: 734259
Conc: 5.66 ug/ml

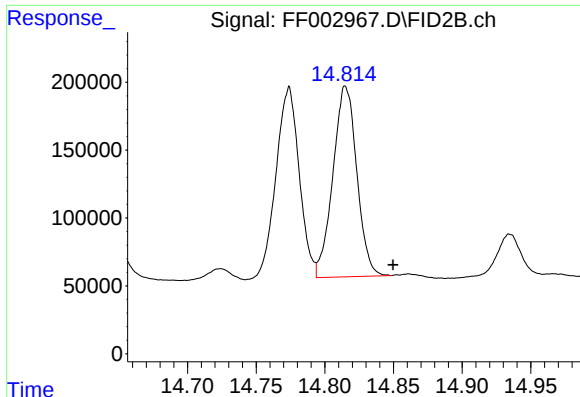

#10 N-TETRACOSANE


R.T.: 14.815 min
Delta R.T.: -0.034 min
Response: 1702408
Conc: 11.78 ug/ml

Instrument :
FID_F
ClientSampleId :

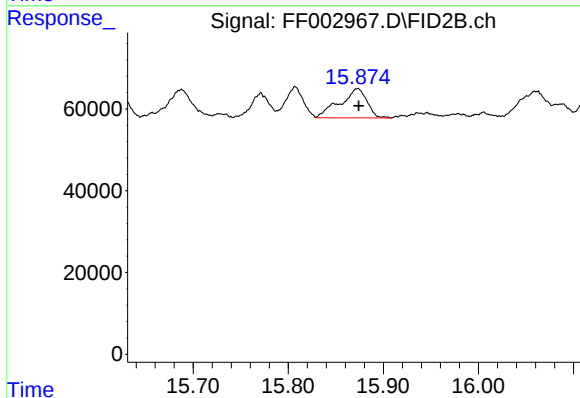


#11 N-HEXACOSANE

R.T.: 15.873 min
Delta R.T.: -0.001 min
Response: 140525
Conc: 1.01 ug/ml

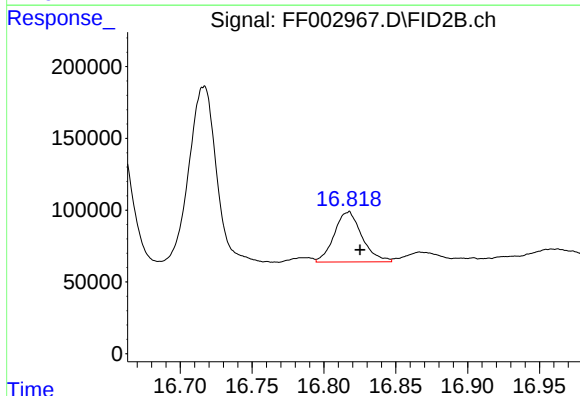


#12 N-OCTACOSANE

R.T.: 16.817 min
Delta R.T.: -0.008 min
Response: 467486
Conc: 3.49 ug/ml

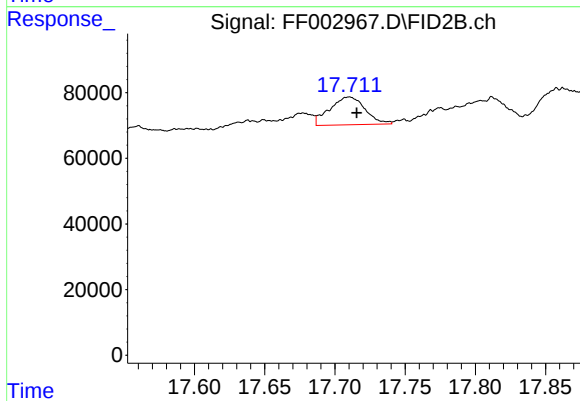

#13 N-TRIACONTANE


R.T.: 17.710 min
Delta R.T.: -0.005 min
Response: 149051
Conc: 1.16 ug/ml

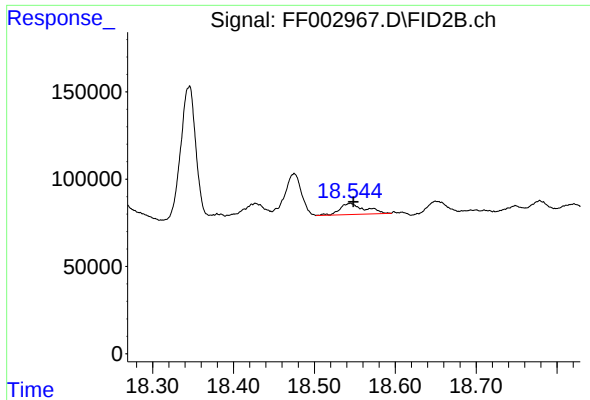

#14 N-DOTRIACONTANE

R.T.: 18.544 min
Delta R.T.: -0.004 min
Response: 135832
Conc: 1.14 ug/ml

Instrument :
FID_F
ClientSampleId :

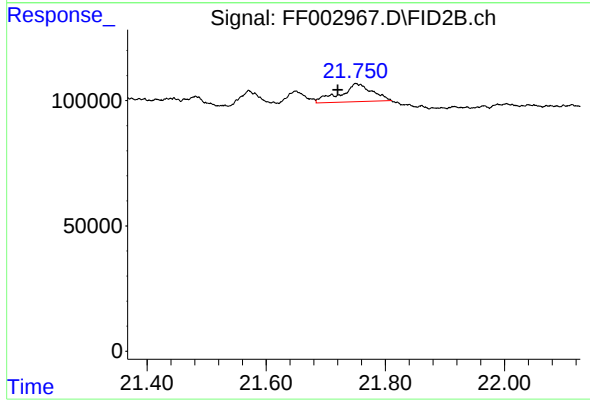

#18 N-TETRACONTANE

R.T.: 21.751 min
Delta R.T.: 0.031 min
Response: 268148
Conc: 2.55 ug/ml