

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121018\
 Data File : FF002970.D
 Signal(s) : FID2B.ch
 Acq On : 10 Dec 2018 21:40
 Operator : AJ\SJ
 Sample : J6316-01 5X
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 11 01:00:24 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.640	366909	2.826 ug/ml
Target Compounds			
3) N-DODECANE	6.390	254061	1.600 ug/ml
4) N-TETRADECANE	8.237f	80854	0.504 ug/ml
7) N-EICOSANE	12.589	500561	3.246 ug/ml
10) N-TETRACOSANE	14.813	482786	3.341 ug/ml
12) N-OCTACOSANE	16.817	141356	1.055 ug/ml
13) N-TRIACONTANE	17.709	134464	1.049 ug/ml
18) N-TETRACONTANE	21.685	9334	0.089 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121018\
Data File : FF002970.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2018 21:40
Operator : AJ\SJ
Sample : J6316-01 5X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 11 01:00:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

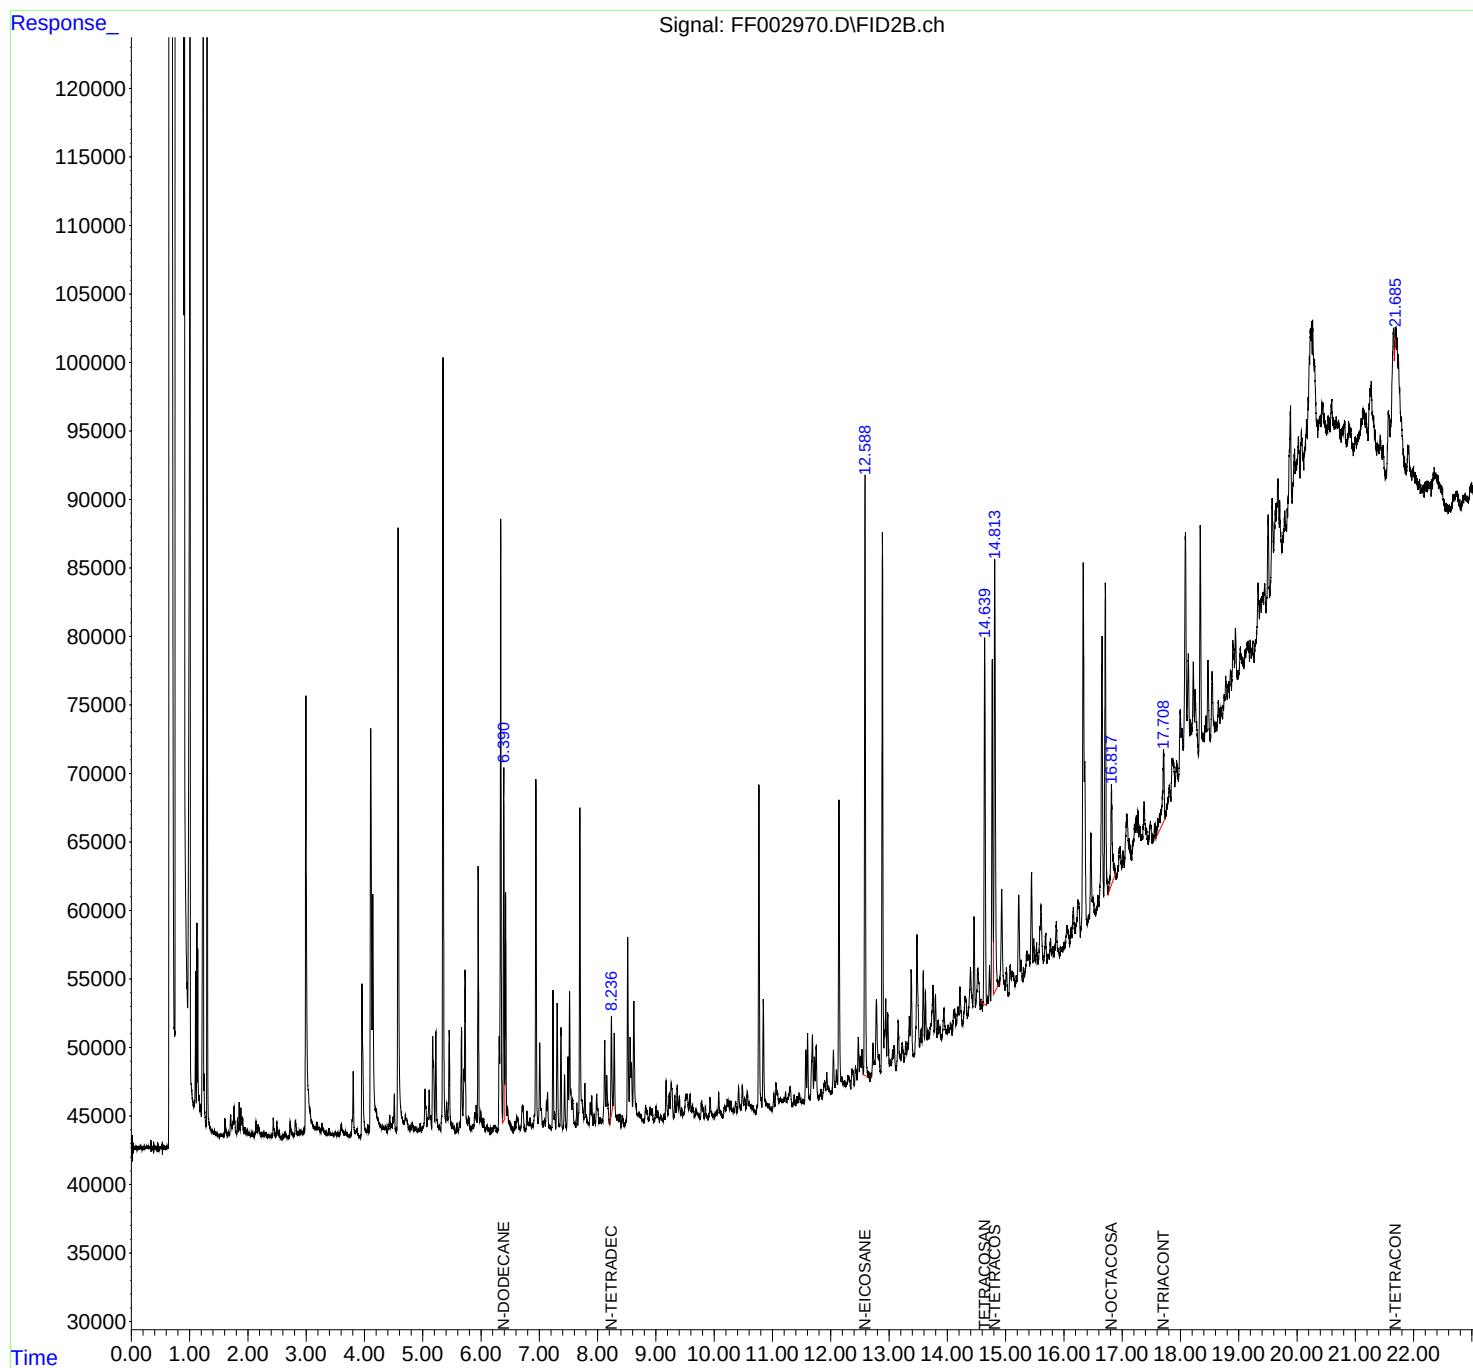


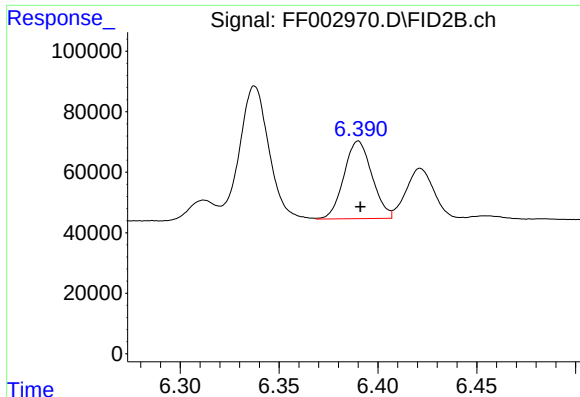

#3 N-DODECANE


R.T.: 6.390 min
Delta R.T.: 0.000 min
Response: 254061
Conc: 1.60 ug/ml

Instrument :
FID_F
ClientSampleId :

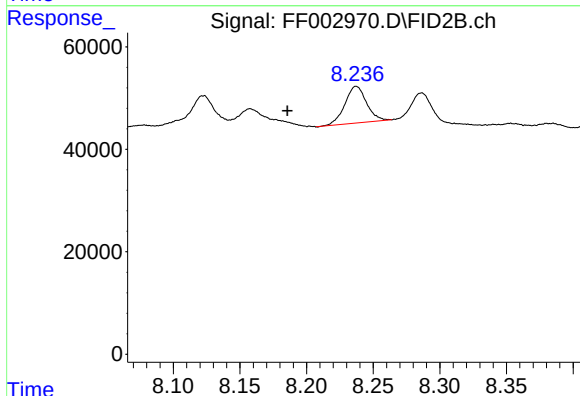


#4 N-TETRADECANE

R.T.: 8.237 min
Delta R.T.: 0.052 min
Response: 80854
Conc: 0.50 ug/ml

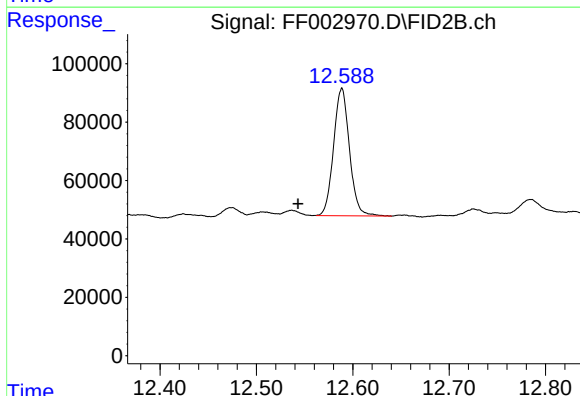


#7 N-EICOSANE

R.T.: 12.589 min
Delta R.T.: 0.045 min
Response: 500561
Conc: 3.25 ug/ml

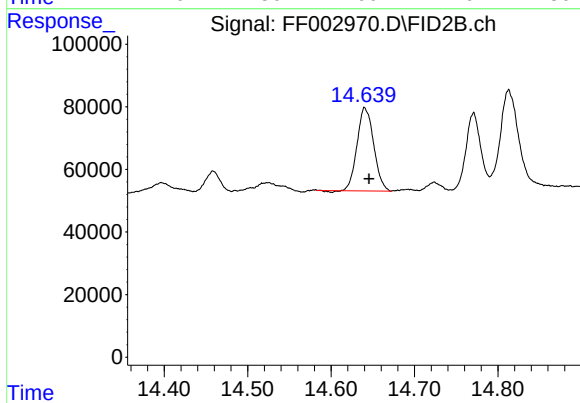

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.640 min
Delta R.T.: -0.005 min
Response: 366909
Conc: 2.83 ug/ml

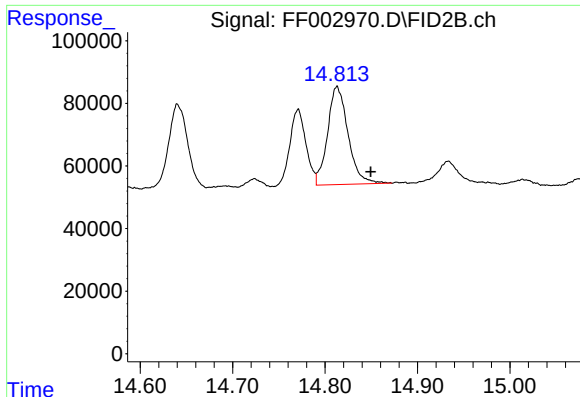

#10 N-TETRACOSANE


R.T.: 14.813 min
Delta R.T.: -0.037 min
Response: 482786
Conc: 3.34 ug/ml

Instrument :
FID_F
ClientSampleId :

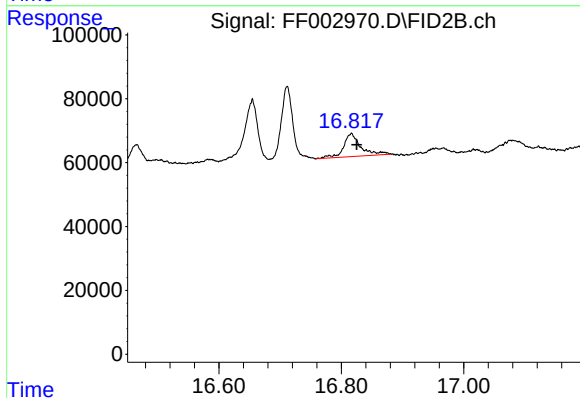


#12 N-OCTACOSANE

R.T.: 16.817 min
Delta R.T.: -0.008 min
Response: 141356
Conc: 1.06 ug/ml

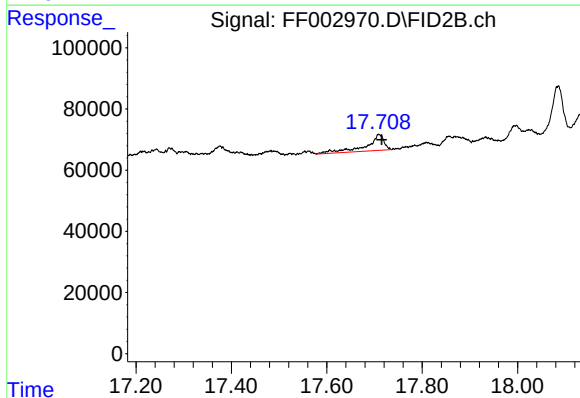

#13 N-TRIACONTANE

R.T.: 17.709 min
Delta R.T.: -0.006 min
Response: 134464
Conc: 1.05 ug/ml

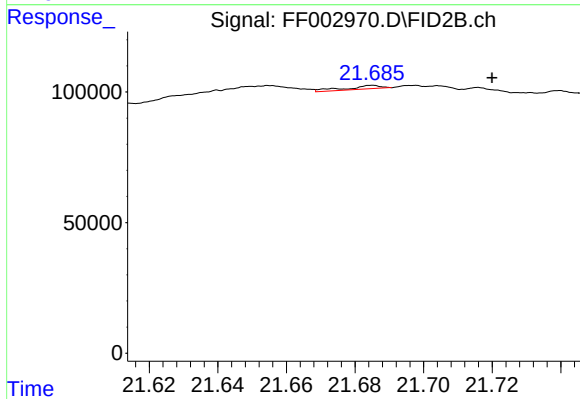

#18 N-TETRACONTANE

R.T.: 21.685 min
Delta R.T.: -0.035 min
Response: 9334
Conc: 0.09 ug/ml