

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121018\
 Data File : FF002957.D
 Signal(s) : FID2B.ch
 Acq On : 10 Dec 2018 15:03
 Operator : AJ\SJ
 Sample : PB115483BS
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Dec 11 00:57:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.639	1707710	13.154 ug/ml
Target Compounds			
1) N-OCTANE	2.270	2096025	13.549 ug/ml
2) N-DECANE	4.364	2440742	15.579 ug/ml
3) N-DODECANE	6.386	2465973	15.529 ug/ml
4) N-TETRADECANE	8.179	2400983	14.979 ug/ml
5) N-HEXADECANE	9.781	2343448	14.633 ug/ml
6) N-OCTADECANE	11.224	2298524	14.509 ug/ml
7) N-EICOSANE	12.536	2234716	14.490 ug/ml
8) N-DOCOSANE	13.737	2187179	14.627 ug/ml
10) N-TETRACOSANE	14.843	2196394	15.198 ug/ml
11) N-HEXACOSANE	15.867	2064690	14.792 ug/ml
12) N-OCTACOSANE	16.820	2031794	15.164 ug/ml
13) N-TRIACONTANE	17.711	1997818	15.592 ug/ml
14) N-DOTRIACONTANE	18.545	2025046	16.957 ug/ml
15) N-TETRATRIACONTANE	19.335	2031643	17.926 ug/ml
16) N-HEXATRIACONTANE	20.079	1981884	18.368 ug/ml
17) N-OCTATRIACONTANE	20.819	1929579	19.011 ug/ml
18) N-TETRACONTANE	21.720	1952404	18.576 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121018\
Data File : FF002957.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2018 15:03
Operator : AJ\SJ
Sample : PB115483BS
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Dec 11 00:57:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

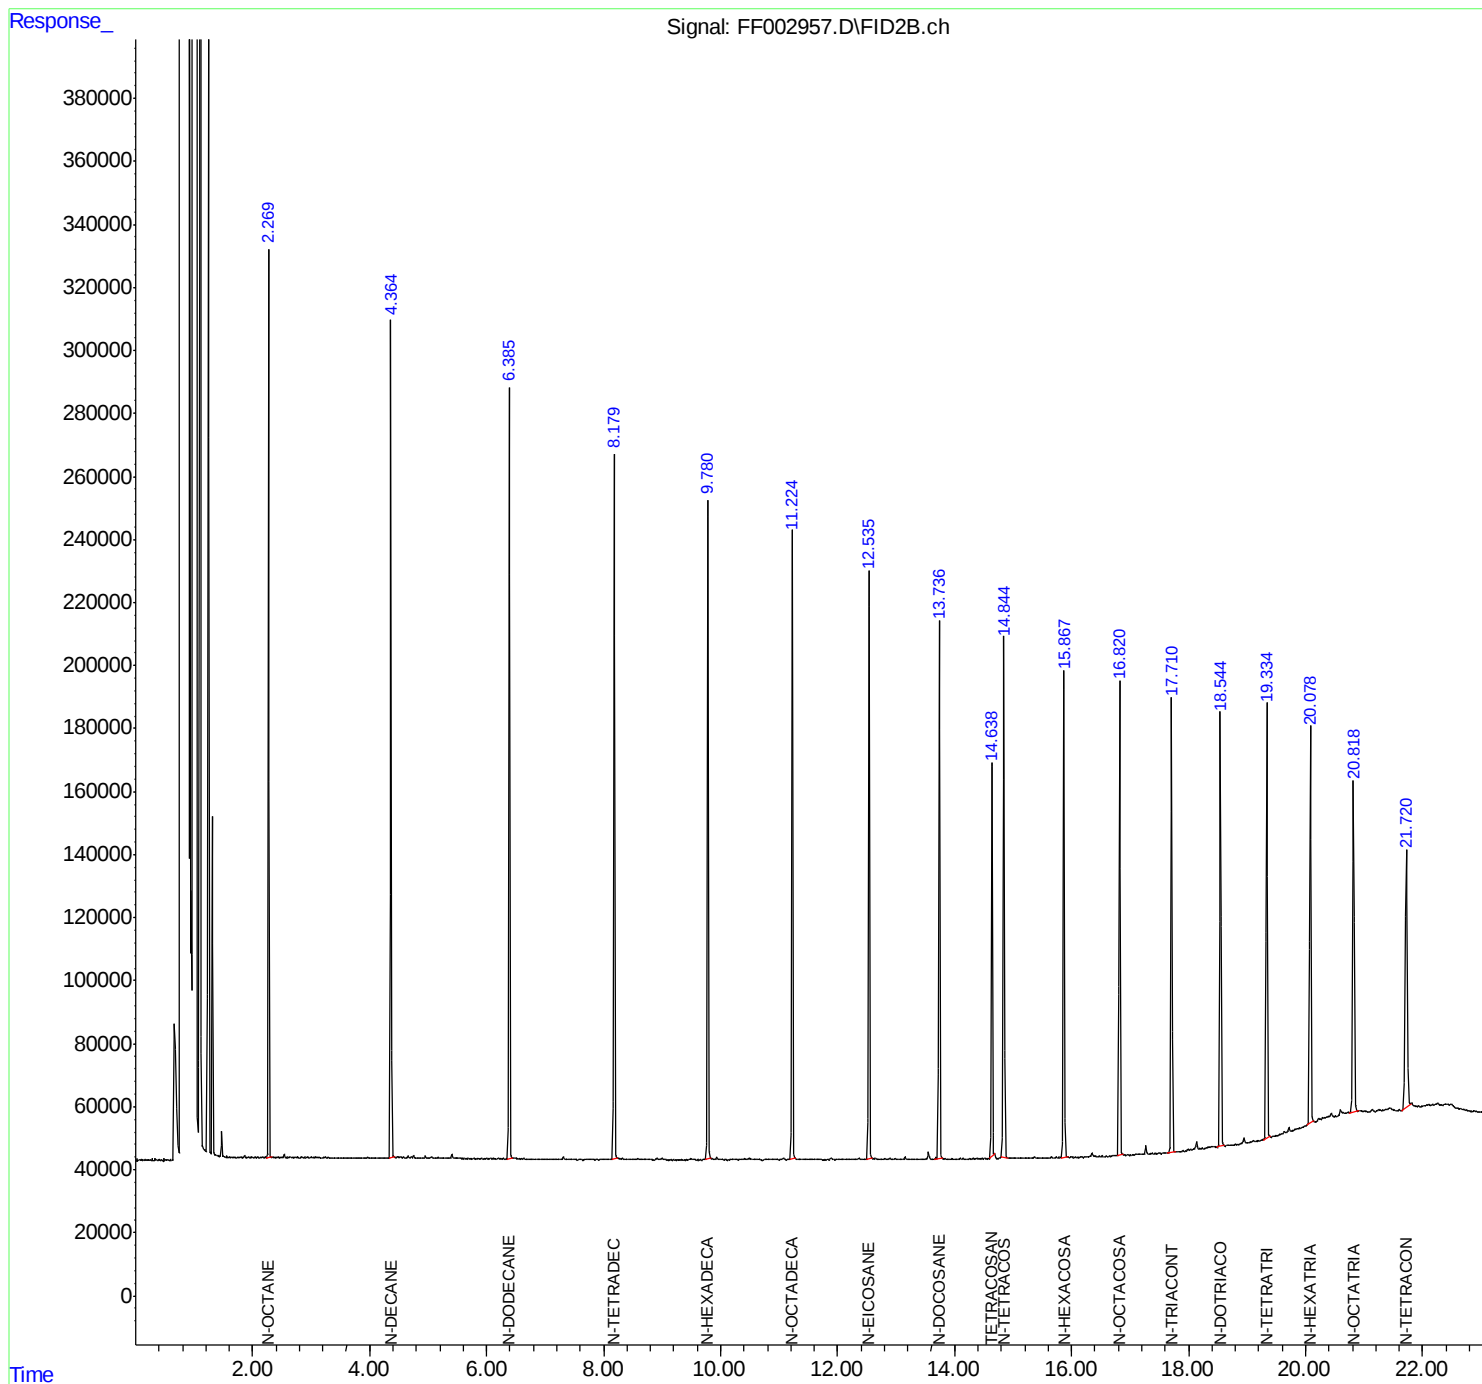


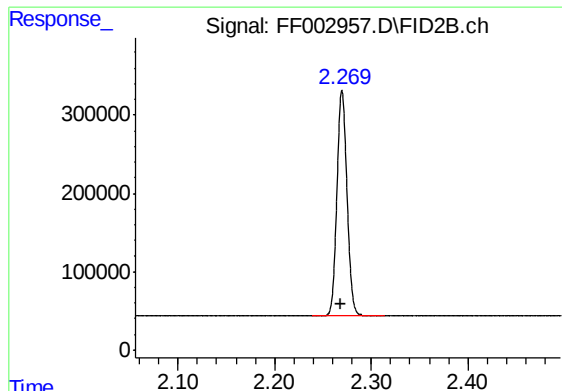

#1 N-OCTANE


R.T.: 2.270 min
Delta R.T.: 0.002 min
Response: 2096025
Conc: 13.55 ug/ml

Instrument :
FID_F
ClientSampleId :

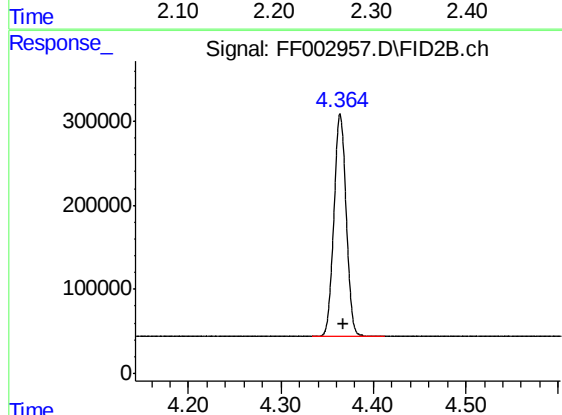


#2 N-DECANE

R.T.: 4.364 min
Delta R.T.: -0.004 min
Response: 2440742
Conc: 15.58 ug/ml

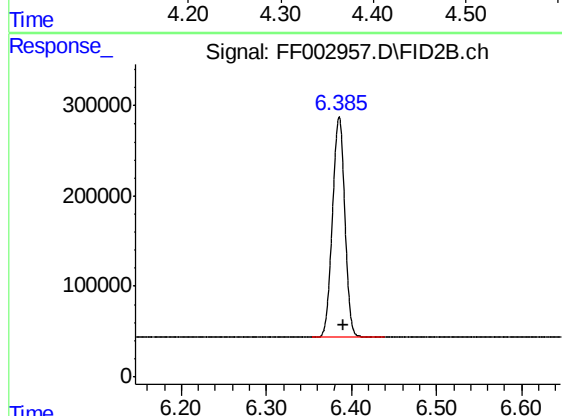


#3 N-DODECANE

R.T.: 6.386 min
Delta R.T.: -0.005 min
Response: 2465973
Conc: 15.53 ug/ml

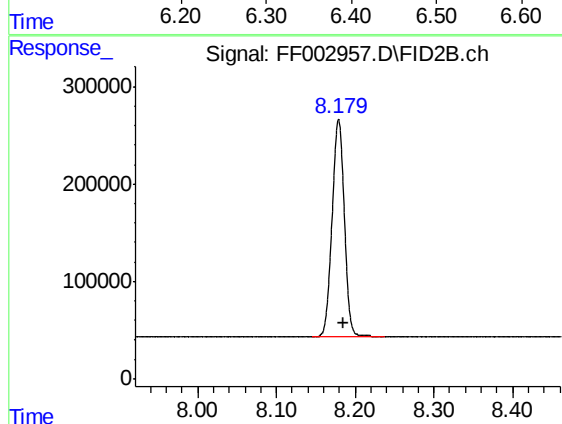

#4 N-TETRADECANE


R.T.: 8.179 min
Delta R.T.: -0.007 min
Response: 2400983
Conc: 14.98 ug/ml

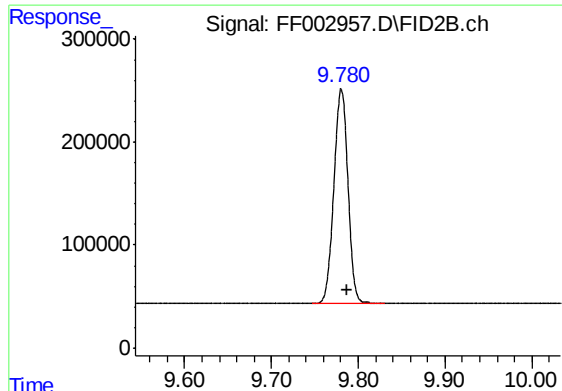

#5 N-HEXADECANE


R.T.: 9.781 min
Delta R.T.: -0.007 min
Response: 2343448
Conc: 14.63 ug/ml

Instrument :
FID_F
ClientSampleId :

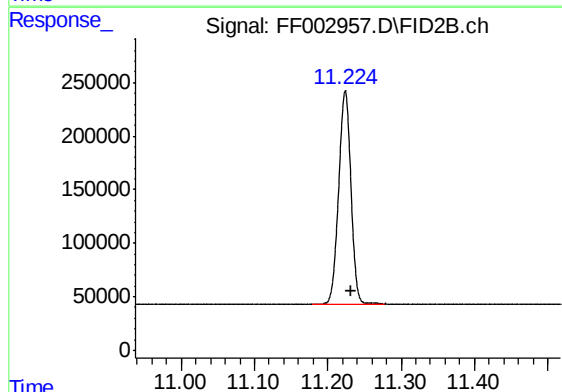


#6 N-OCTADECANE

R.T.: 11.224 min
Delta R.T.: -0.007 min
Response: 2298524
Conc: 14.51 ug/ml

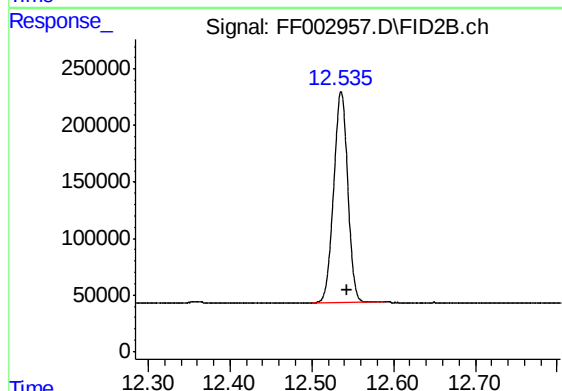


#7 N-EICOSANE

R.T.: 12.536 min
Delta R.T.: -0.007 min
Response: 2234716
Conc: 14.49 ug/ml

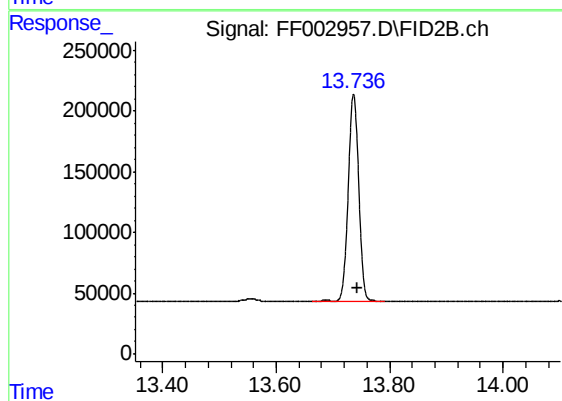

#8 N-DOCOSANE


R.T.: 13.737 min
Delta R.T.: -0.007 min
Response: 2187179
Conc: 14.63 ug/ml

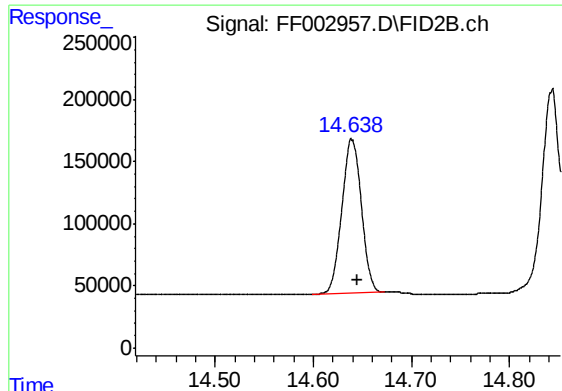

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.639 min
Delta R.T.: -0.006 min
Response: 1707710
Conc: 13.15 ug/ml

Instrument :
FID_F
ClientSampleId :

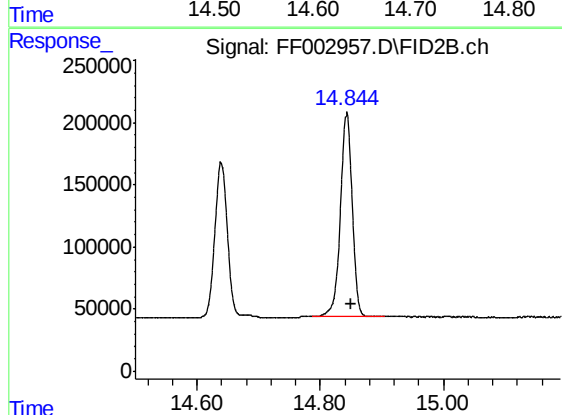


#10 N-TETRACOSANE

R.T.: 14.843 min
Delta R.T.: -0.006 min
Response: 2196394
Conc: 15.20 ug/ml

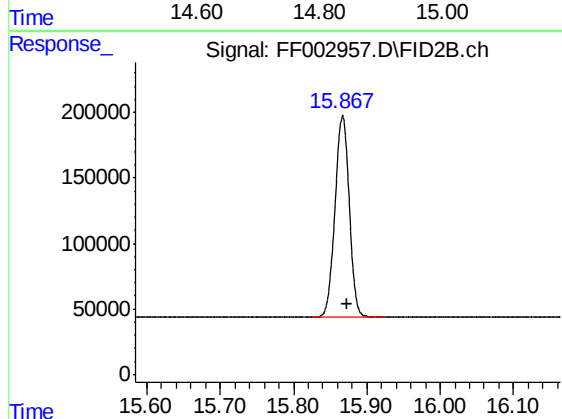


#11 N-HEXACOSANE

R.T.: 15.867 min
Delta R.T.: -0.007 min
Response: 2064690
Conc: 14.79 ug/ml

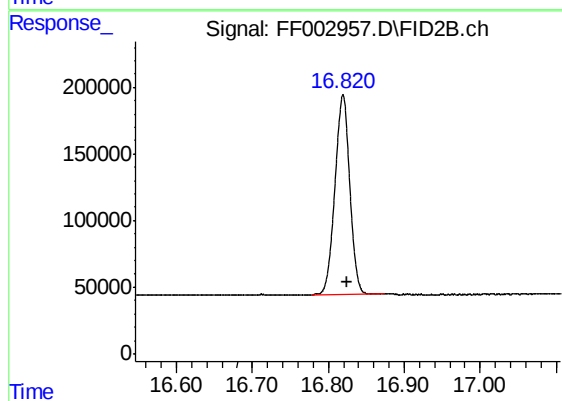

#12 N-OCTACOSANE


R.T.: 16.820 min
Delta R.T.: -0.005 min
Response: 2031794
Conc: 15.16 ug/ml

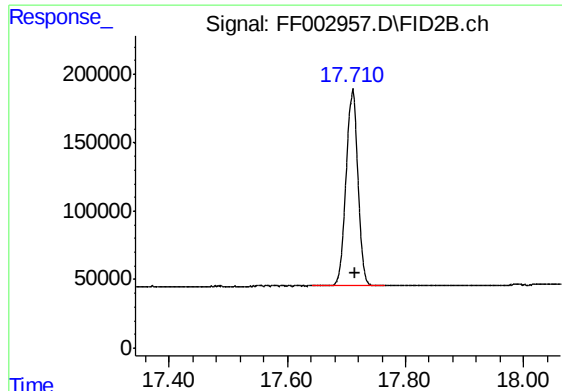

#13 N-TRIACONTANE


R.T.: 17.711 min
Delta R.T.: -0.005 min
Response: 1997818
Conc: 15.59 ug/ml

Instrument :
FID_F
ClientSampleId :

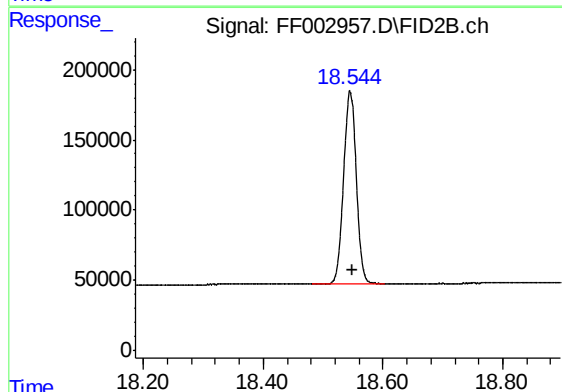


#14 N-DOTRIACONTANE

R.T.: 18.545 min
Delta R.T.: -0.004 min
Response: 2025046
Conc: 16.96 ug/ml

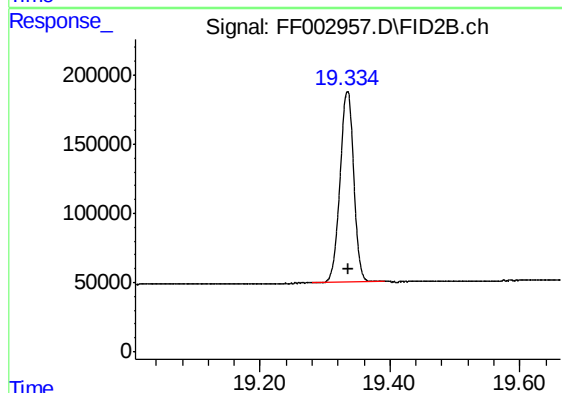


#15 N-TETRATRIACONTANE

R.T.: 19.335 min
Delta R.T.: 0.000 min
Response: 2031643
Conc: 17.93 ug/ml

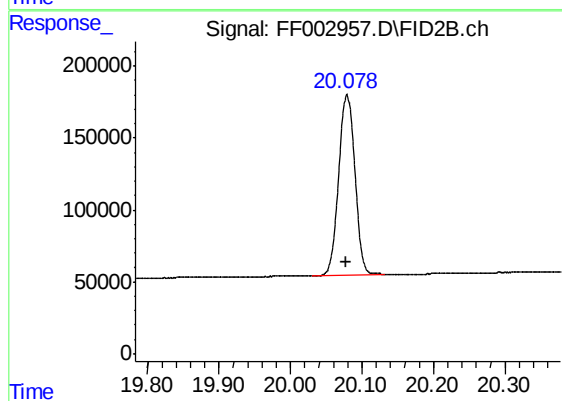

#16 N-HEXATRIACONTANE


R.T.: 20.079 min
Delta R.T.: 0.002 min
Response: 1981884
Conc: 18.37 ug/ml

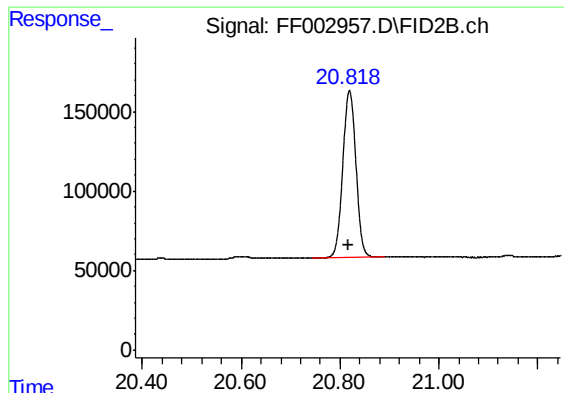

#17 N-OCTATRIACONTANE

R.T.: 20.819 min
Delta R.T.: 0.003 min
Response: 1929579
Conc: 19.01 ug/ml

Instrument :
FID_F
ClientSampleId :

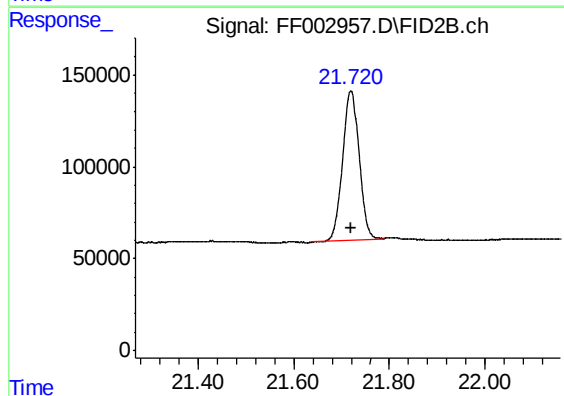

#18 N-TETRACONTANE

R.T.: 21.720 min
Delta R.T.: 0.000 min
Response: 1952404
Conc: 18.58 ug/ml