

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121020\
Data File : FF007942.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2020 10:07
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 11 01:00:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120220.M
Quant Title :
QLast Update : Thu Dec 03 09:08:10 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.615	99431	0.897 ug/ml
15) N-TETRATRIACONTANE	19.402	82290	0.959 ug/ml
16) N-HEXATRIACONTANE	20.144	38202	0.588 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121020\
Data File : FF007942.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2020 10:07
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 11 01:00:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120220.M
Quant Title :
QLast Update : Thu Dec 03 09:08:10 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

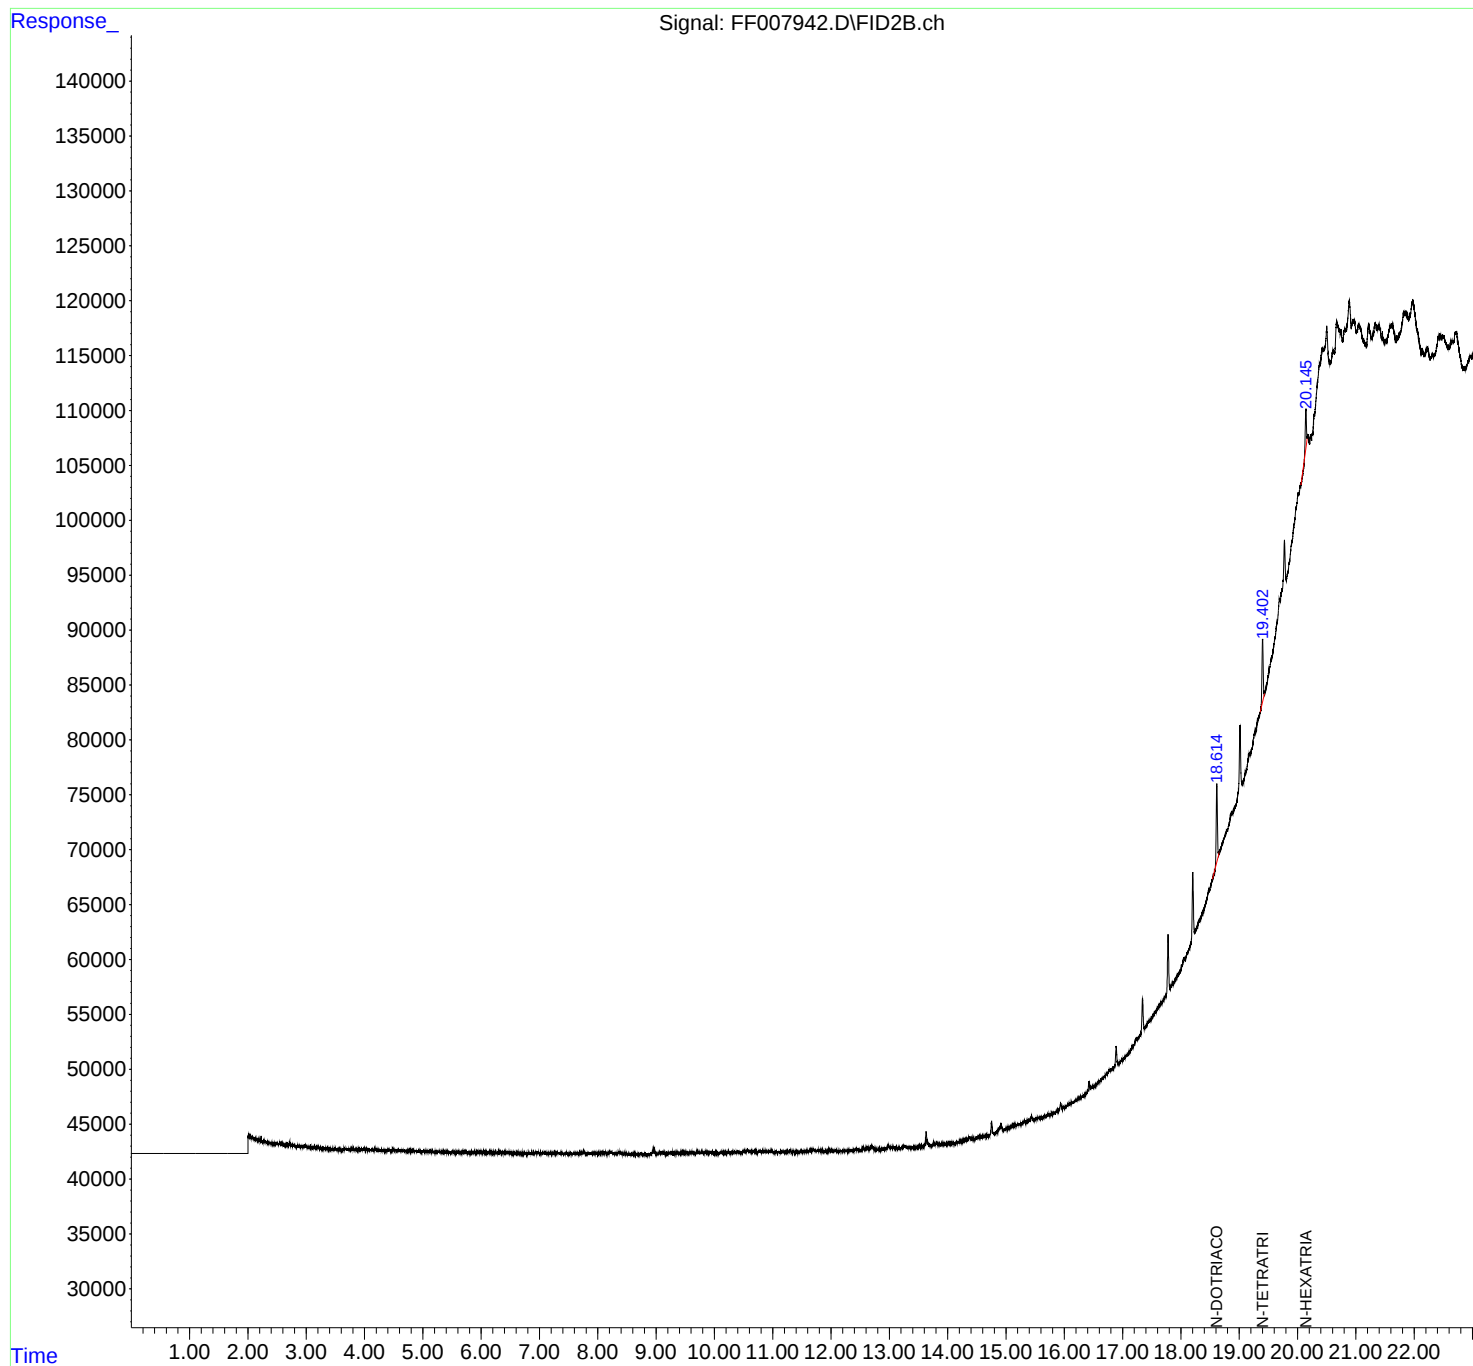


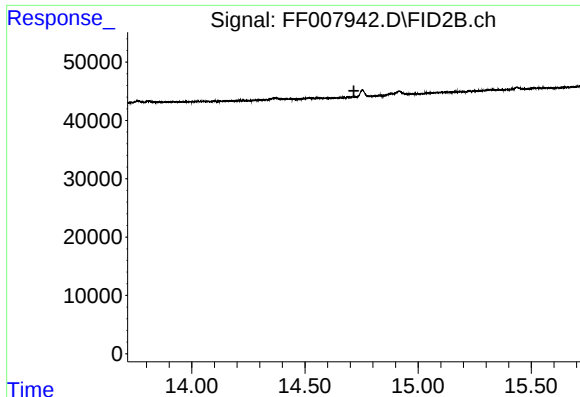

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.716 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

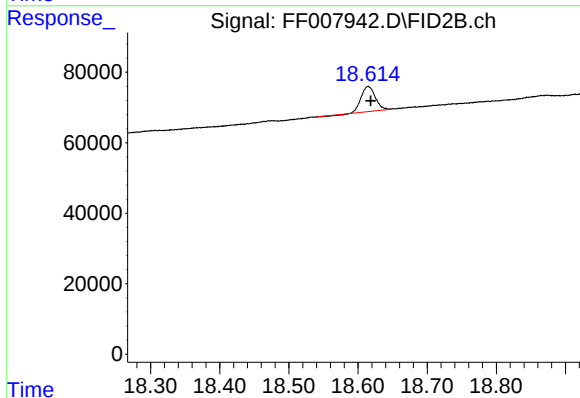


#14 N-DOTRIACONTANE

R.T.: 18.615 min
Delta R.T.: -0.004 min
Response: 99431
Conc: 0.90 ug/ml

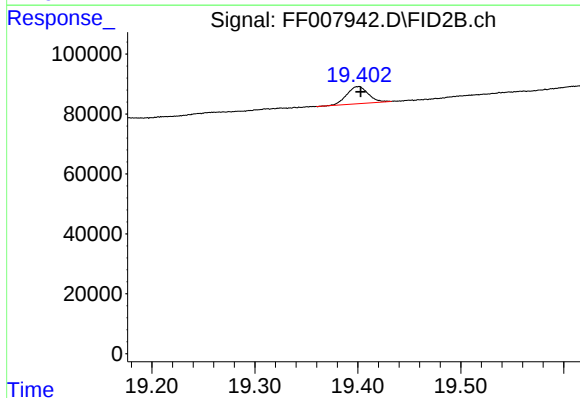

#15 N-TETRATRIACONTANE

R.T.: 19.402 min
Delta R.T.: -0.001 min
Response: 82290
Conc: 0.96 ug/ml

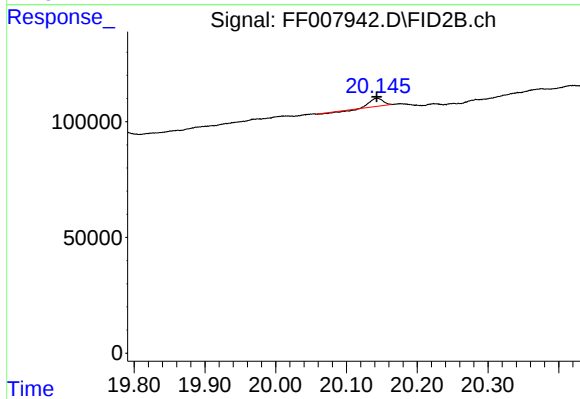

#16 N-HEXATRIACONTANE

R.T.: 20.144 min
Delta R.T.: 0.001 min
Response: 38202
Conc: 0.59 ug/ml