

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF121020\  
 Data File : FF007951.D  
 Signal(s) : FID2B.ch  
 Acq On : 10 Dec 2020 16:11  
 Operator : DD\AJ  
 Sample : L5009-06  
 Misc :  
 ALS Vial : 60 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Dec 11 01:02:11 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF120220.M  
 Quant Title :  
 QLast Update : Thu Dec 03 09:08:10 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.707 | 2394968  | 18.943 ug/ml |
| Target Compounds              |        |          |              |
| 4) N-TETRADECANE              | 8.313f | 248133   | 1.690 ug/ml  |
| 14) N-DOTRIACONTANE           | 18.606 | 131120   | 1.183 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF121020\  
Data File : FF007951.D  
Signal(s) : FID2B.ch  
Acq On : 10 Dec 2020 16:11  
Operator : DD\AJ  
Sample : L5009-06  
Misc :  
ALS Vial : 60 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Dec 11 01:02:11 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF120220.M  
Quant Title :  
QLast Update : Thu Dec 03 09:08:10 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

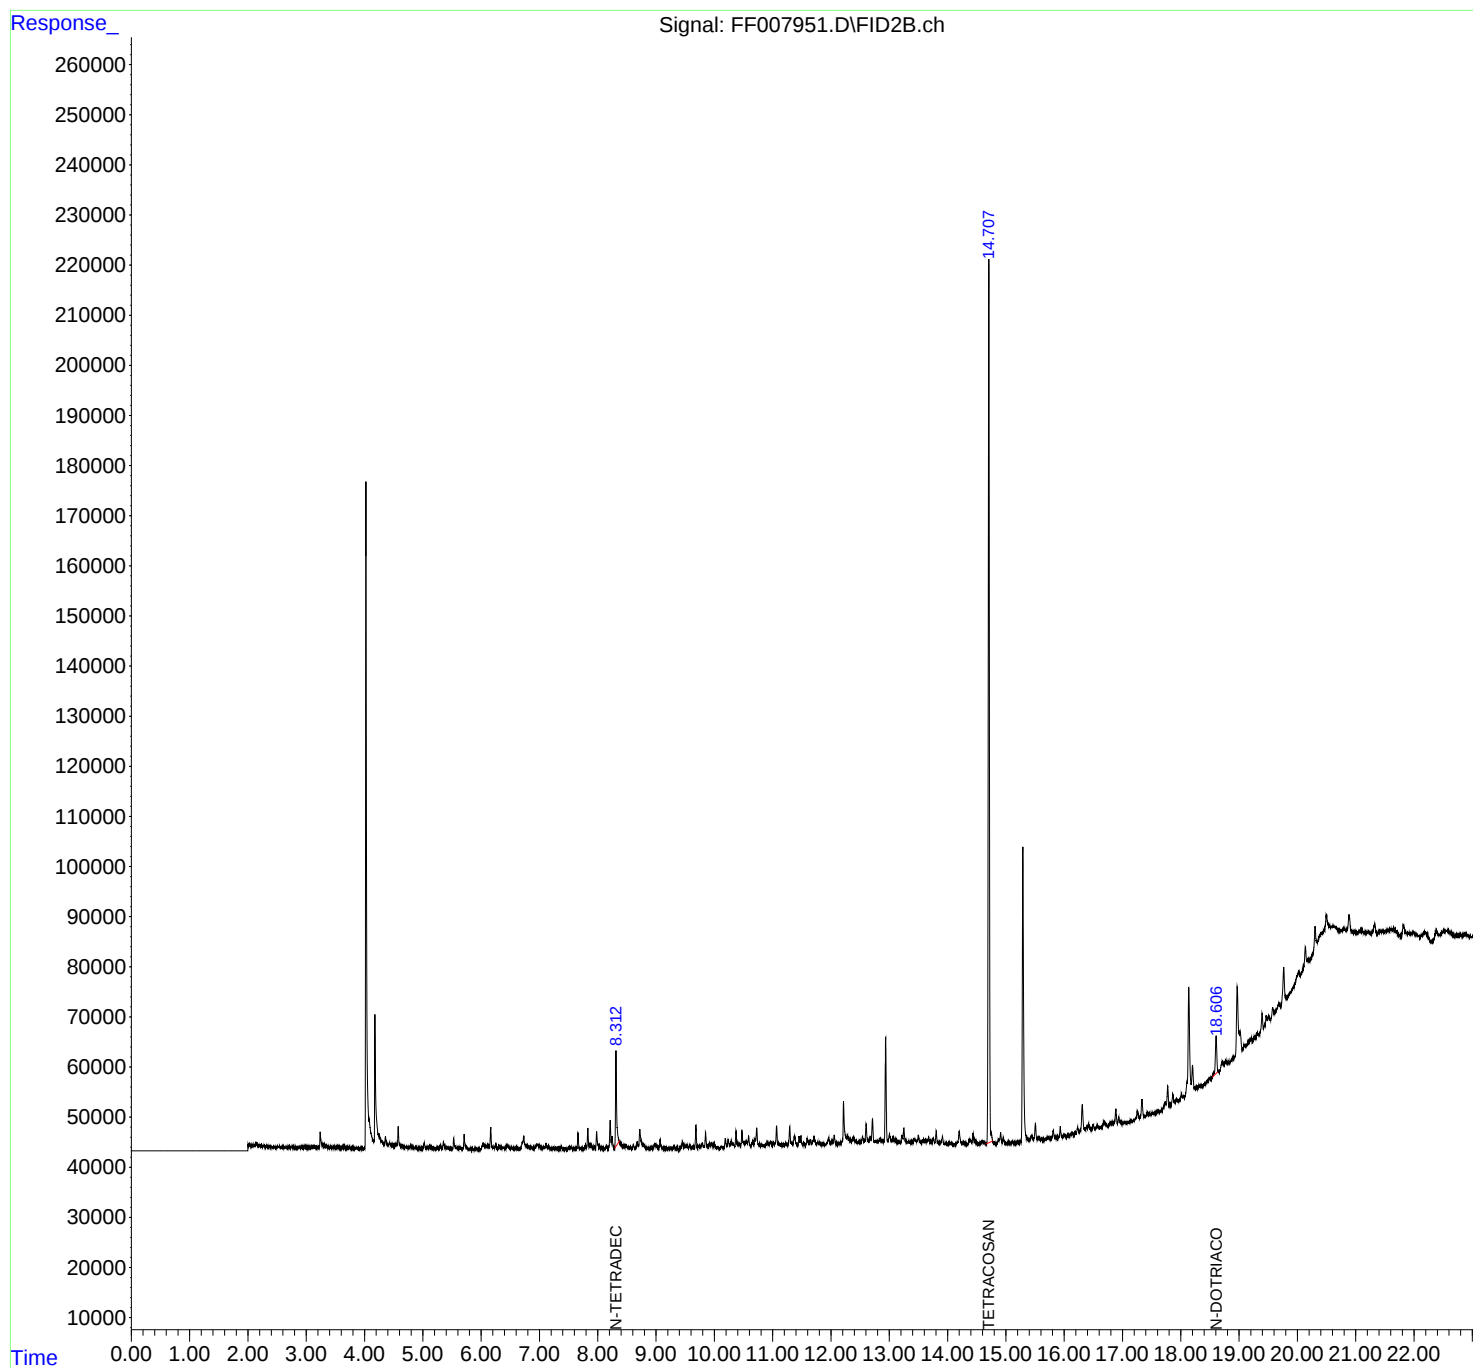


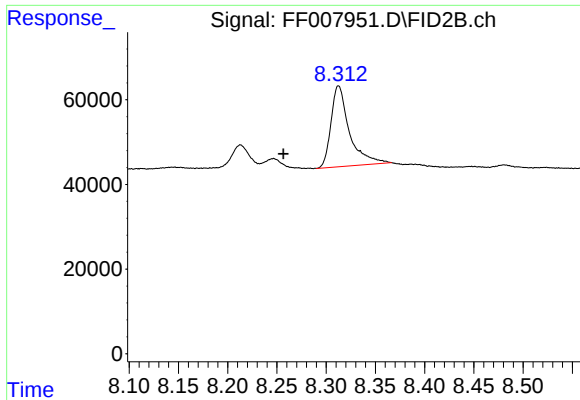

#4 N-TETRADECANE


R.T.: 8.313 min  
Delta R.T.: 0.056 min  
Response: 248133  
Conc: 1.69 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

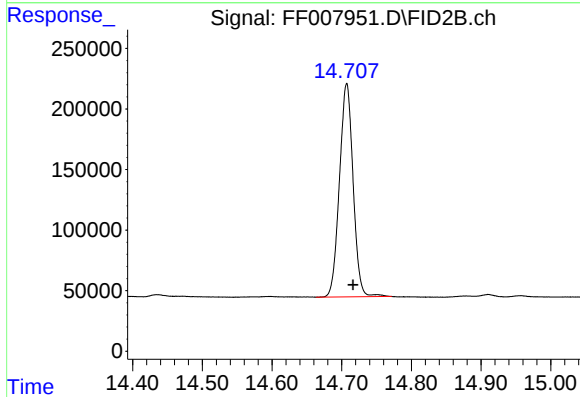

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.707 min  
Delta R.T.: -0.009 min  
Response: 2394968  
Conc: 18.94 ug/ml

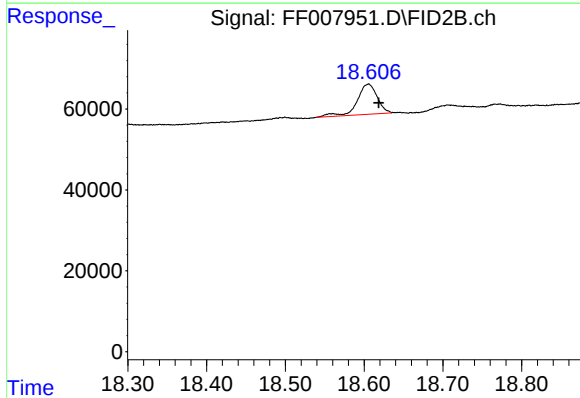

#14 N-DOTRIACONTANE

R.T.: 18.606 min  
Delta R.T.: -0.012 min  
Response: 131120  
Conc: 1.18 ug/ml