

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121020\
Data File : FF007950.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2020 15:40
Operator : DD\AJ
Sample : L5009-03
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
KENS-B5-120920-13-15

Integration File: autoint1.e
Quant Time: Dec 11 01:02:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120220.M
Quant Title :
QLast Update : Thu Dec 03 09:08:10 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.708	2802439	22.166 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121020\
Data File : FF007950.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2020 15:40
Operator : DD\AJ
Sample : L5009-03
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
KENS-B5-120920-13-15

Integration File: autoint1.e
Quant Time: Dec 11 01:02:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120220.M
Quant Title :
QLast Update : Thu Dec 03 09:08:10 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

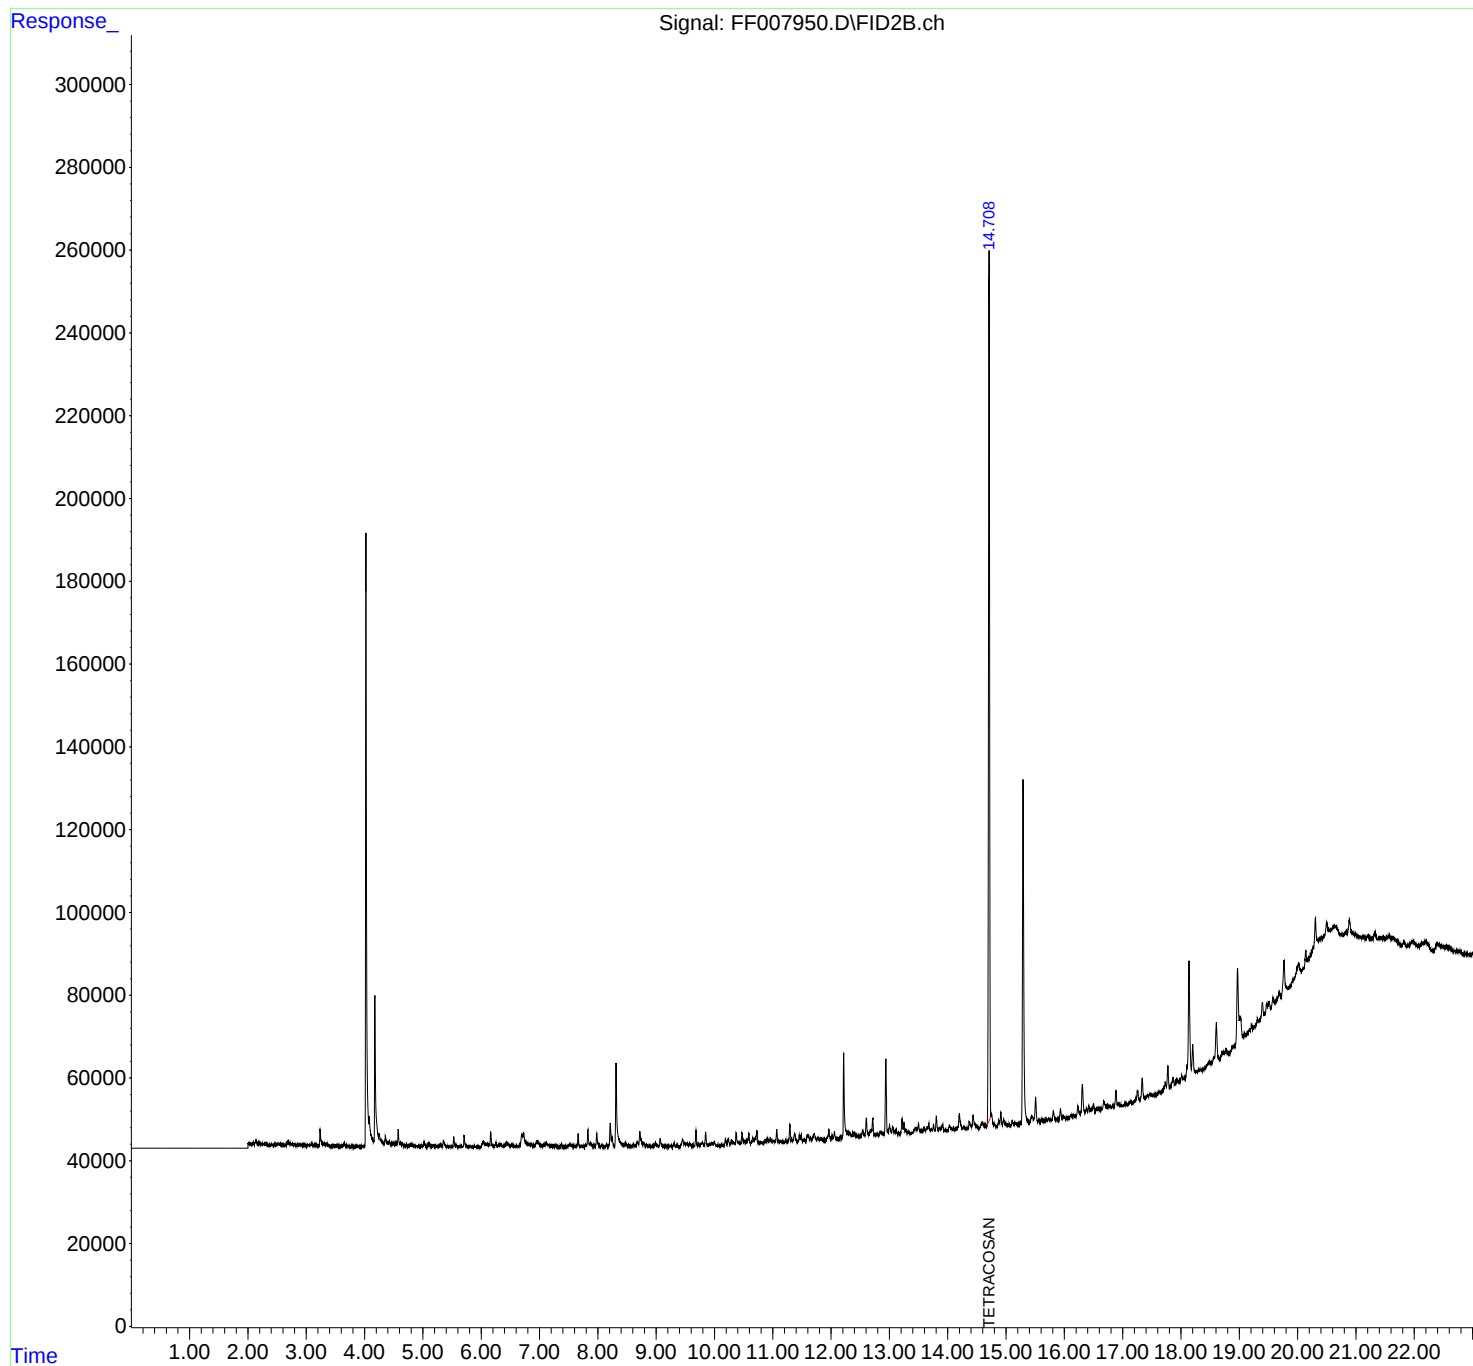

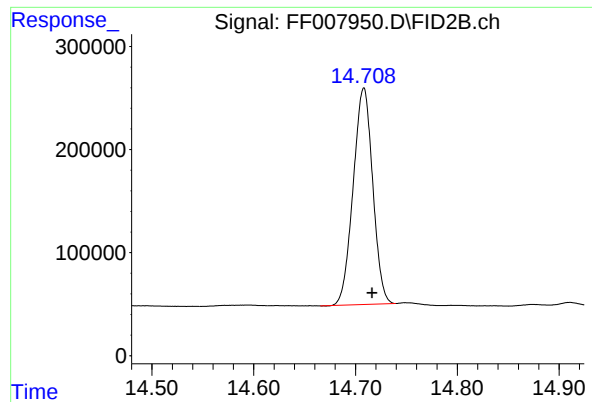

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.708 min
Delta R.T.: -0.008 min
Response: 2802439
Conc: 22.17 ug/ml

Instrument :
FID_F
ClientSampleId :
KENS-B5-120920-13-15