

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121020\
 Data File : FF007952.D
 Signal(s) : FID2B.ch
 Acq On : 10 Dec 2020 16:42
 Operator : DD\AJ
 Sample : L5009-06MS
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 KENS-B5-120920-DPMS

Integration File: autoint1.e
 Quant Time: Dec 11 01:02:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120220.M
 Quant Title :
 QLast Update : Thu Dec 03 09:08:10 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.706	1504992	11.904 ug/ml
Target Compounds			
2) N-DECANE	4.429	2911490	20.446 ug/ml
3) N-DODECANE	6.451	2939328	20.410 ug/ml
4) N-TETRADECANE	8.247	2989299	20.365 ug/ml
5) N-HEXADECANE	9.850	2931632	19.875 ug/ml
6) N-OCTADECANE	11.293	2914560	19.390 ug/ml
7) N-EICOSANE	12.604	2887497	19.252 ug/ml
8) N-DOCOSANE	13.805	2785198	19.022 ug/ml
10) N-TETRACOSANE	14.911	2649323	18.192 ug/ml
11) N-HEXACOSANE	15.934	2533809	17.980 ug/ml
12) N-OCTACOSANE	16.886	2451463	18.114 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121020\
Data File : FF007952.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2020 16:42
Operator : DD\AJ
Sample : L5009-06MS
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
KENS-B5-120920-DPMS

Integration File: autoint1.e
Quant Time: Dec 11 01:02:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120220.M
Quant Title :
QLast Update : Thu Dec 03 09:08:10 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

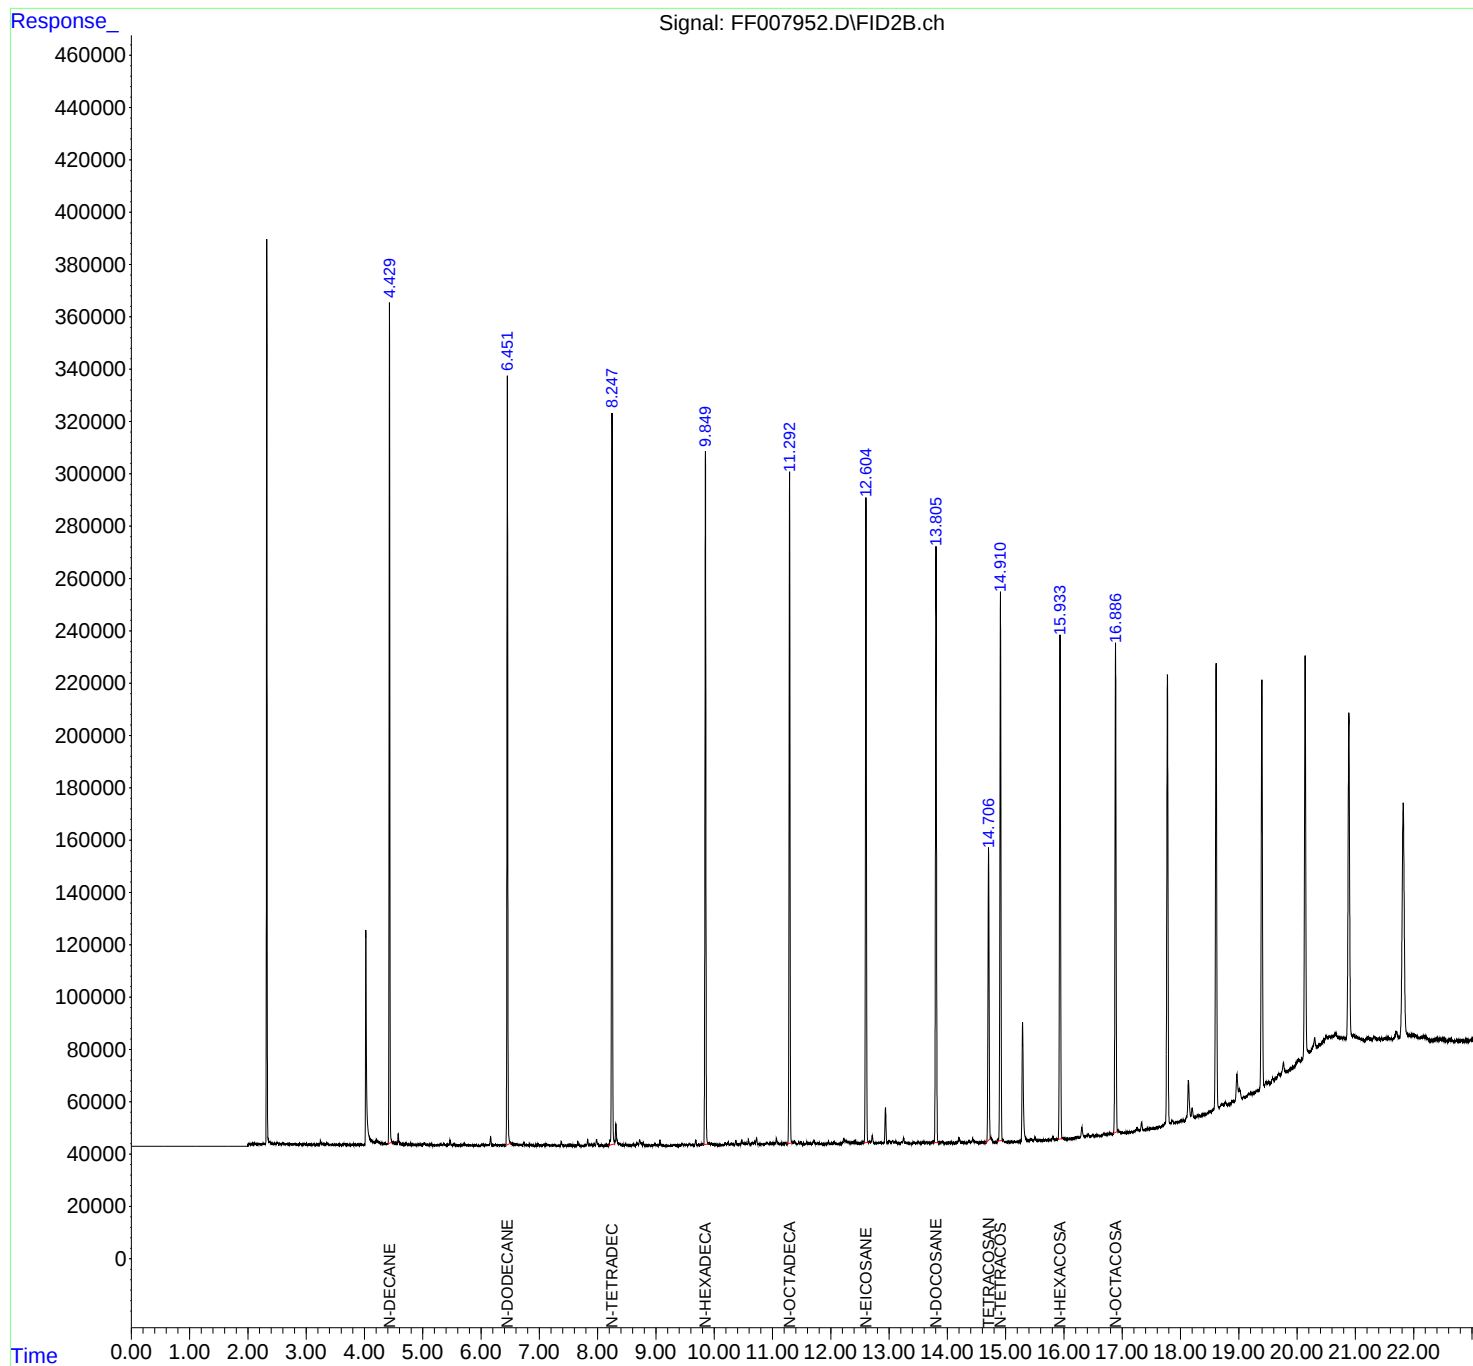


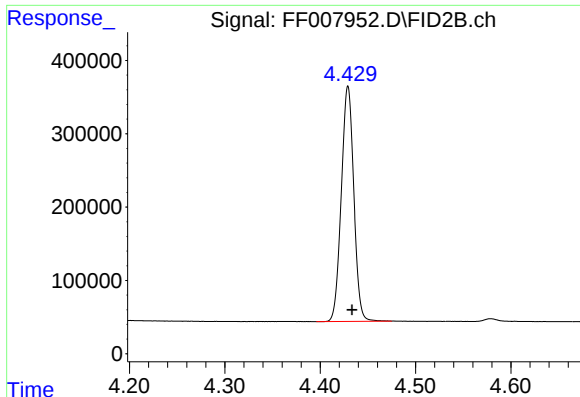

#2 N-DECANE


R.T.: 4.429 min
Delta R.T.: -0.004 min
Response: 2911490
Conc: 20.45 ug/ml

Instrument :
FID_F
ClientSampleId :
KENS-B5-120920-DPMS

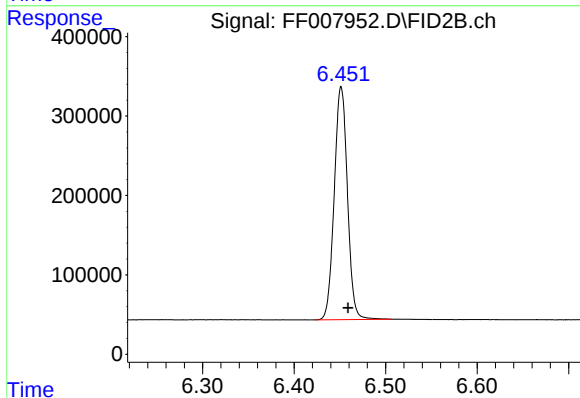


#3 N-DODECANE

R.T.: 6.451 min
Delta R.T.: -0.008 min
Response: 2939328
Conc: 20.41 ug/ml

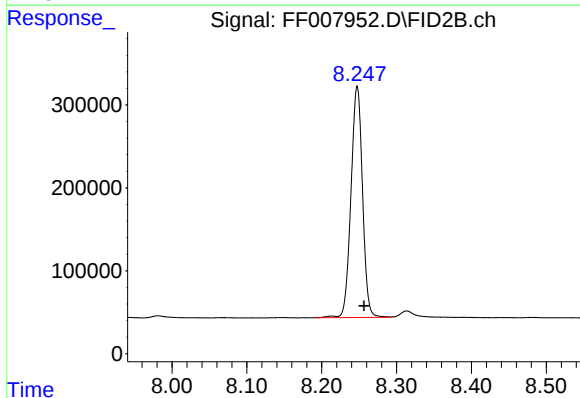


#4 N-TETRADECANE

R.T.: 8.247 min
Delta R.T.: -0.009 min
Response: 2989299
Conc: 20.36 ug/ml

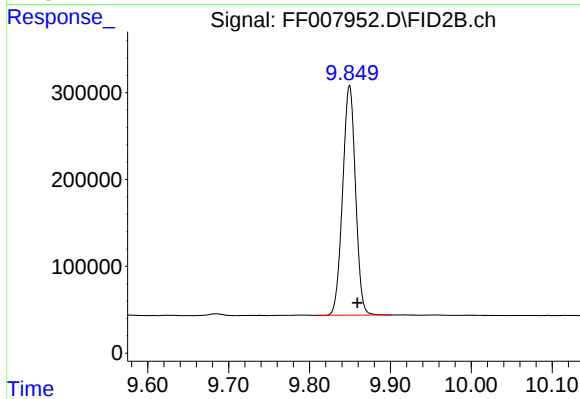

#5 N-HEXADECANE


R.T.: 9.850 min
Delta R.T.: -0.010 min
Response: 2931632
Conc: 19.87 ug/ml

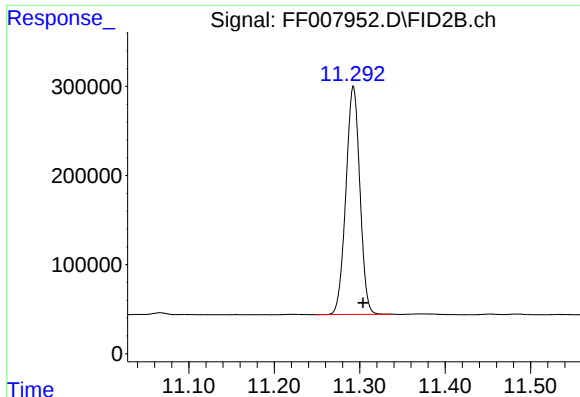

#6 N-OCTADECANE


R.T.: 11.293 min
Delta R.T.: -0.011 min
Response: 2914560
Conc: 19.39 ug/ml

Instrument :
FID_F
ClientSampleId :
KENS-B5-120920-DPMS

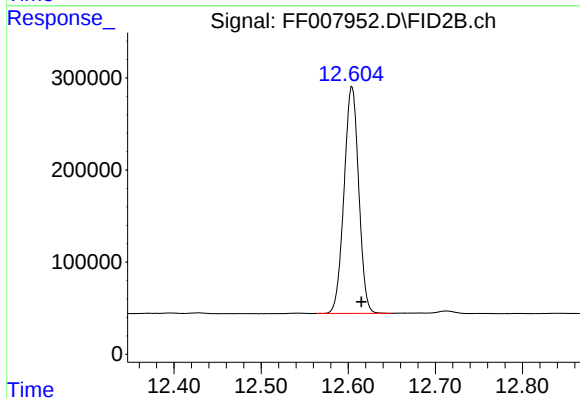


#7 N-EICOSANE

R.T.: 12.604 min
Delta R.T.: -0.011 min
Response: 2887497
Conc: 19.25 ug/ml

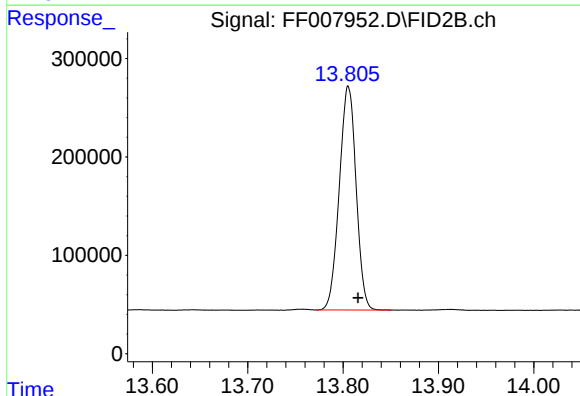


#8 N-DOCOSANE

R.T.: 13.805 min
Delta R.T.: -0.010 min
Response: 2785198
Conc: 19.02 ug/ml

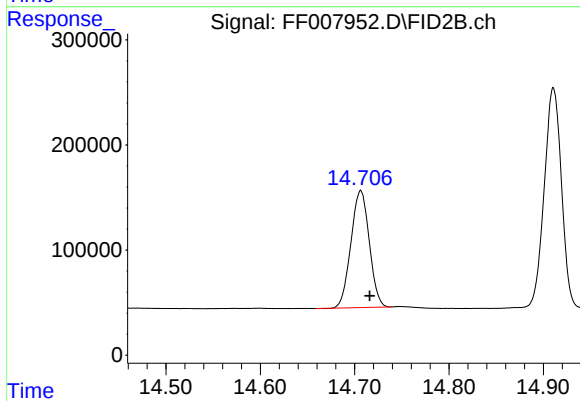

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.706 min
Delta R.T.: -0.010 min
Response: 1504992
Conc: 11.90 ug/ml

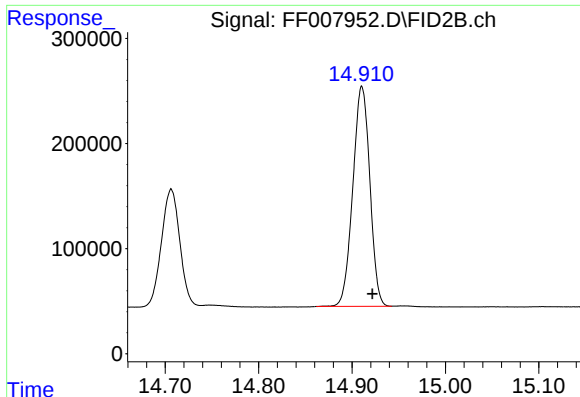

#10 N-TETRACOSANE


R.T.: 14.911 min
Delta R.T.: -0.011 min
Response: 2649323
Conc: 18.19 ug/ml

Instrument :
FID_F
ClientSampleId :
KENS-B5-120920-DPMS

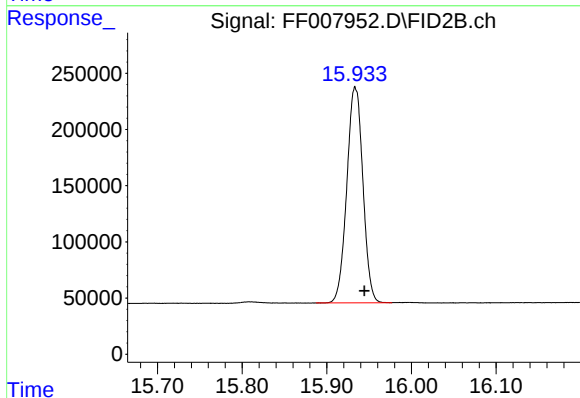

#11 N-HEXACOSANE

R.T.: 15.934 min
Delta R.T.: -0.011 min
Response: 2533809
Conc: 17.98 ug/ml

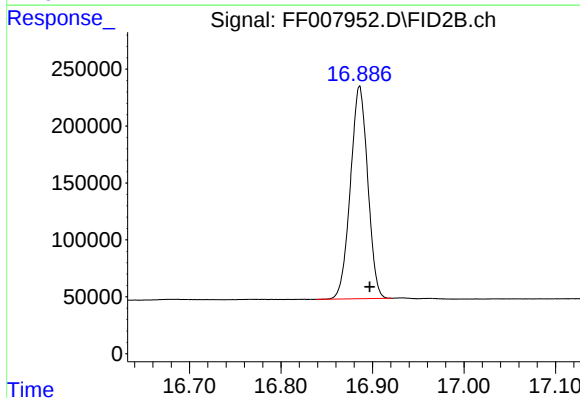

#12 N-OCTACOSANE

R.T.: 16.886 min
Delta R.T.: -0.011 min
Response: 2451463
Conc: 18.11 ug/ml