

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121021\
 Data File : FF009349.D
 Signal(s) : FID2B.ch
 Acq On : 10 Dec 2021 11:00
 Operator : AJ\MA
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 10 23:11:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112321.M
 Quant Title :
 QLast Update : Wed Nov 24 00:27:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.448	3782333	27.208 ug/ml
12)	N-OCTACOSANE	16.853	3073997	24.134 ug/ml
13)	N-TRIACONTANE	17.745	182042	1.487 ug/ml
14)	N-DOTRIACONTANE	18.572	230194	2.004 ug/ml
15)	N-TETRATRIACONTANE	19.357	197214	1.837 ug/ml
16)	N-HEXATRIACONTANE	20.096	103377	1.032 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121021\
Data File : FF009349.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2021 11:00
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 10 23:11:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112321.M
Quant Title :
QLast Update : Wed Nov 24 00:27:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

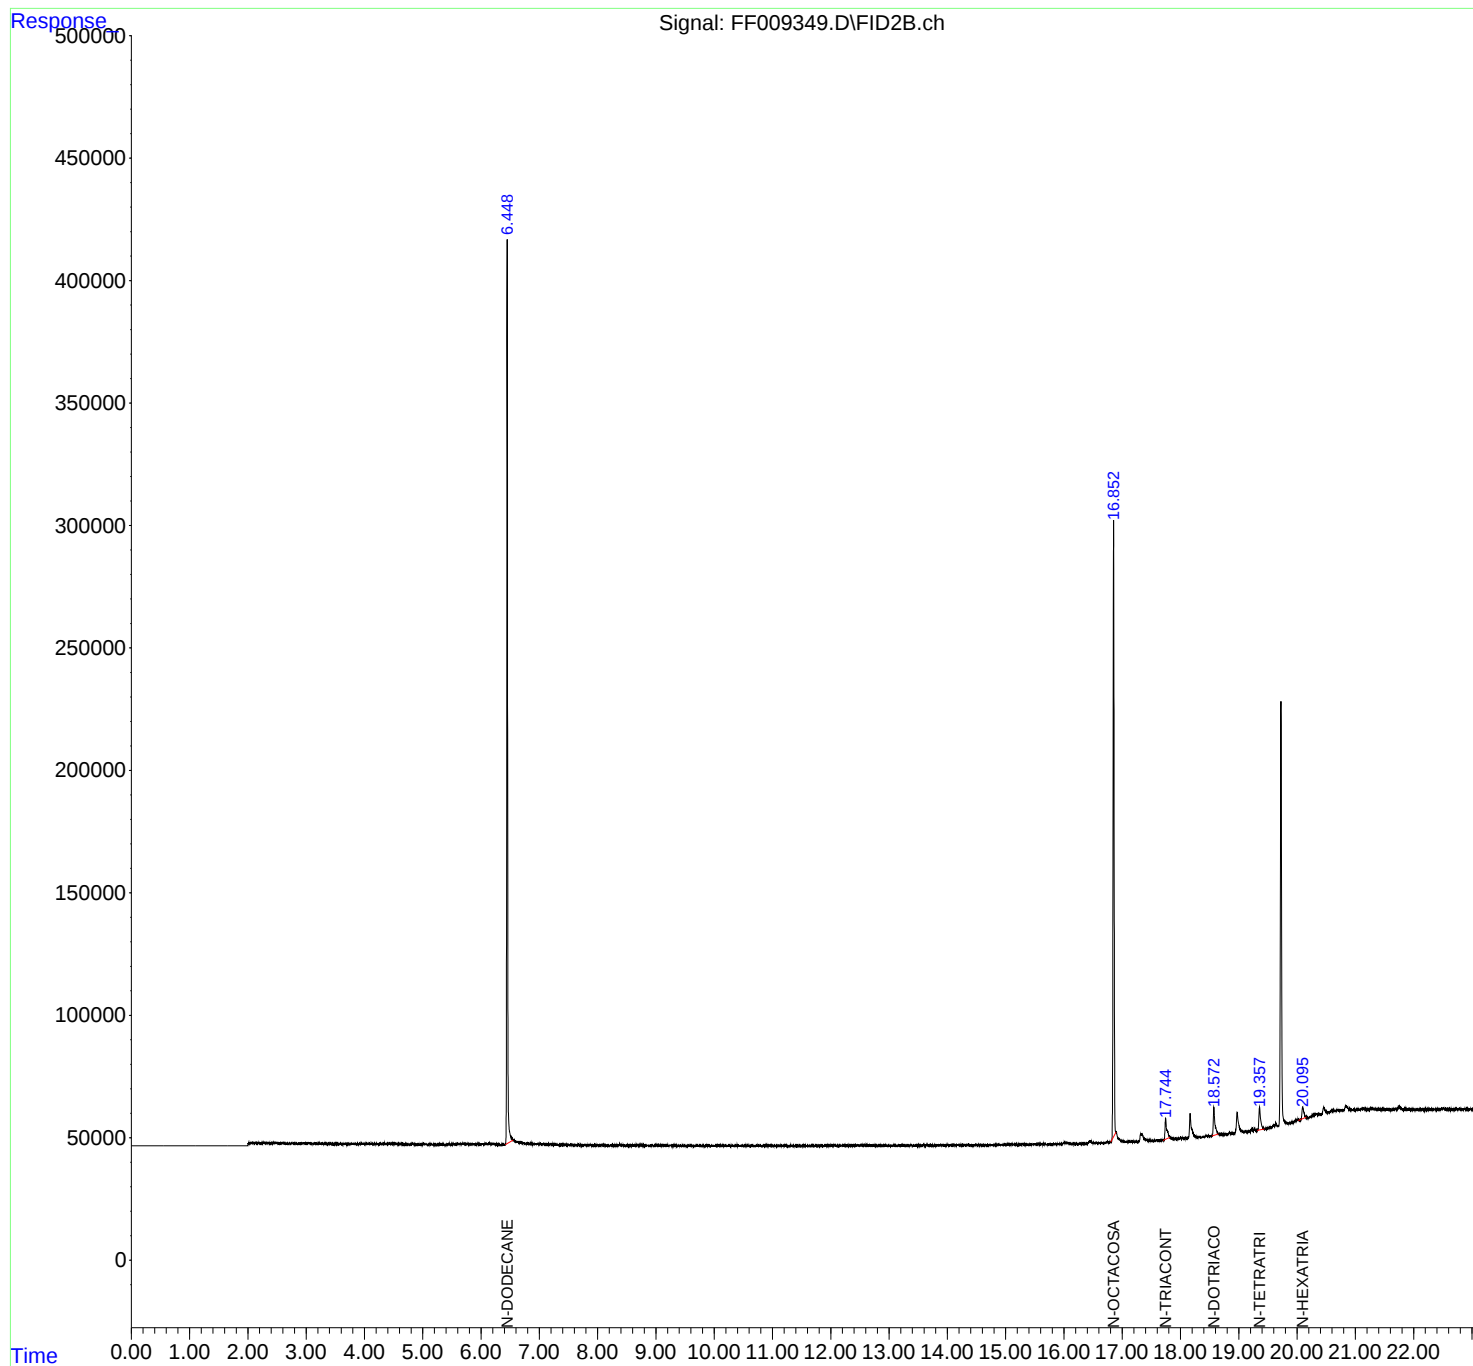


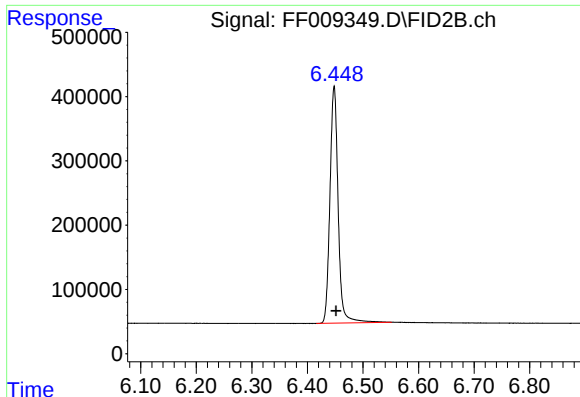

#3 N-DODECANE


R.T.: 6.448 min
Delta R.T.: -0.003 min
Response: 3782333
Conc: 27.21 ug/ml

Instrument :
FID_F
ClientSampleId :

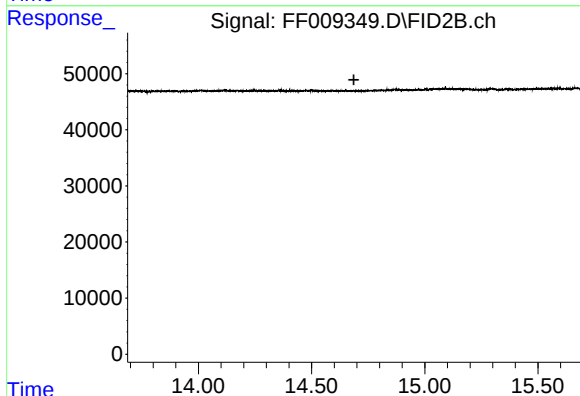


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.687 min
Response: 0
Conc: N.D.

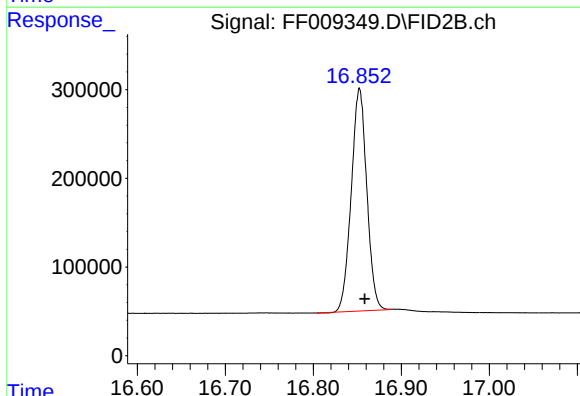


#12 N-OCTACOSANE

R.T.: 16.853 min
Delta R.T.: -0.006 min
Response: 3073997
Conc: 24.13 ug/ml

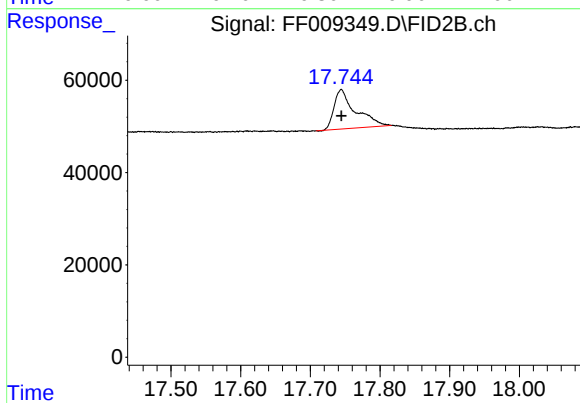

#13 N-TRIACONTANE


R.T.: 17.745 min
Delta R.T.: 0.000 min
Response: 182042
Conc: 1.49 ug/ml

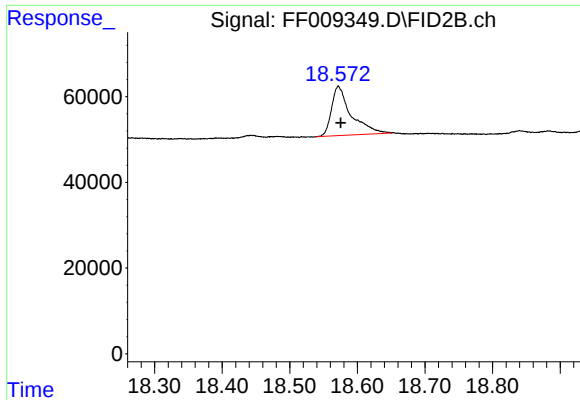

#14 N-DOTRIACONTANE


R.T.: 18.572 min
Delta R.T.: -0.003 min
Response: 230194
Conc: 2.00 ug/ml

Instrument :
FID_F
ClientSampleId :

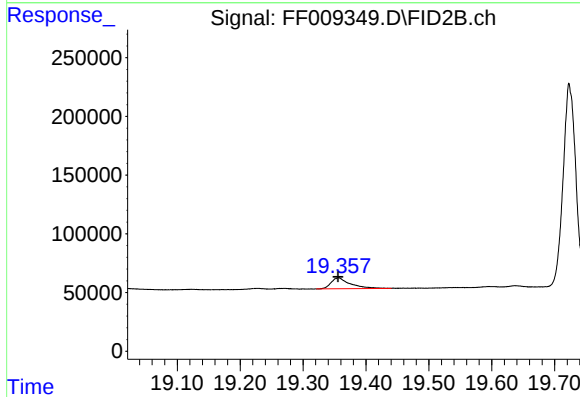

#15 N-TETRATRIACONTANE

R.T.: 19.357 min
Delta R.T.: 0.001 min
Response: 197214
Conc: 1.84 ug/ml

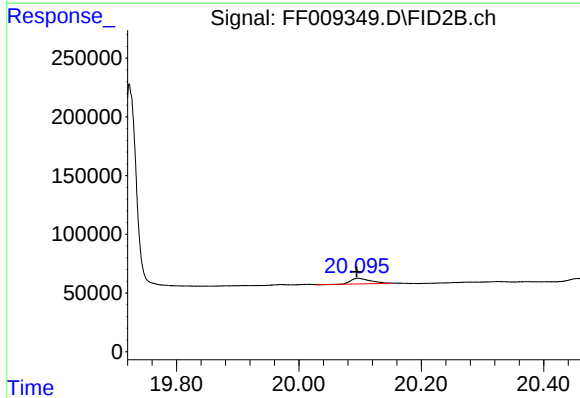

#16 N-HEXATRIACONTANE

R.T.: 20.096 min
Delta R.T.: 0.002 min
Response: 103377
Conc: 1.03 ug/ml