

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121021\
 Data File : FF009358.D
 Signal(s) : FID2B.ch
 Acq On : 10 Dec 2021 20:47
 Operator : AJ\MA
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 10 23:13:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112321.M
 Quant Title :
 QLast Update : Wed Nov 24 00:27:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.446	4919984	35.392 ug/ml
12)	N-OCTACOSANE	16.853	4274666	33.560 ug/ml
13)	N-TRIACONTANE	17.735	427351	3.491 ug/ml
14)	N-DOTRIACONTANE	18.567	504202	4.390 ug/ml
15)	N-TETRATRIACONTANE	19.349	401389	3.738 ug/ml
16)	N-HEXATRIACONTANE	20.086	272484	2.720 ug/ml
17)	N-OCTATRIACONTANE	20.819	149867	1.622 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121021\
Data File : FF009358.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2021 20:47
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 10 23:13:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112321.M
Quant Title :
QLast Update : Wed Nov 24 00:27:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

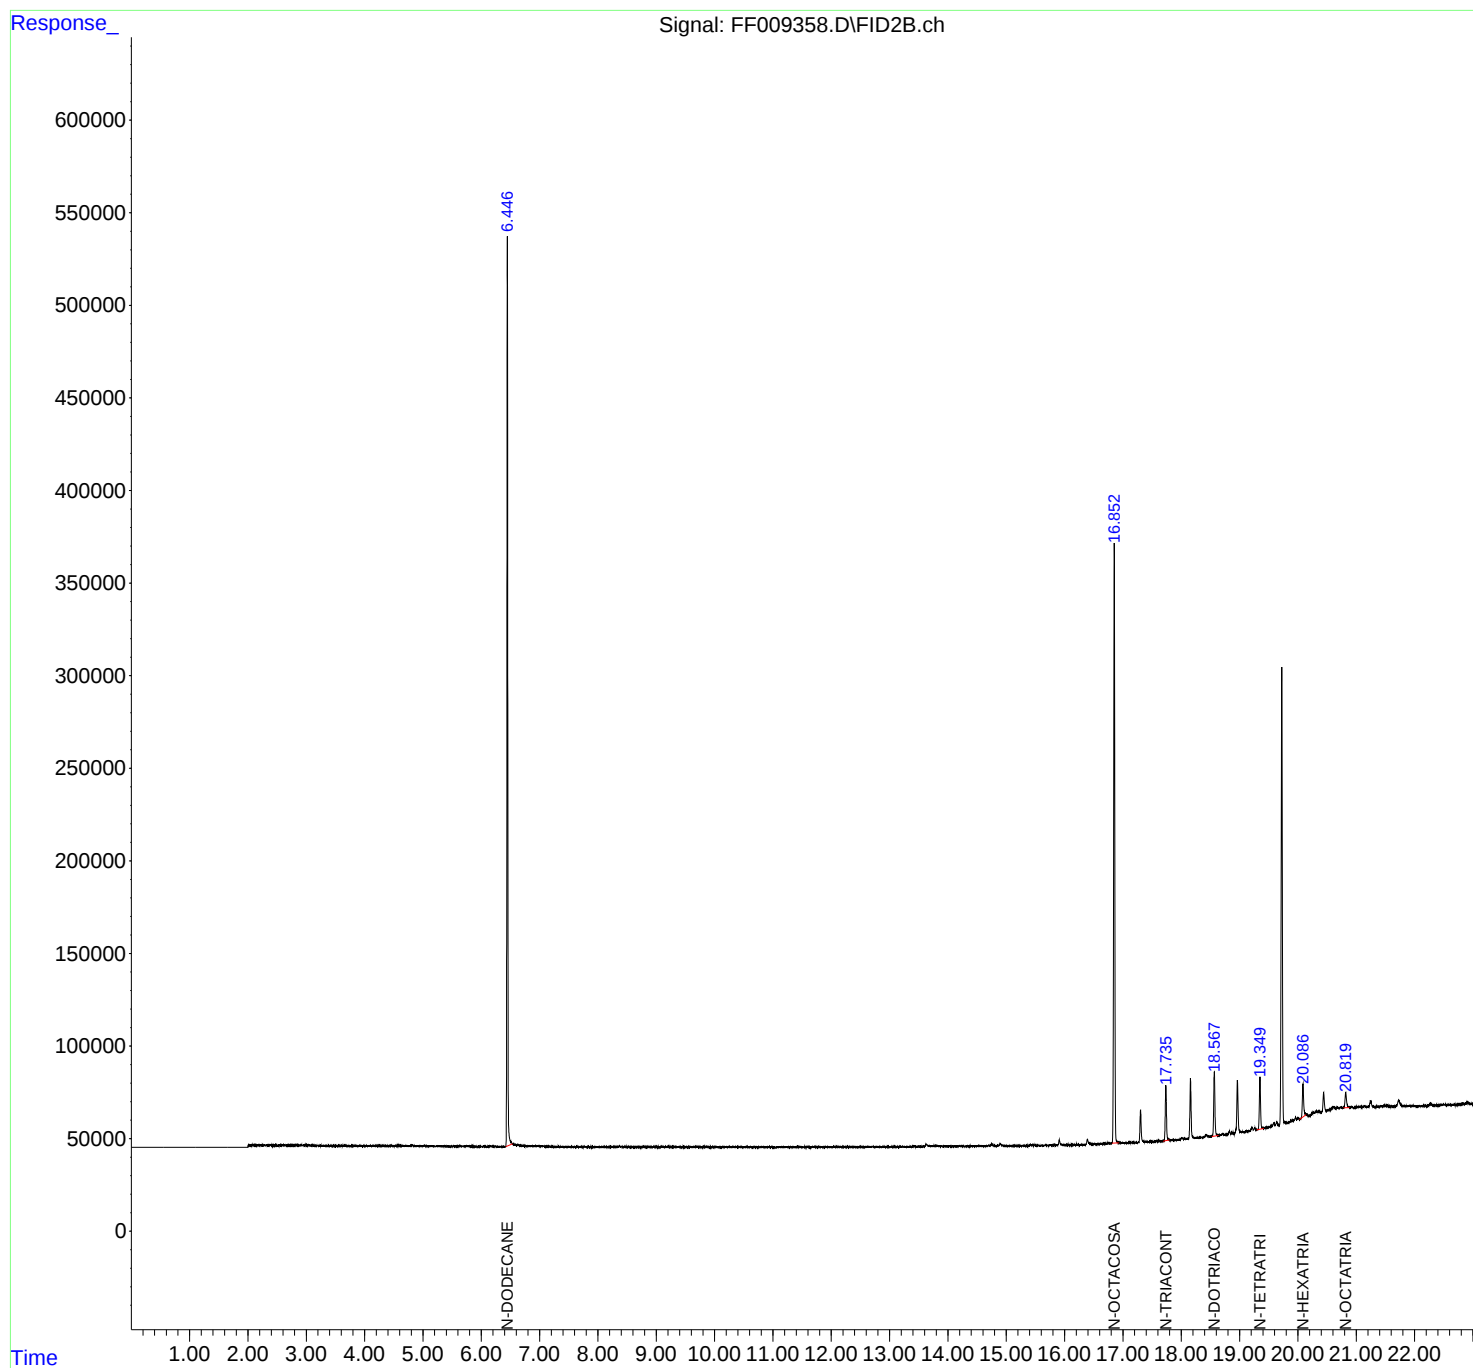


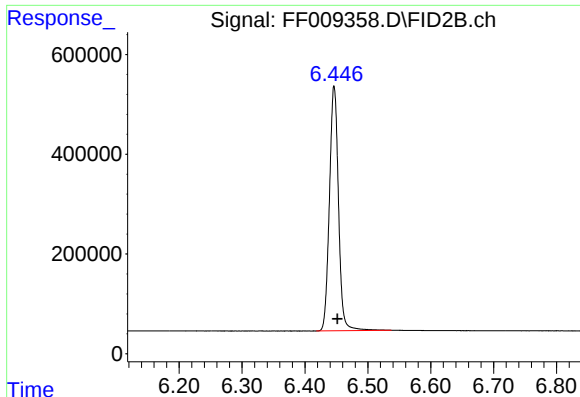

#3 N-DODECANE


R.T.: 6.446 min
Delta R.T.: -0.006 min
Response: 4919984
Conc: 35.39 ug/ml

Instrument :
FID_F
ClientSampleId :

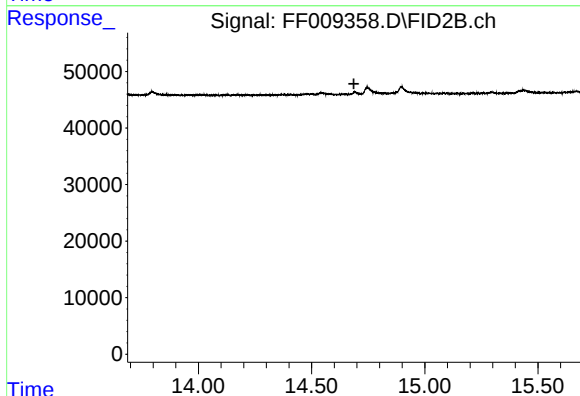


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.687 min
Response: 0
Conc: N.D.

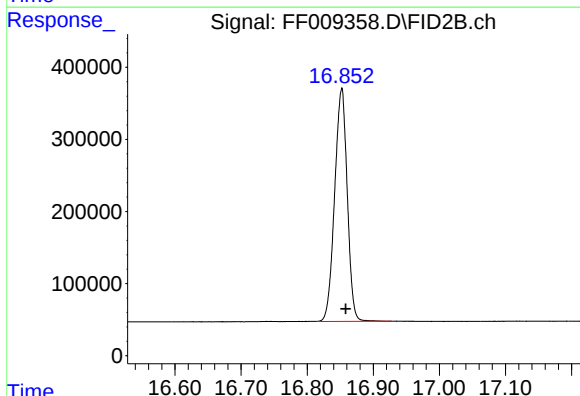


#12 N-OCTACOSANE

R.T.: 16.853 min
Delta R.T.: -0.006 min
Response: 4274666
Conc: 33.56 ug/ml

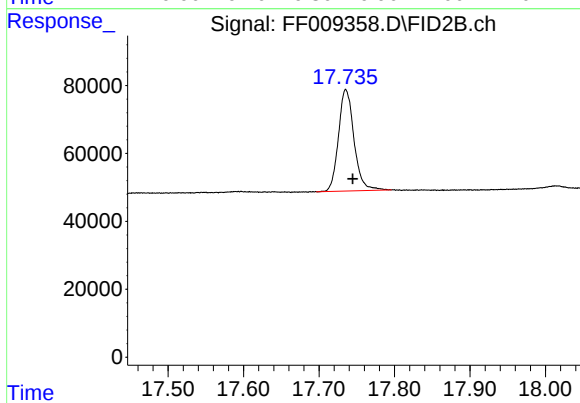

#13 N-TRIACONTANE


R.T.: 17.735 min
Delta R.T.: -0.009 min
Response: 427351
Conc: 3.49 ug/ml

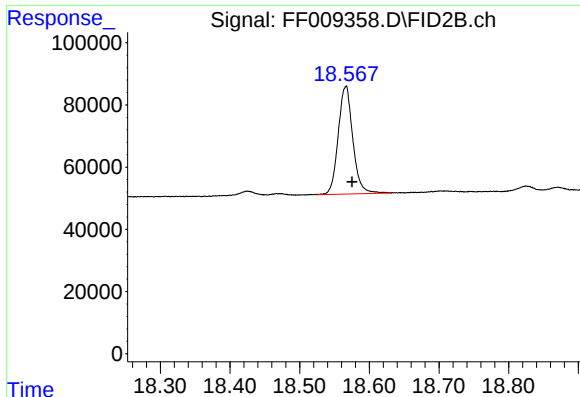

#14 N-DOTRIACONTANE


R.T.: 18.567 min
Delta R.T.: -0.008 min
Response: 504202
Conc: 4.39 ug/ml

Instrument :
FID_F
ClientSampleId :

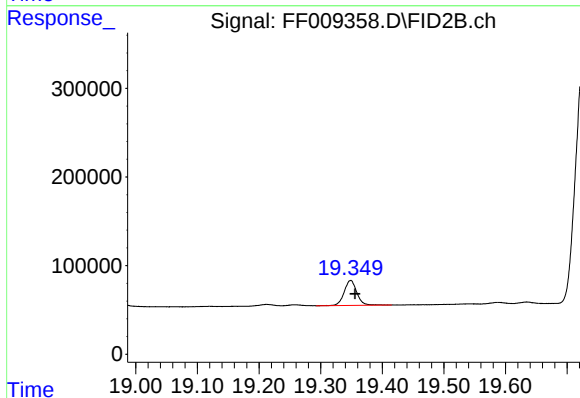


#15 N-TETRATRIACONTANE

R.T.: 19.349 min
Delta R.T.: -0.007 min
Response: 401389
Conc: 3.74 ug/ml

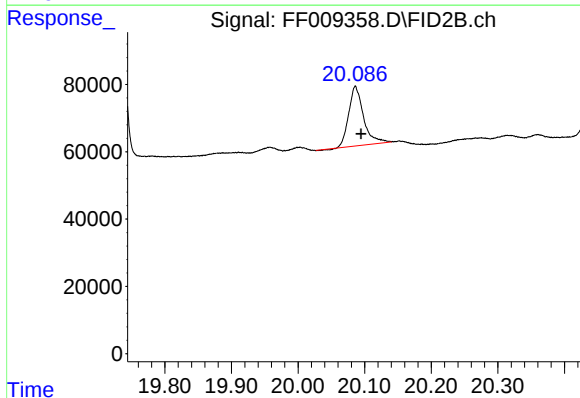

#16 N-HEXATRIACONTANE

R.T.: 20.086 min
Delta R.T.: -0.008 min
Response: 272484
Conc: 2.72 ug/ml

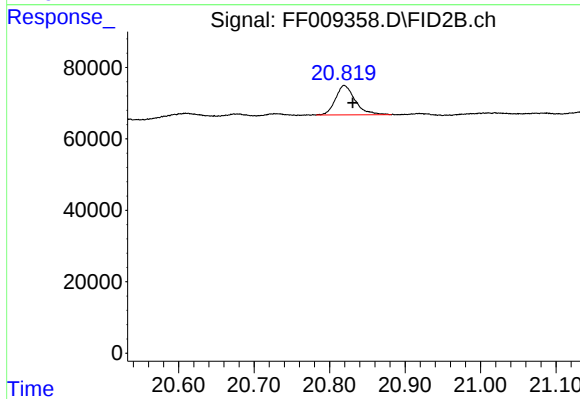

#17 N-OCTATRIACONTANE

R.T.: 20.819 min
Delta R.T.: -0.011 min
Response: 149867
Conc: 1.62 ug/ml