

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121021\
 Data File : FF009360.D
 Signal(s) : FID2B.ch
 Acq On : 10 Dec 2021 21:49
 Operator : AJ\MA
 Sample : M4992-06
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 10 23:14:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112321.M
 Quant Title :
 QLast Update : Wed Nov 24 00:27:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.679	2293437	18.984 ug/ml
Target Compounds			
2) N-DECANE	4.410	46170	0.337 ug/ml
3) N-DODECANE	6.453	306391	2.204 ug/ml
4) N-TETRADECANE	8.285	197457	1.389 ug/ml
5) N-HEXADECANE	9.832	73051	0.517 ug/ml
6) N-OCTADECANE	11.292	695920	4.869 ug/ml
7) N-EICOSANE	12.631	498941	3.505 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121021\
Data File : FF009360.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2021 21:49
Operator : AJ\MA
Sample : M4992-06
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 10 23:14:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112321.M
Quant Title :
QLast Update : Wed Nov 24 00:27:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

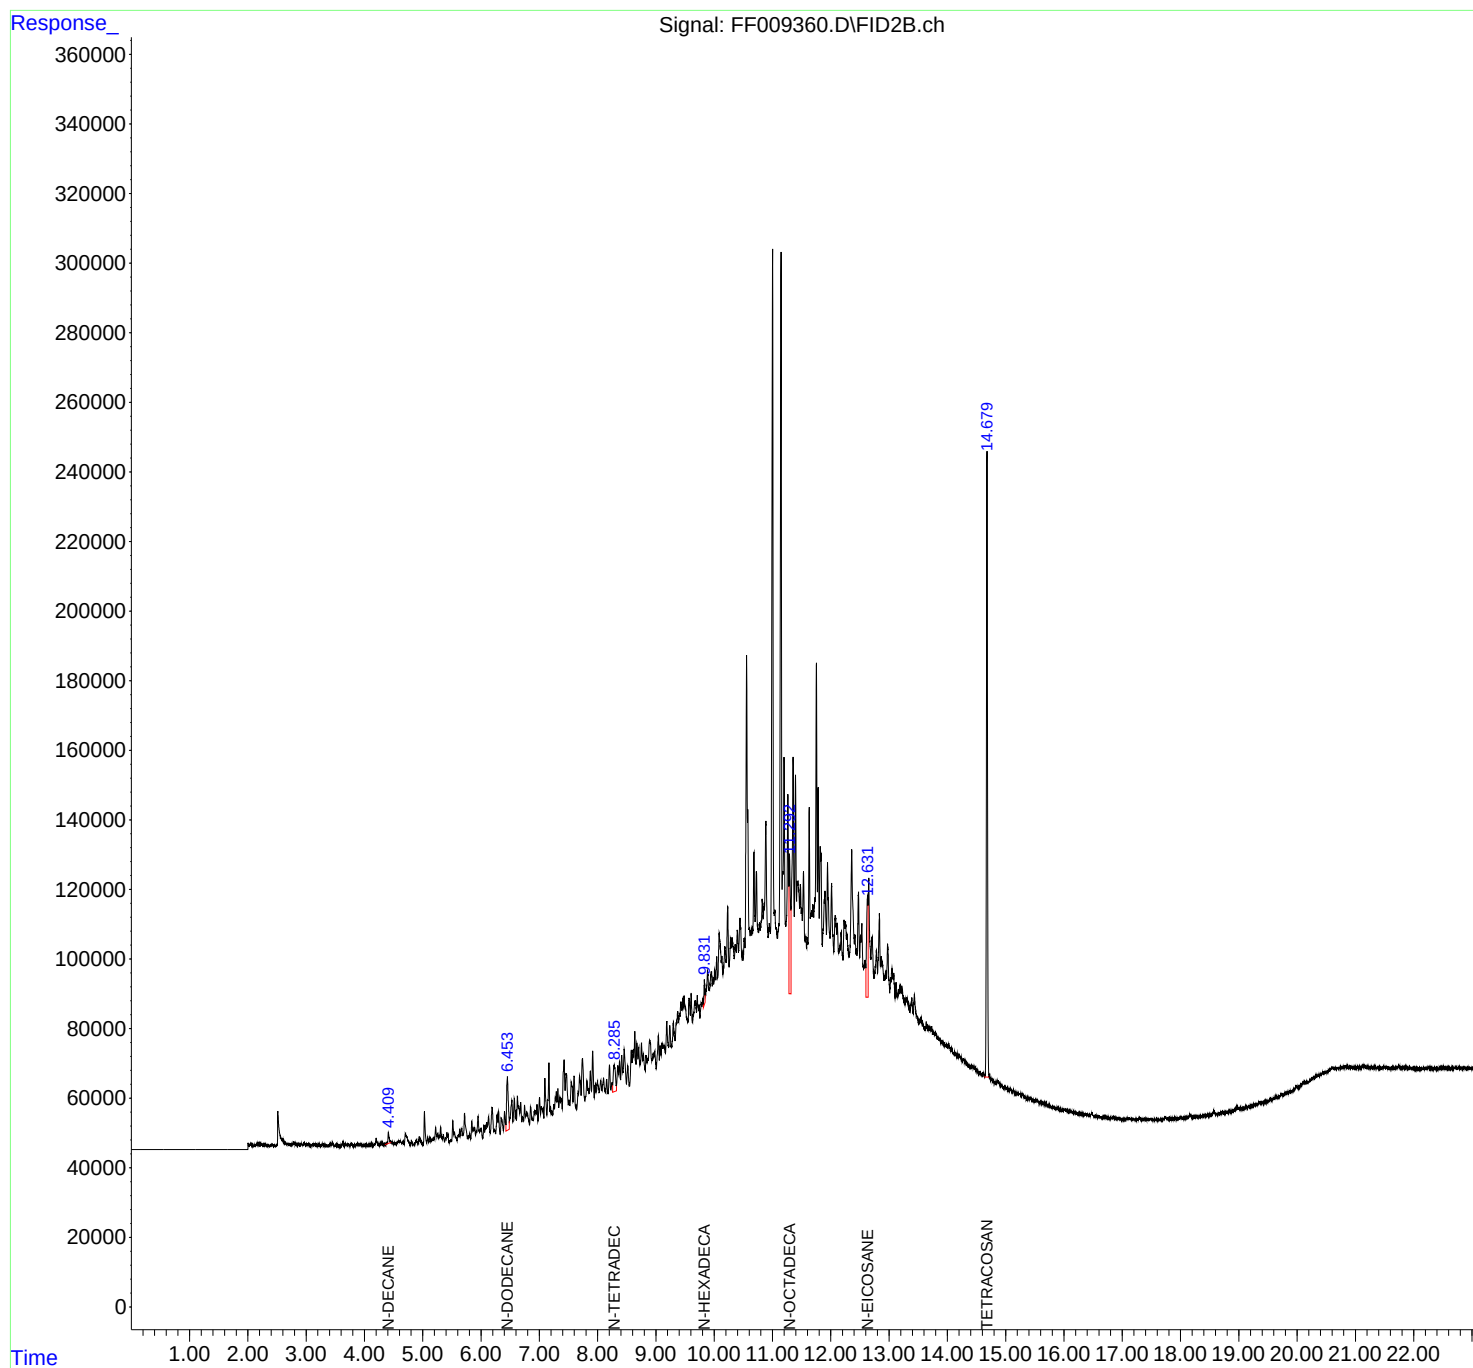


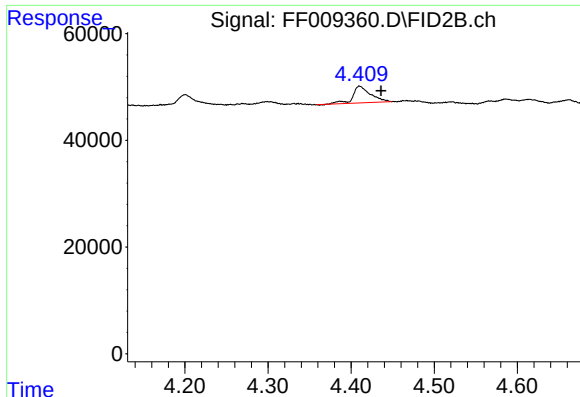

#2 N-DECANE


R.T.: 4.410 min
Delta R.T.: -0.026 min
Response: 46170
Conc: 0.34 ug/ml

Instrument :
FID_F
ClientSampleId :

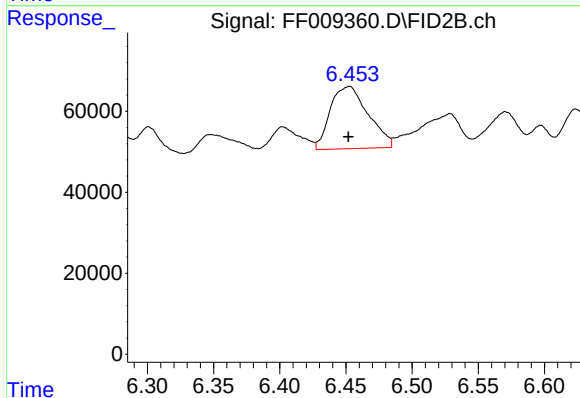


#3 N-DODECANE

R.T.: 6.453 min
Delta R.T.: 0.001 min
Response: 306391
Conc: 2.20 ug/ml

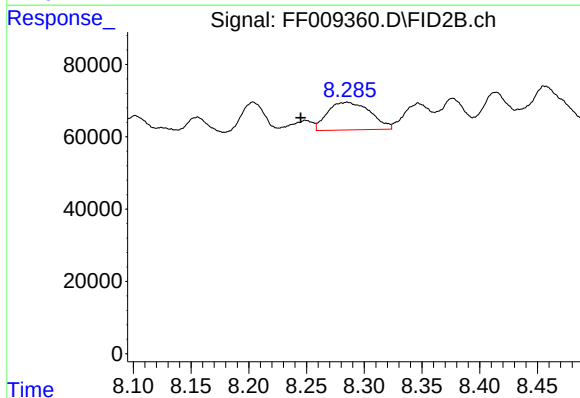


#4 N-TETRADECANE

R.T.: 8.285 min
Delta R.T.: 0.040 min
Response: 197457
Conc: 1.39 ug/ml

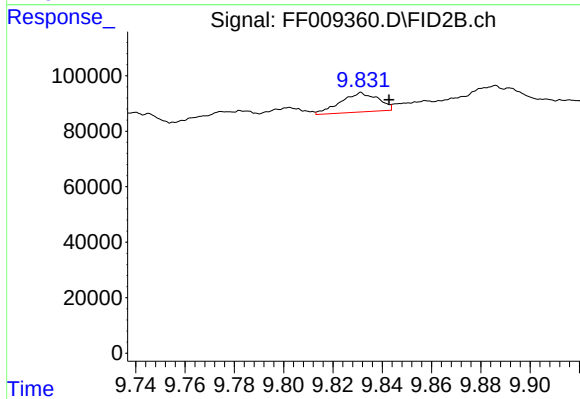

#5 N-HEXADECANE


R.T.: 9.832 min
Delta R.T.: -0.011 min
Response: 73051
Conc: 0.52 ug/ml

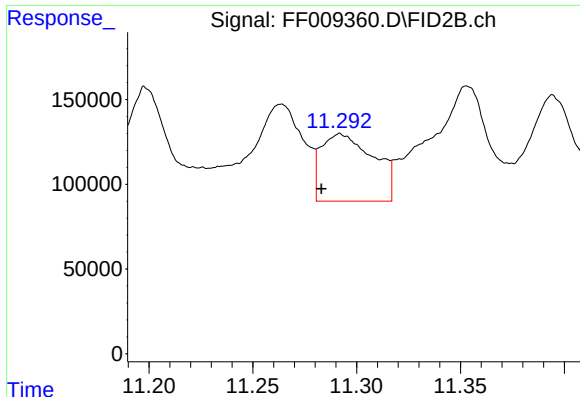

#6 N-OCTADECANE


R.T.: 11.292 min
Delta R.T.: 0.009 min
Response: 695920
Conc: 4.87 ug/ml

Instrument :
FID_F
ClientSampleId :

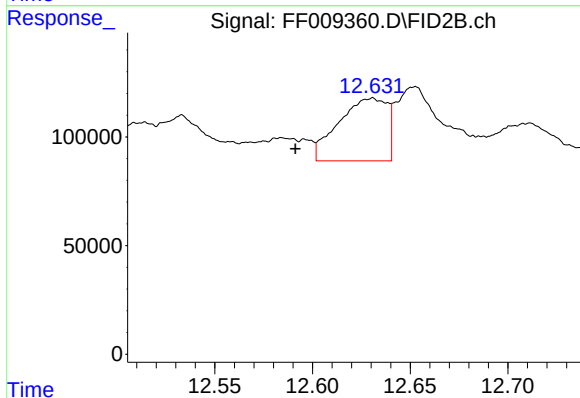

#7 N-EICOSANE

R.T.: 12.631 min
Delta R.T.: 0.040 min
Response: 498941
Conc: 3.50 ug/ml

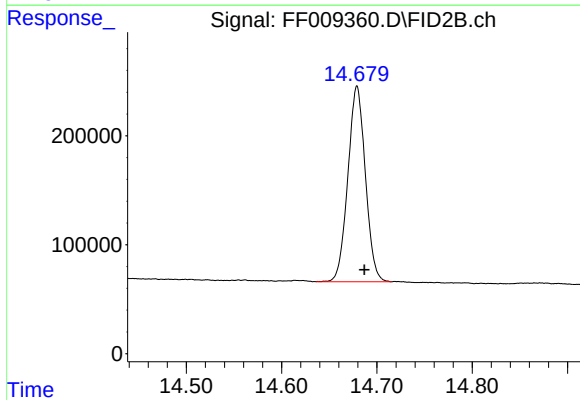

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.679 min
Delta R.T.: -0.008 min
Response: 2293437
Conc: 18.98 ug/ml