

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121021\
 Data File : FF009365.D
 Signal(s) : FID2B.ch
 Acq On : 11 Dec 2021 00:22
 Operator : AJ\MA
 Sample : M4992-11
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 11 02:34:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112321.M
 Quant Title :
 QLast Update : Wed Nov 24 00:27:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.680	2587390	21.417 ug/ml
Target Compounds			
3) N-DODECANE	6.454	201822	1.452 ug/ml
4) N-TETRADECANE	8.245	123347	0.868 ug/ml
5) N-HEXADECANE	9.845	139224	0.986 ug/ml
6) N-OCTADECANE	11.288	284227	1.989 ug/ml
7) N-EICOSANE	12.595	40478	0.284 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121021\
Data File : FF009365.D
Signal(s) : FID2B.ch
Acq On : 11 Dec 2021 00:22
Operator : AJ\MA
Sample : M4992-11
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 11 02:34:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112321.M
Quant Title :
QLast Update : Wed Nov 24 00:27:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

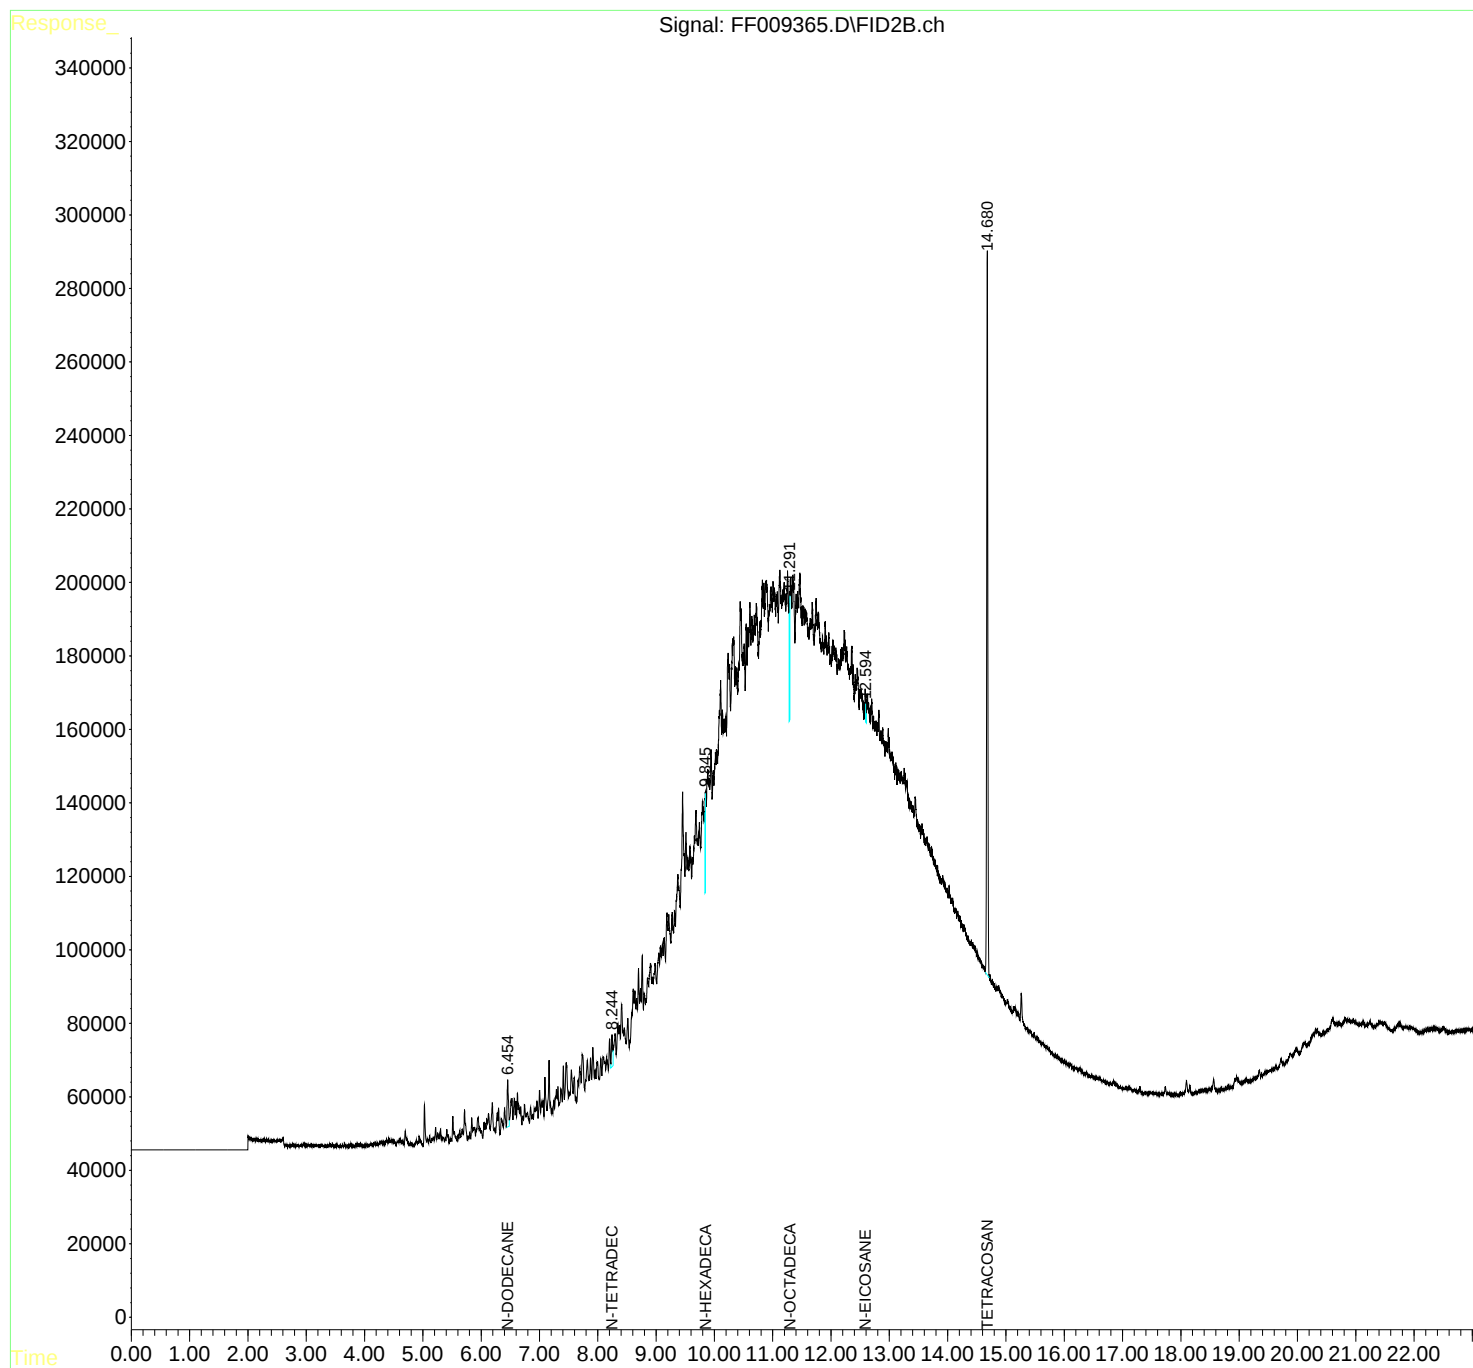


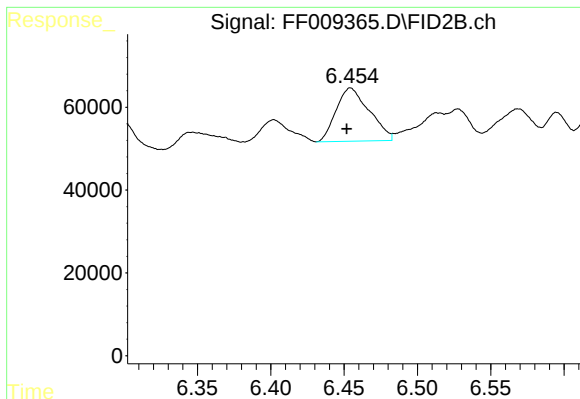

#3 N-DODECANE


R.T.: 6.454 min
Delta R.T.: 0.003 min
Response: 201822
Conc: 1.45 ug/ml

Instrument :
FID_F
ClientSampleId :

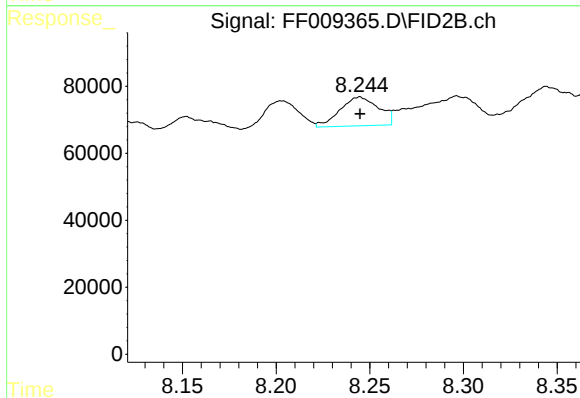


#4 N-TETRADECANE

R.T.: 8.245 min
Delta R.T.: 0.000 min
Response: 123347
Conc: 0.87 ug/ml

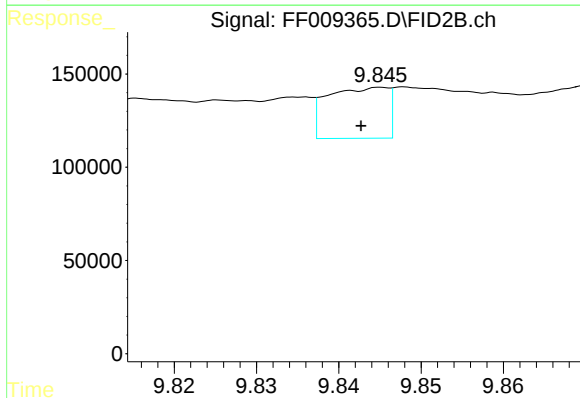


#5 N-HEXADECANE

R.T.: 9.845 min
Delta R.T.: 0.003 min
Response: 139224
Conc: 0.99 ug/ml

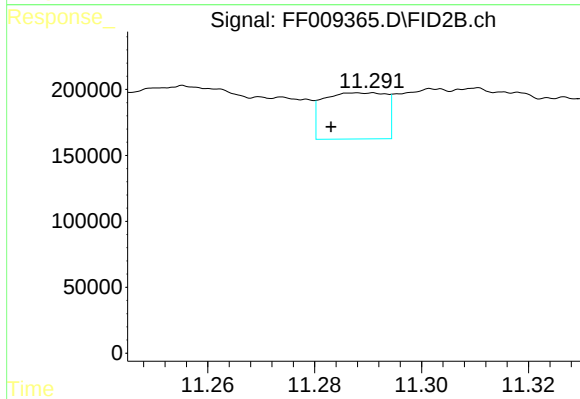

#6 N-OCTADECANE


R.T.: 11.288 min
Delta R.T.: 0.005 min
Response: 284227
Conc: 1.99 ug/ml

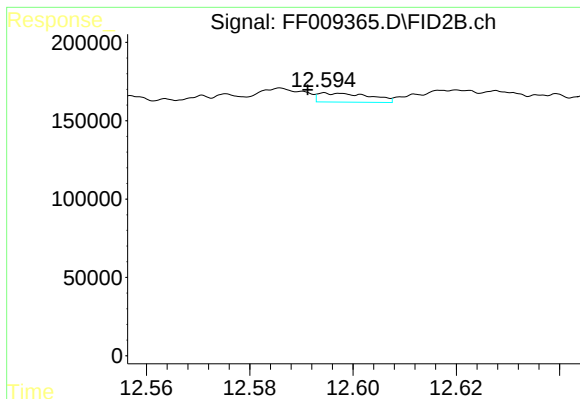

#7 N-EICOSANE

R.T.: 12.595 min
Delta R.T.: 0.003 min
Response: 40478
Conc: 0.28 ug/ml

Instrument :
FID_F
ClientSampleId :

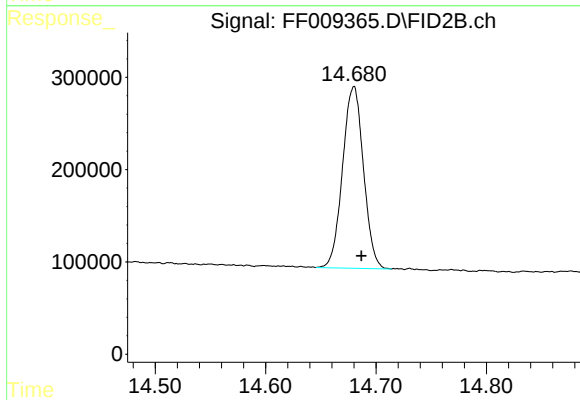

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.680 min
Delta R.T.: -0.006 min
Response: 2587390
Conc: 21.42 ug/ml