

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121021\
Data File : FF009355.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2021 19:16
Operator : AJ\MA
Sample : M4992-04
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SIMW-02-20211208-A

Integration File: autoint1.e
Quant Time: Dec 10 23:12:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112321.M
Quant Title :
QLast Update : Wed Nov 24 00:27:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.678	2514589	20.815 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121021\
Data File : FF009355.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2021 19:16
Operator : AJ\MA
Sample : M4992-04
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SIMW-02-20211208-A

Integration File: autoint1.e
Quant Time: Dec 10 23:12:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112321.M
Quant Title :
QLast Update : Wed Nov 24 00:27:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

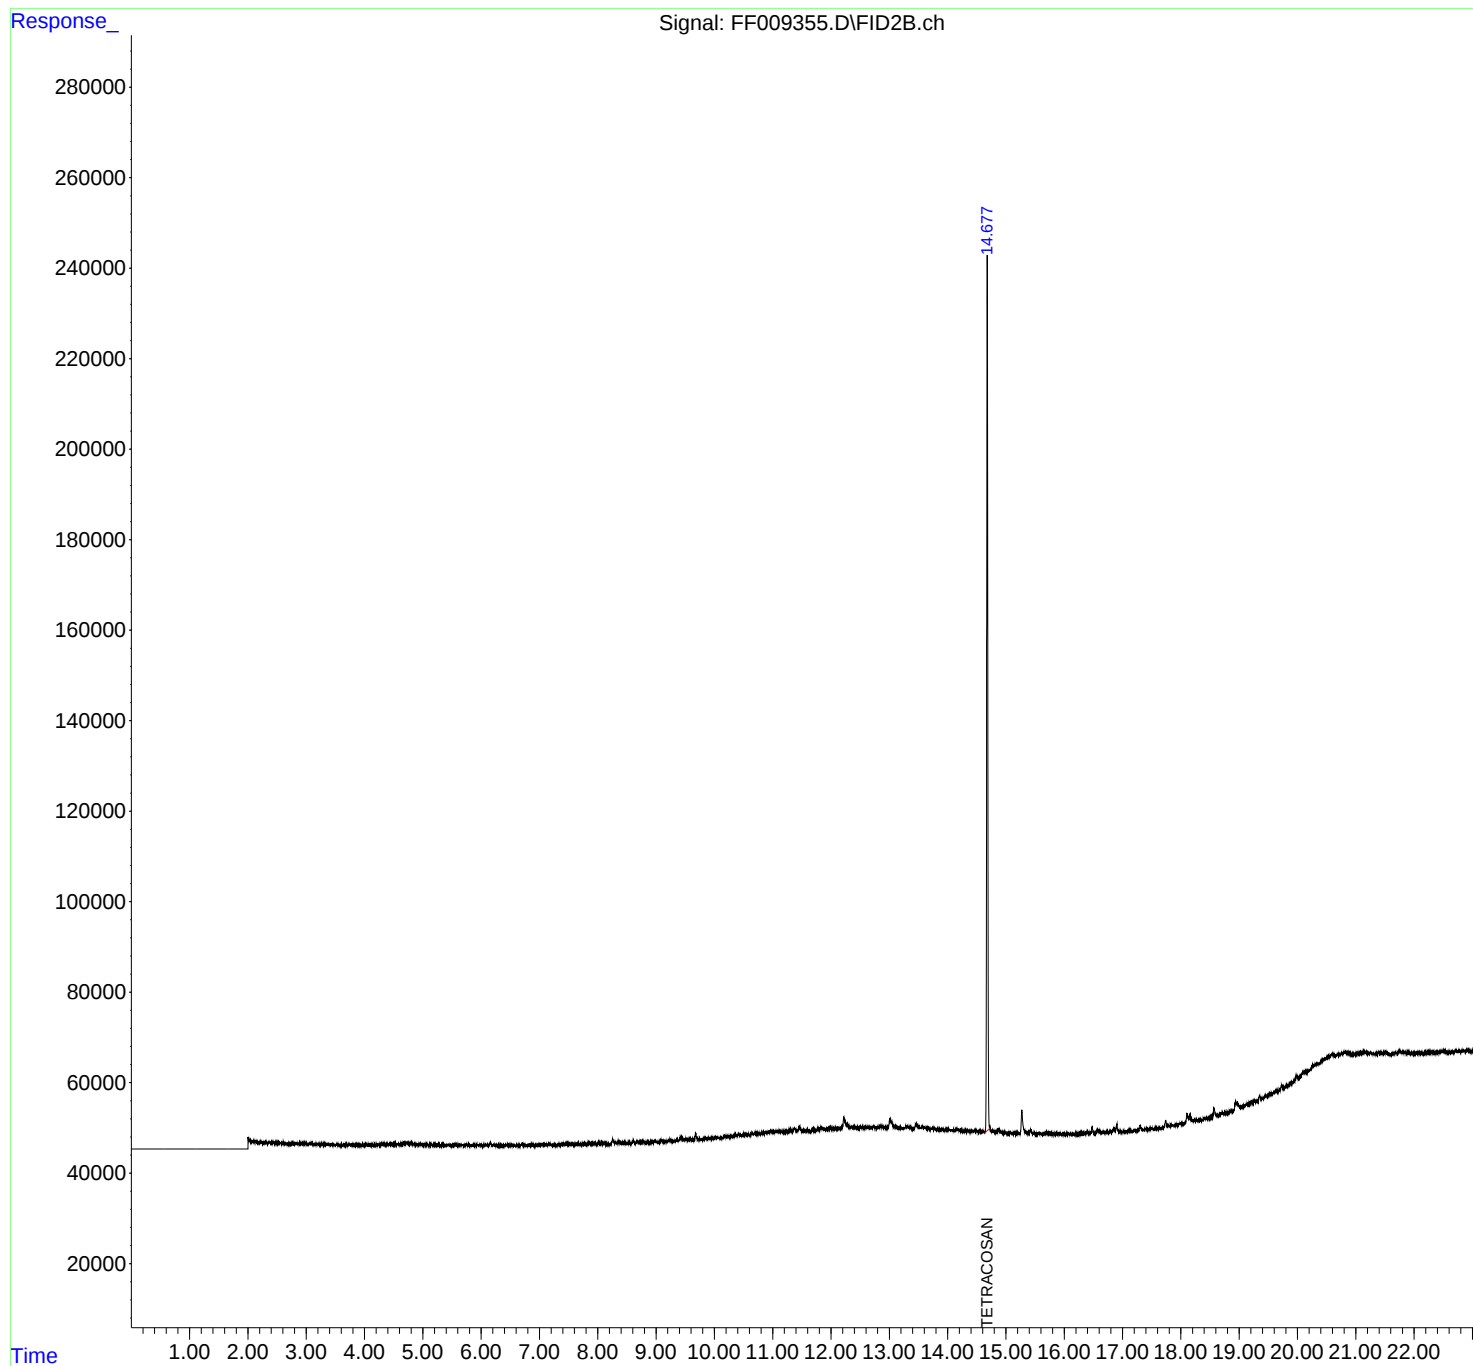

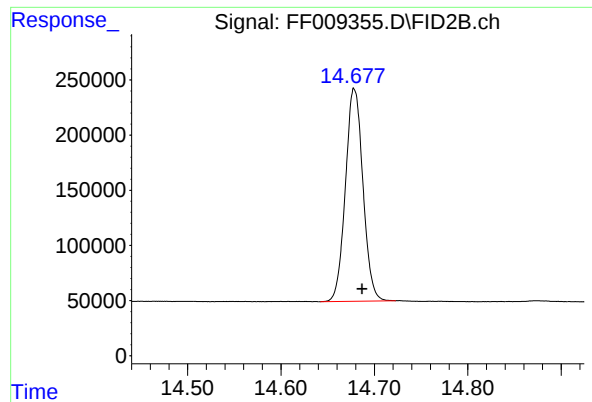

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.678 min
Delta R.T.: -0.009 min
Response: 2514589
Conc: 20.81 ug/ml

Instrument :
FID_F
ClientSampleId :
SIMW-02-20211208-A