

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121021\
Data File : FF009358.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2021 20:47
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Dec 10 23:13:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112321.M
Quant Title :
QLast Update : Wed Nov 24 00:27:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.446	4919984	35.392 ug/ml
12) N-OCTACOSANE	16.853	4274666	33.560 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121021\
Data File : FF009358.D
Signal(s) : FID2B.ch
Acq On : 10 Dec 2021 20:47
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Dec 10 23:13:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112321.M
Quant Title :
QLast Update : Wed Nov 24 00:27:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

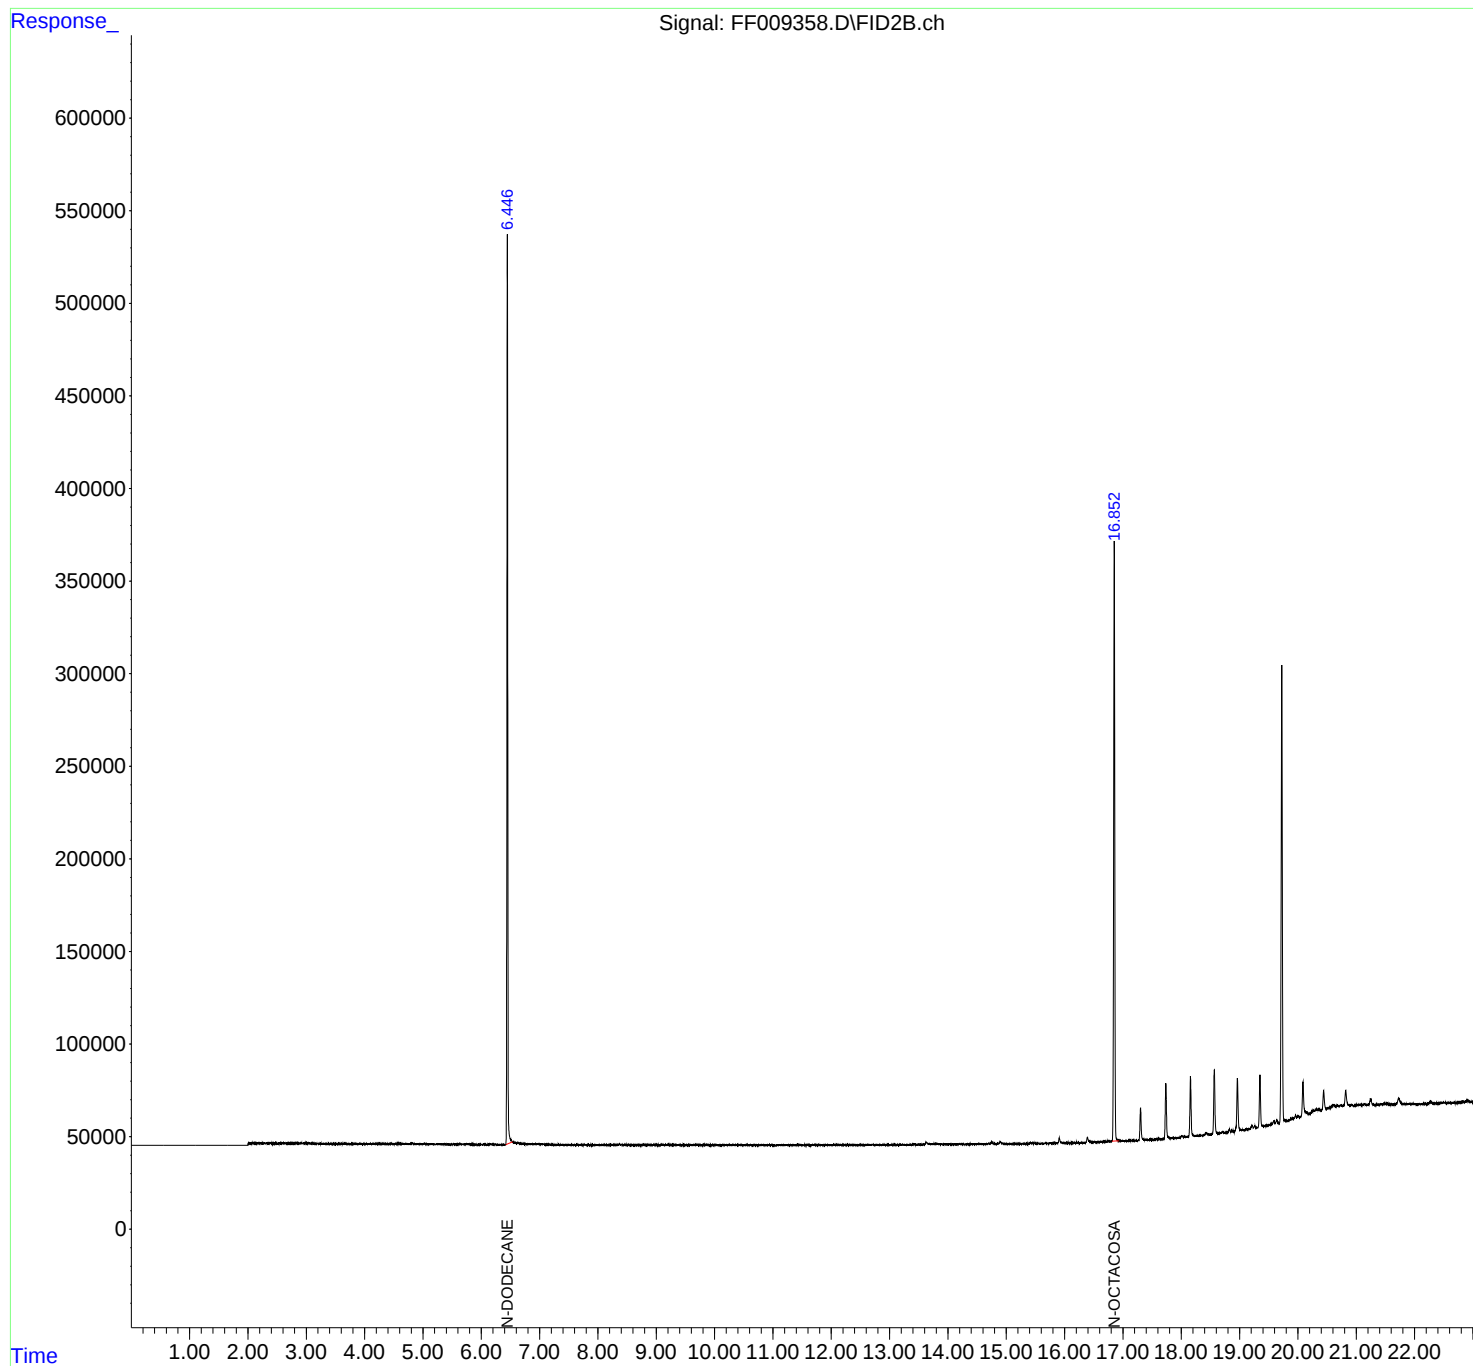


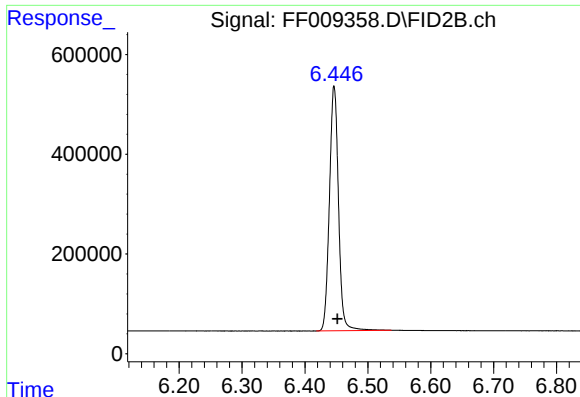

#3 N-DODECANE


R.T.: 6.446 min
Delta R.T.: -0.006 min
Response: 4919984
Conc: 35.39 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

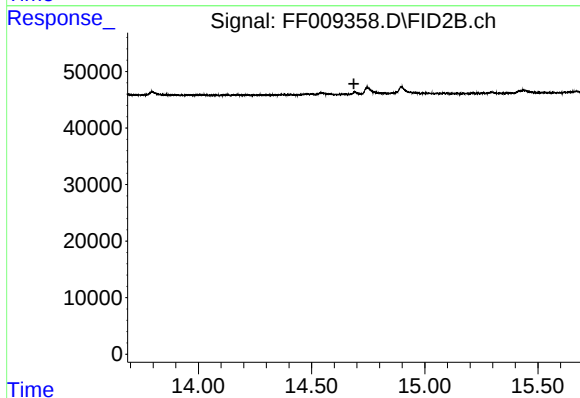

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.687 min
Response: 0
Conc: N.D.

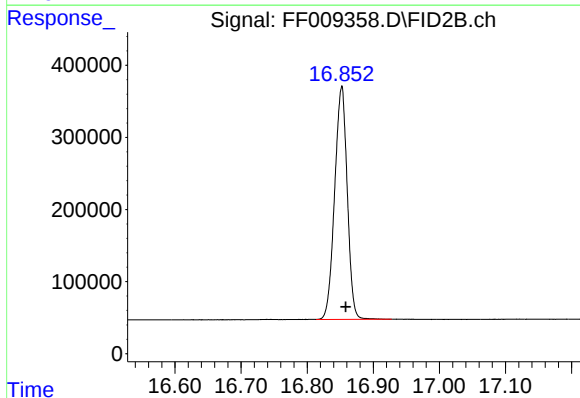

#12 N-OCTACOSANE

R.T.: 16.853 min
Delta R.T.: -0.006 min
Response: 4274666
Conc: 33.56 ug/ml