

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121118\
 Data File : FF002988.D
 Signal(s) : FID2B.ch
 Acq On : 11 Dec 2018 17:19
 Operator : AJ\SJ
 Sample : J6196-03 10X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 12 02:52:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.641	148016	1.140 ug/ml
Target Compounds			
5) N-HEXADECANE	9.781	84997	0.531 ug/ml
6) N-OCTADECANE	11.225	78475	0.495 ug/ml
7) N-EICOSANE	12.589	87018	0.564 ug/ml
10) N-TETRACOSANE	14.822	246873	1.708 ug/ml
11) N-HEXACOSANE	15.872	87856	0.629 ug/ml
12) N-OCTACOSANE	16.822	106115	0.792 ug/ml
13) N-TRIACONTANE	17.714	211355	1.649 ug/ml
14) N-DOTRIACONTANE	18.551	287660	2.409 ug/ml
15) N-TETRATRIACONTANE	19.341	53080	0.468 ug/ml
16) N-HEXATRIACONTANE	20.094	132516	1.228 ug/ml
18) N-TETRACONTANE	21.750	72564	0.690 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121118\
Data File : FF002988.D
Signal(s) : FID2B.ch
Acq On : 11 Dec 2018 17:19
Operator : AJ\SJ
Sample : J6196-03 10X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 12 02:52:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

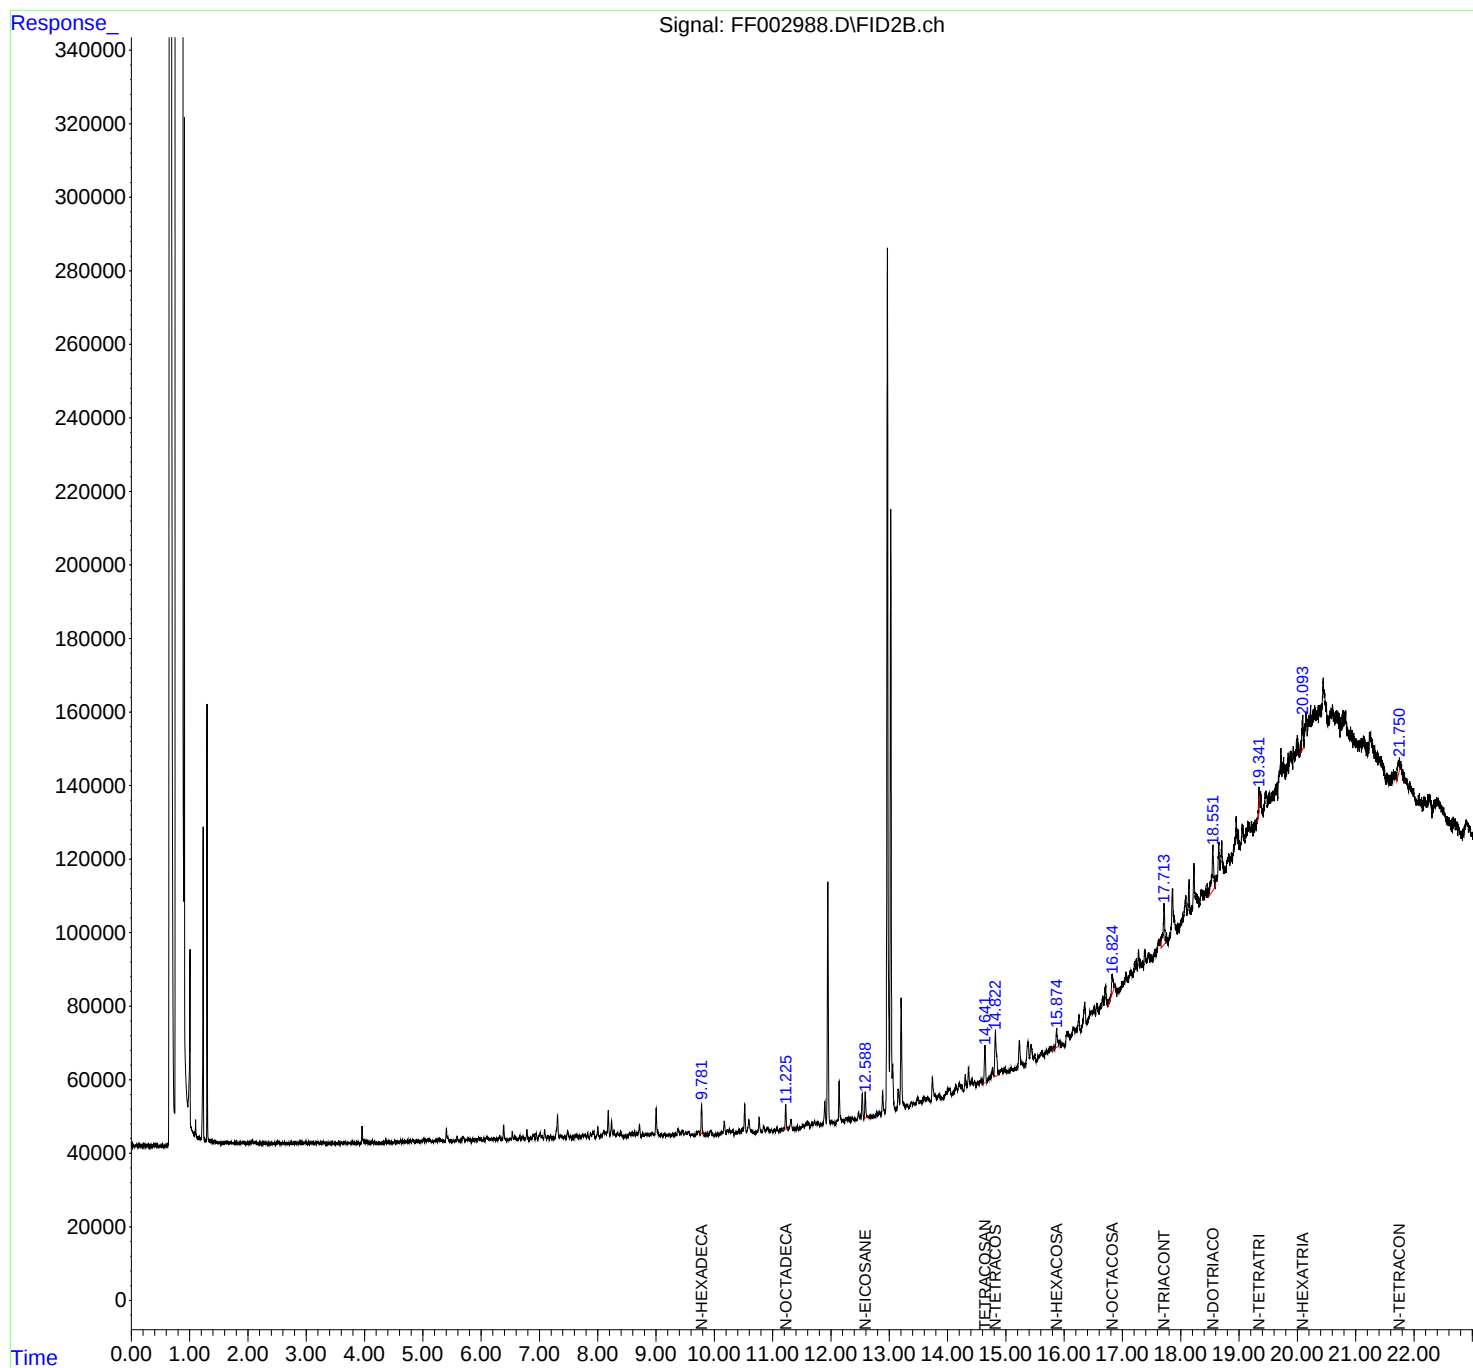

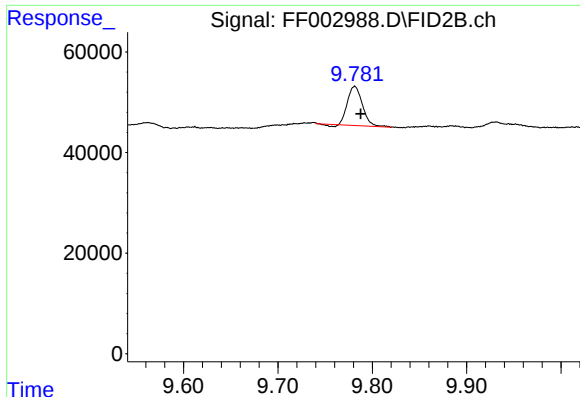


#5 N-HEXADECANE

R.T.: 9.781 min
Delta R.T.: -0.006 min
Response: 84997
Conc: 0.53 ug/ml

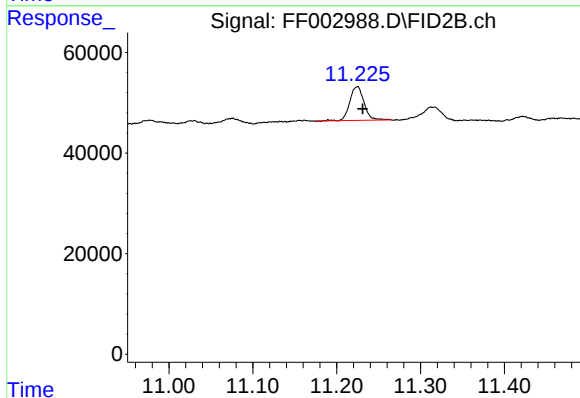


#6 N-OCTADECANE

R.T.: 11.225 min
Delta R.T.: -0.007 min
Response: 78475
Conc: 0.50 ug/ml

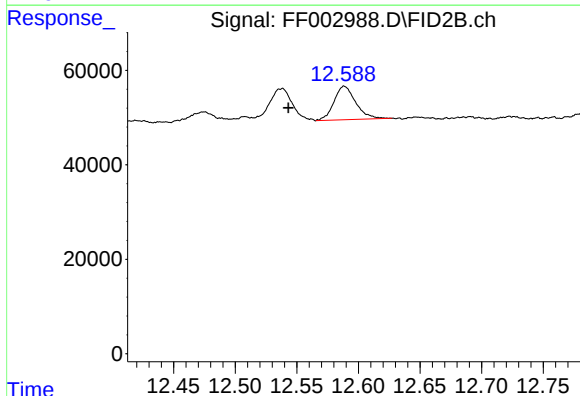


#7 N-EICOSANE

R.T.: 12.589 min
Delta R.T.: 0.045 min
Response: 87018
Conc: 0.56 ug/ml

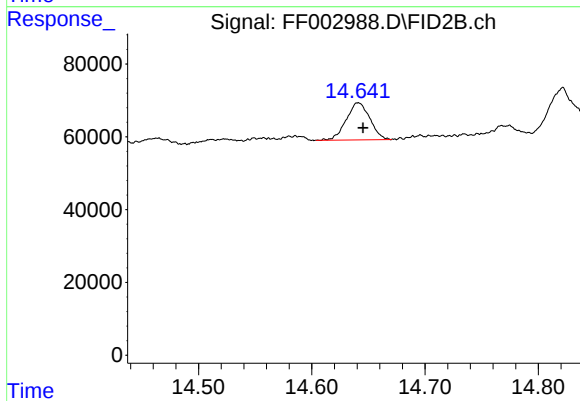


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.641 min
Delta R.T.: -0.004 min
Response: 148016
Conc: 1.14 ug/ml

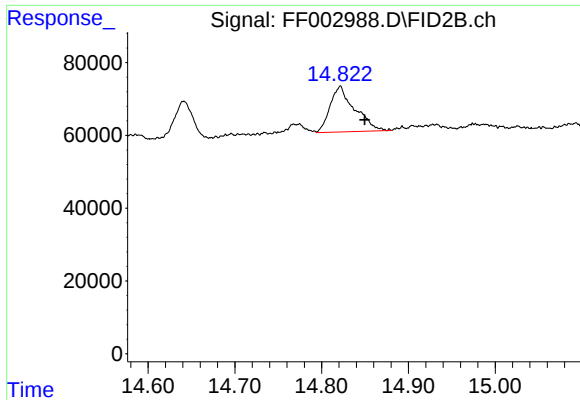


#10 N-TETRACOSANE

R.T.: 14.822 min
Delta R.T.: -0.028 min
Response: 246873
Conc: 1.71 ug/ml

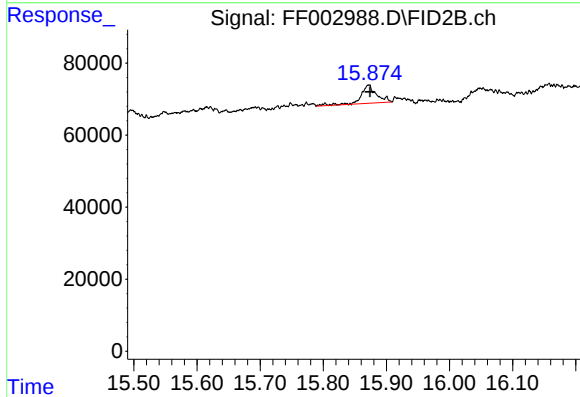


#11 N-HEXACOSANE

R.T.: 15.872 min
Delta R.T.: -0.002 min
Response: 87856
Conc: 0.63 ug/ml

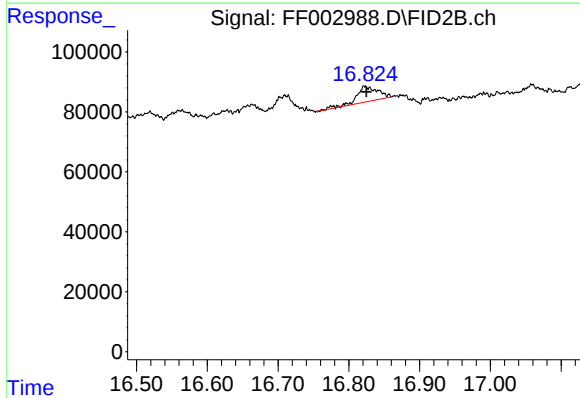


#12 N-OCTACOSANE

R.T.: 16.822 min
Delta R.T.: -0.003 min
Response: 106115
Conc: 0.79 ug/ml

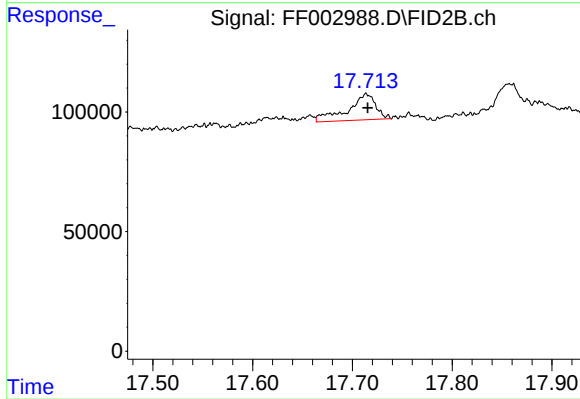


#13 N-TRIACONTANE

R.T.: 17.714 min
Delta R.T.: -0.002 min
Response: 211355
Conc: 1.65 ug/ml

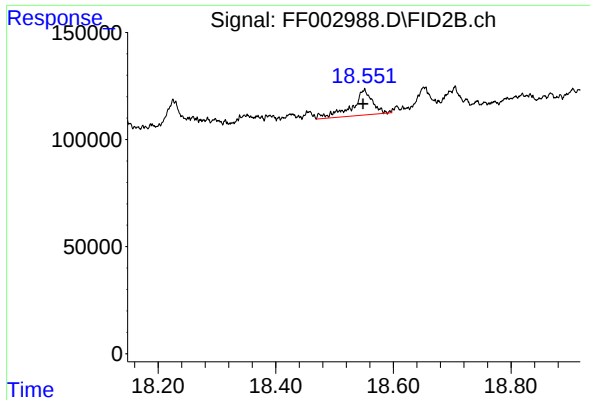


#14 N-DOTRIACONTANE

R.T.: 18.551 min
Delta R.T.: 0.002 min
Response: 287660
Conc: 2.41 ug/ml

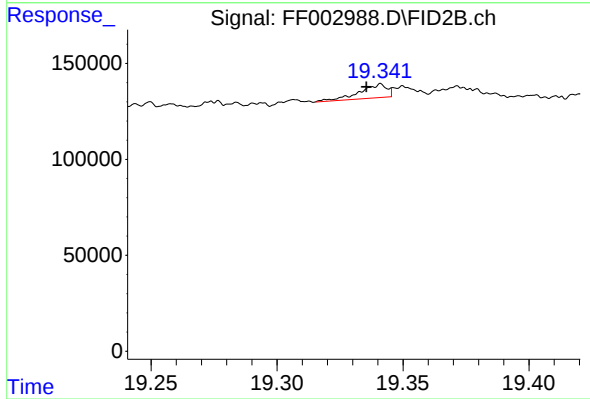


#15 N-TETRATRIACONTANE

R.T.: 19.341 min
Delta R.T.: 0.006 min
Response: 53080
Conc: 0.47 ug/ml

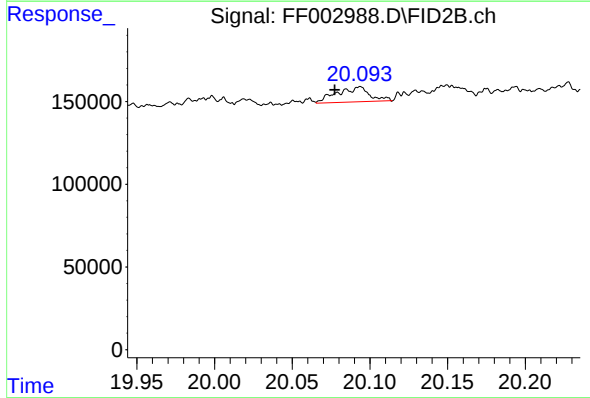

#16 N-HEXATRIACONTANE

R.T.: 20.094 min
Delta R.T.: 0.016 min
Response: 132516
Conc: 1.23 ug/ml

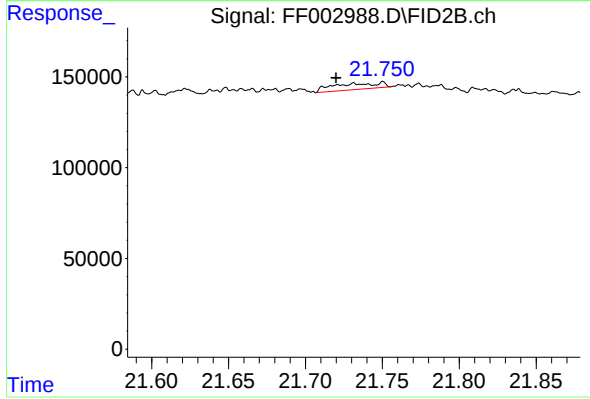

#18 N-TETRACONTANE

R.T.: 21.750 min
Delta R.T.: 0.030 min
Response: 72564
Conc: 0.69 ug/ml