

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121118\
Data File : FF002990.D
Signal(s) : FID2B.ch
Acq On : 11 Dec 2018 18:21
Operator : AJ\SJ
Sample : J6290-01
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 12 02:53:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.642	1424737	10.974 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.238f	357465	2.230 ug/ml
10)	N-TETRACOSANE	14.820	158301	1.095 ug/ml
14)	N-DOTRIACONTANE	18.551	111936	0.937 ug/ml
16)	N-HEXATRIACONTANE	20.087	40121	0.372 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121118\
Data File : FF002990.D
Signal(s) : FID2B.ch
Acq On : 11 Dec 2018 18:21
Operator : AJ\SJ
Sample : J6290-01
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 12 02:53:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

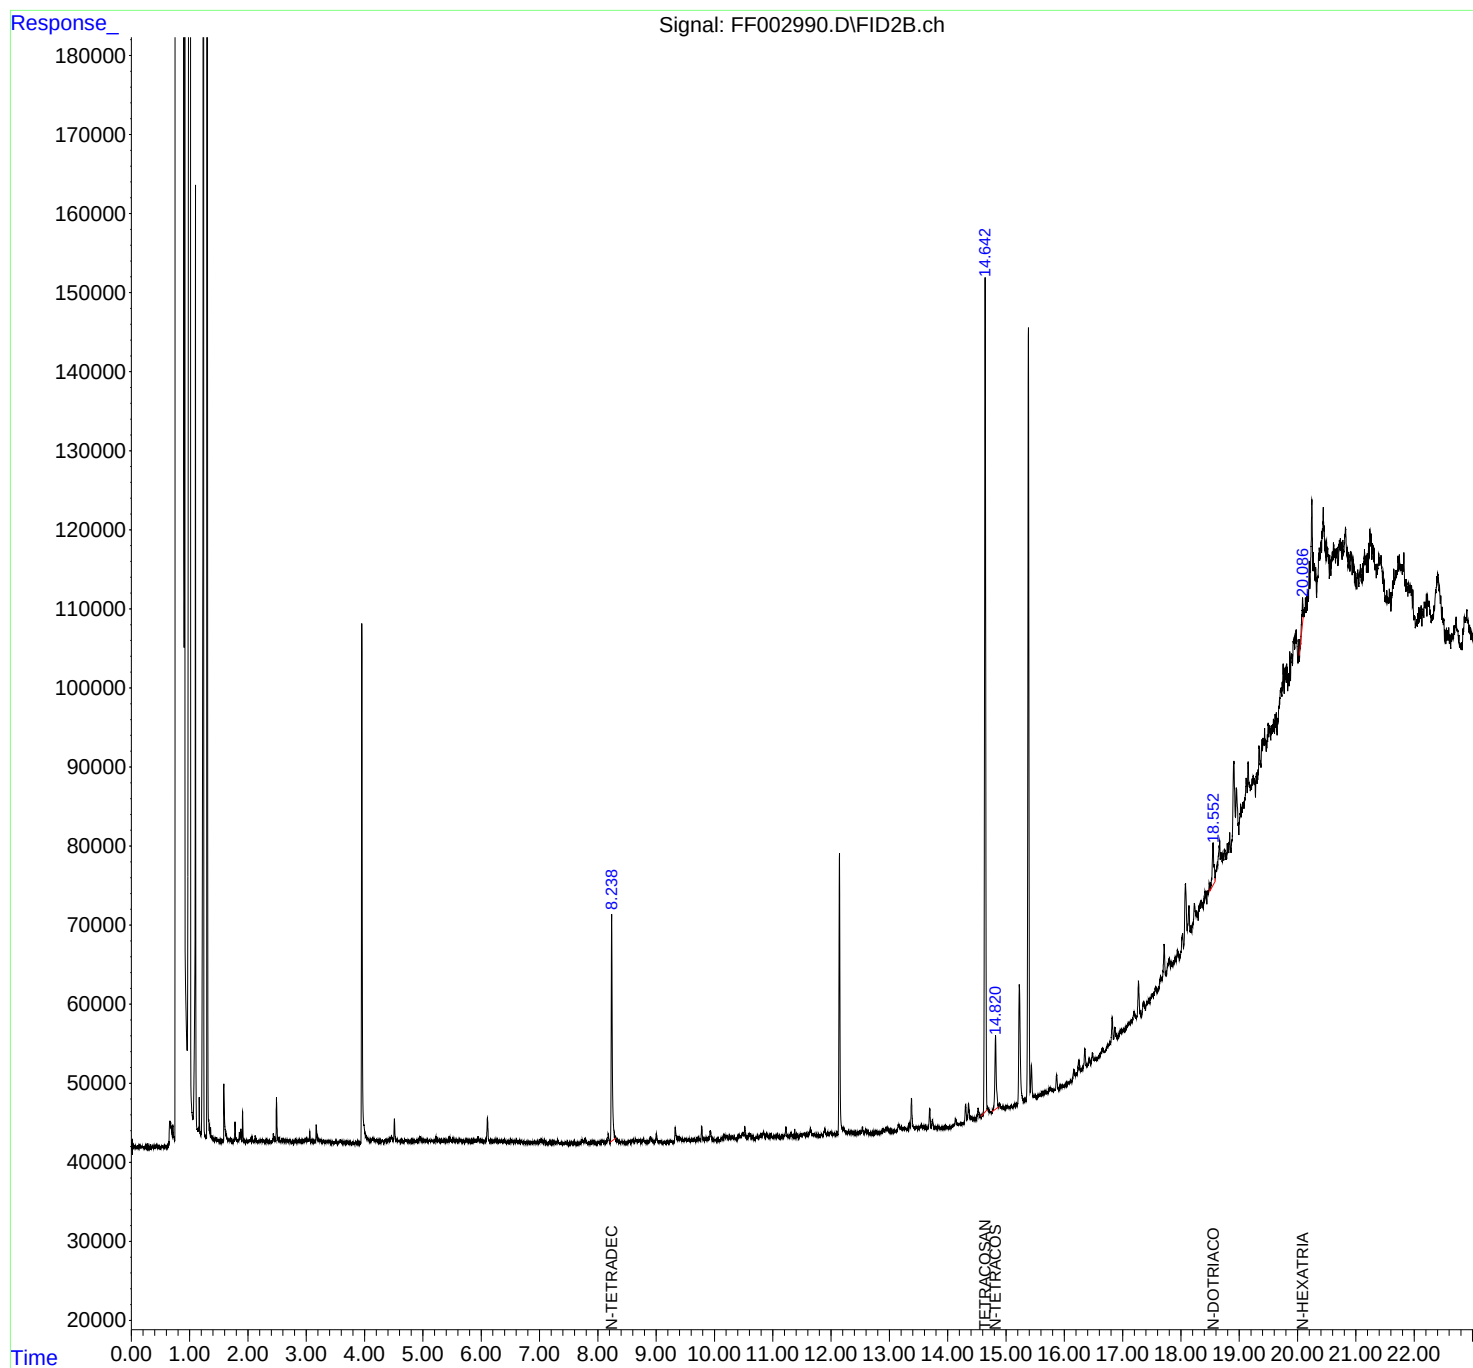

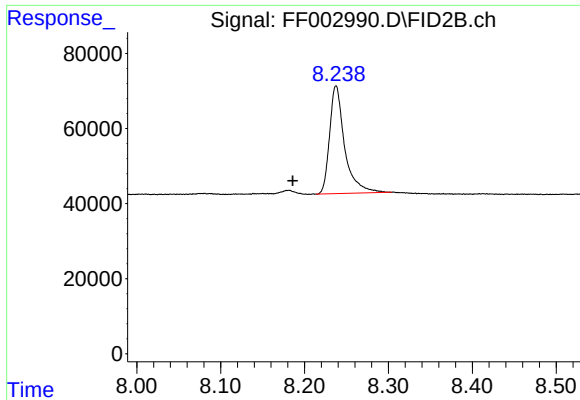


#4 N-TETRADECANE

R.T.: 8.238 min
Delta R.T.: 0.052 min
Response: 357465
Conc: 2.23 ug/ml

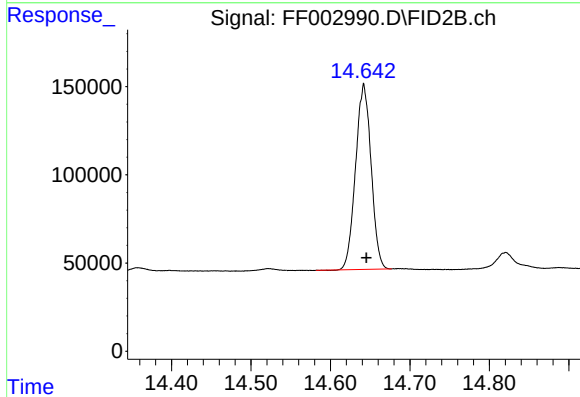


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.642 min
Delta R.T.: -0.003 min
Response: 1424737
Conc: 10.97 ug/ml

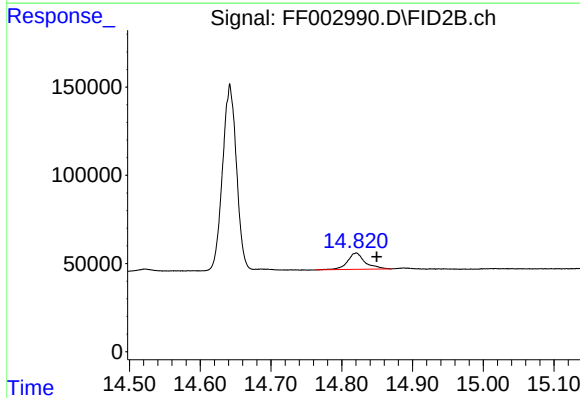


#10 N-TETRACOSANE

R.T.: 14.820 min
Delta R.T.: -0.029 min
Response: 158301
Conc: 1.10 ug/ml

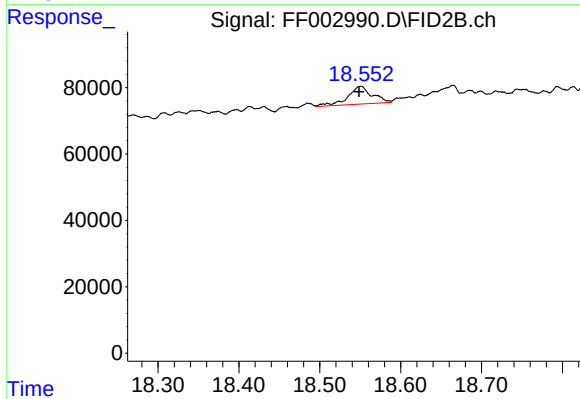

#14 N-DOTRIACONTANE

R.T.: 18.551 min
Delta R.T.: 0.002 min
Response: 111936
Conc: 0.94 ug/ml

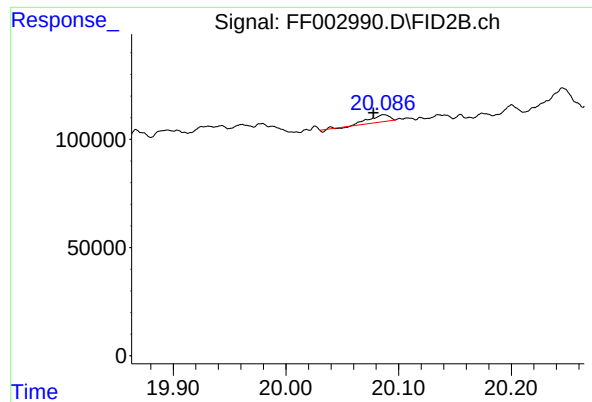

#16 N-HEXATRIACONTANE

R.T.: 20.087 min
Delta R.T.: 0.010 min
Response: 40121
Conc: 0.37 ug/ml