

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121118\
 Data File : FF002992.D
 Signal(s) : FID2B.ch
 Acq On : 11 Dec 2018 19:22
 Operator : AJ\SJ
 Sample : J6303-03 10X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 12 02:53:38 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.643	133315	1.027 ug/ml
Target Compounds			
7) N-EICOSANE	12.591	203136	1.317 ug/ml
10) N-TETRACOSANE	14.819	268948	1.861 ug/ml
12) N-OCTACOSANE	16.822	110868	0.827 ug/ml
13) N-TRIACONTANE	17.715	156321	1.220 ug/ml
14) N-DOTRIACONTANE	18.550	105091	0.880 ug/ml
15) N-TETRATRIACONTANE	19.342	105278	0.929 ug/ml
16) N-HEXATRIACONTANE	20.101	34151	0.317 ug/ml
17) N-OCTATRIACONTANE	20.817	150028	1.478 ug/ml
18) N-TETRACONTANE	21.709	44700	0.425 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121118\
Data File : FF002992.D
Signal(s) : FID2B.ch
Acq On : 11 Dec 2018 19:22
Operator : AJ\SJ
Sample : J6303-03 10X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 12 02:53:38 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

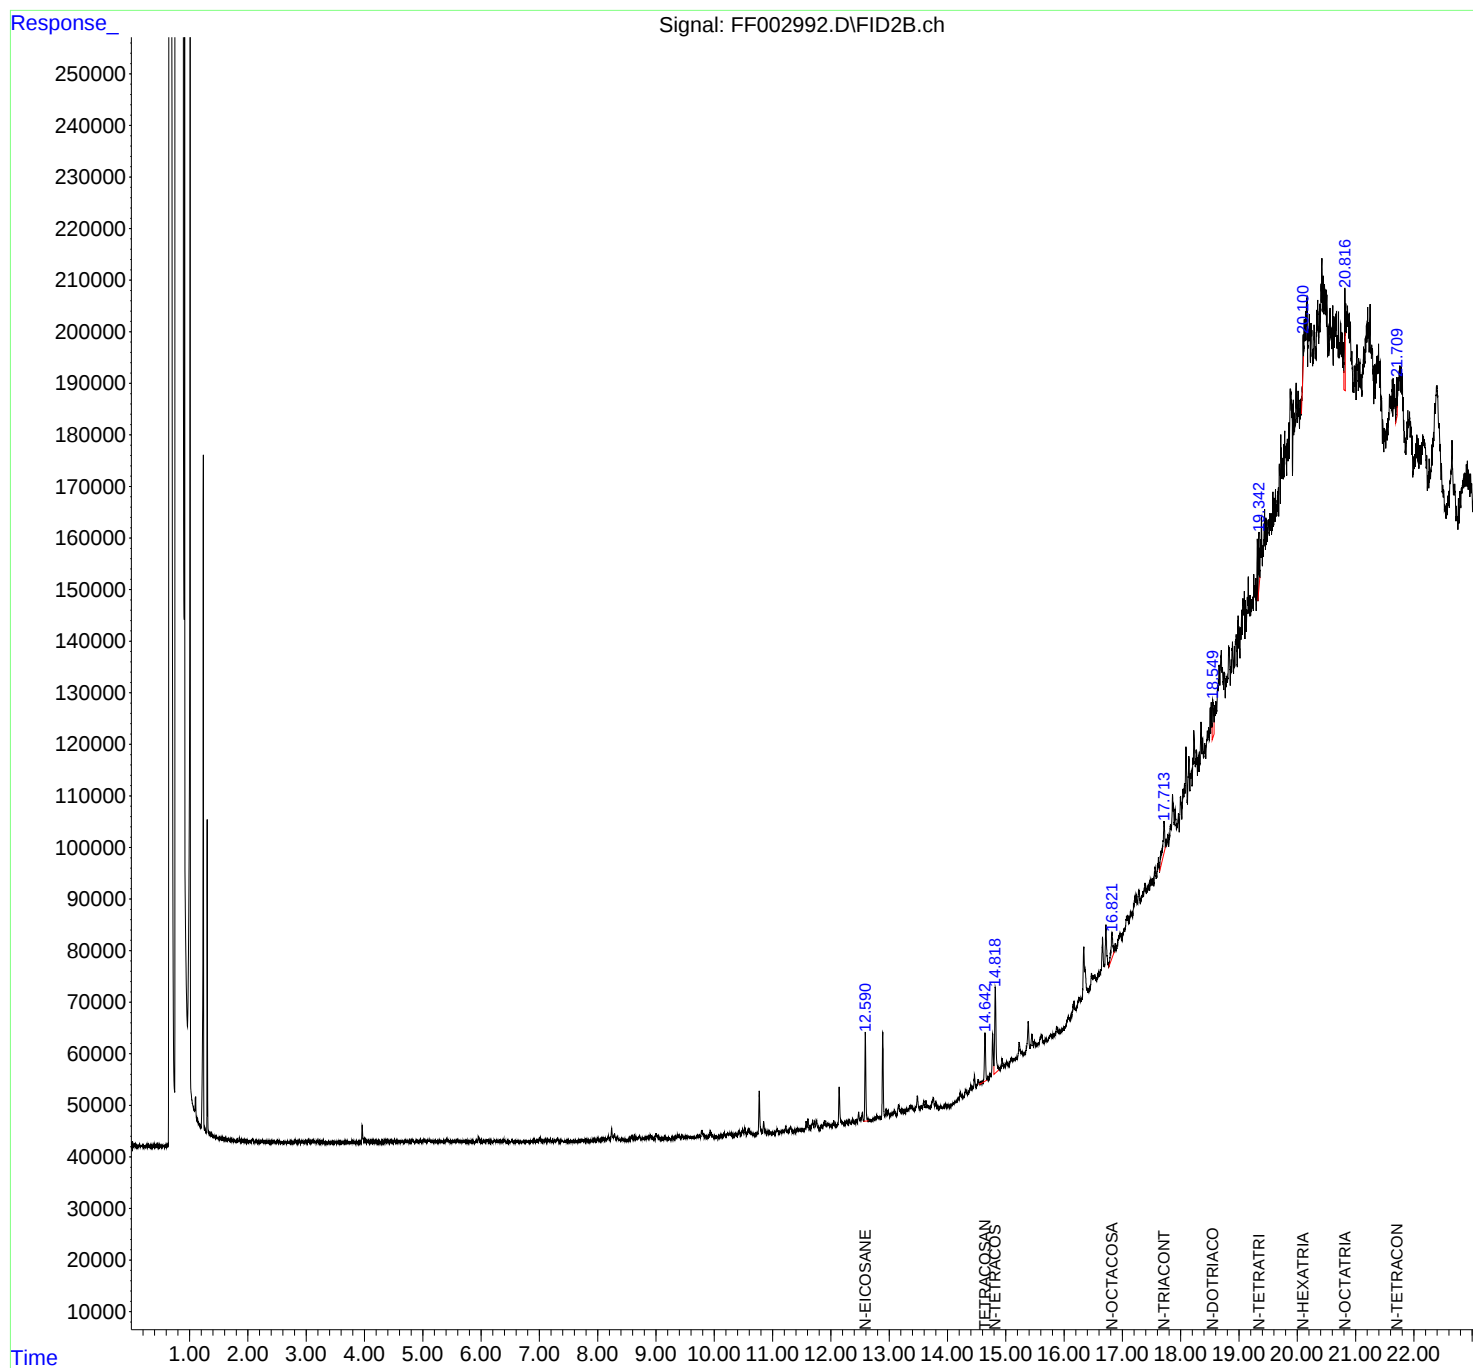

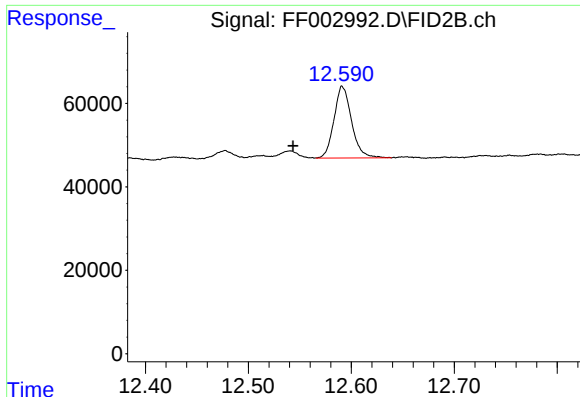


#7 N-EICOSANE

R.T.: 12.591 min
Delta R.T.: 0.048 min
Response: 203136
Conc: 1.32 ug/ml

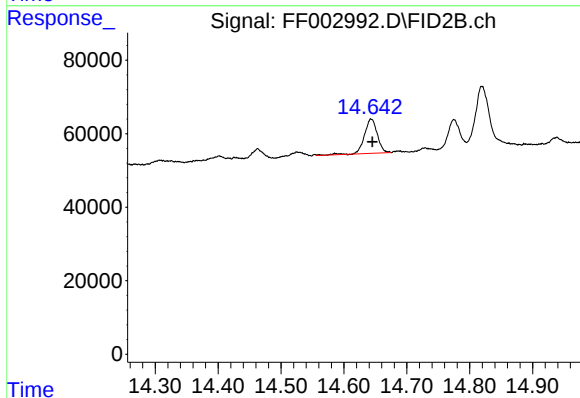


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.643 min
Delta R.T.: -0.002 min
Response: 133315
Conc: 1.03 ug/ml

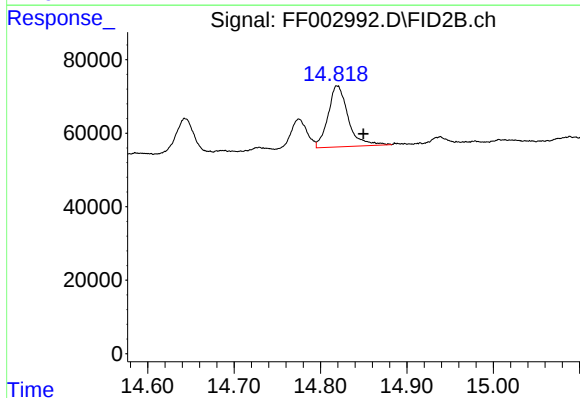


#10 N-TETRACOSANE

R.T.: 14.819 min
Delta R.T.: -0.030 min
Response: 268948
Conc: 1.86 ug/ml

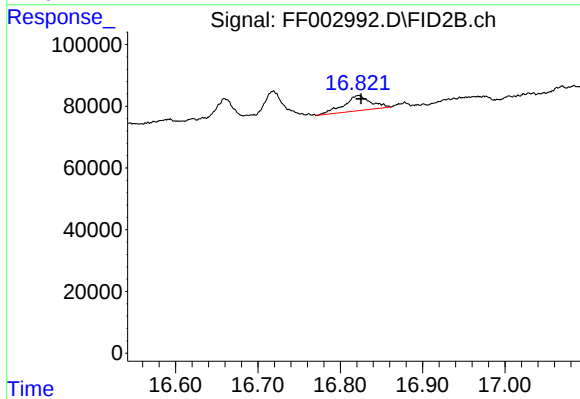


#12 N-OCTACOSANE

R.T.: 16.822 min
Delta R.T.: -0.003 min
Response: 110868
Conc: 0.83 ug/ml

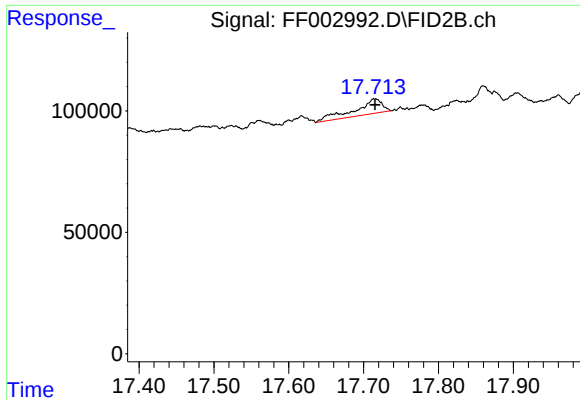


#13 N-TRIACONTANE

R.T.: 17.715 min
Delta R.T.: 0.000 min
Response: 156321
Conc: 1.22 ug/ml

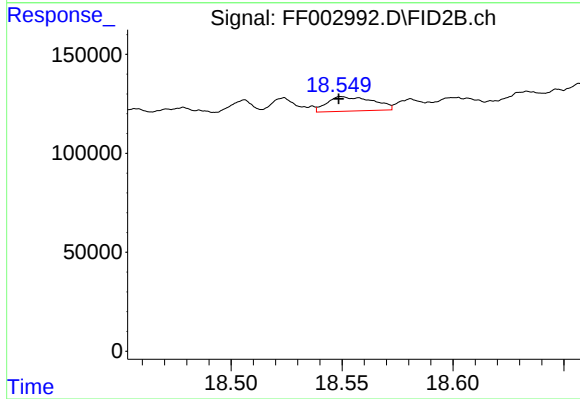


#14 N-DOTRIACONTANE

R.T.: 18.550 min
Delta R.T.: 0.001 min
Response: 105091
Conc: 0.88 ug/ml

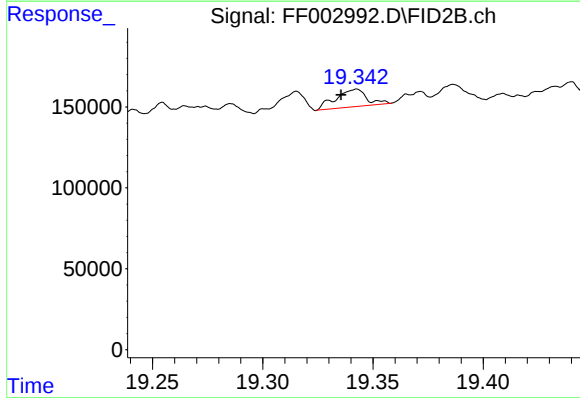


#15 N-TETRATRIACONTANE

R.T.: 19.342 min
Delta R.T.: 0.007 min
Response: 105278
Conc: 0.93 ug/ml

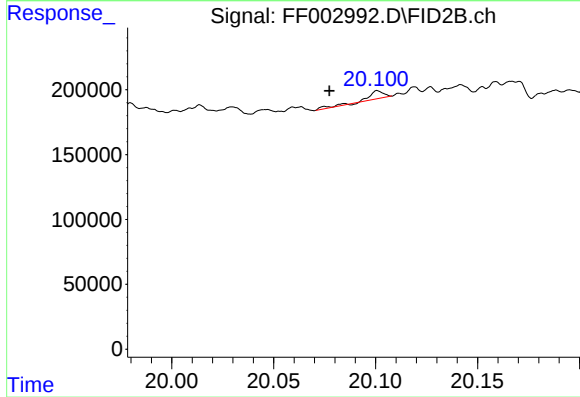


#16 N-HEXATRIACONTANE

R.T.: 20.101 min
Delta R.T.: 0.024 min
Response: 34151
Conc: 0.32 ug/ml

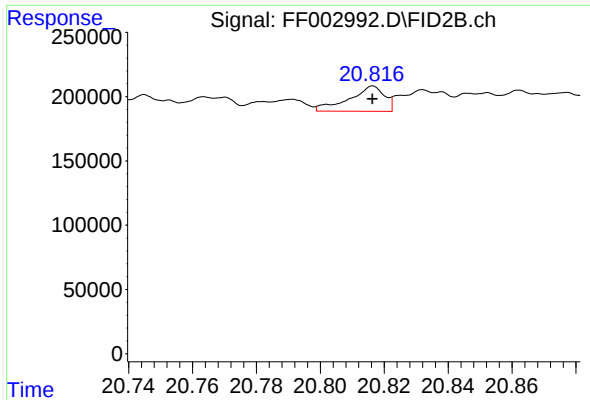

#17 N-OCTATRIACONTANE

R.T.: 20.817 min
Delta R.T.: 0.000 min
Response: 150028
Conc: 1.48 ug/ml

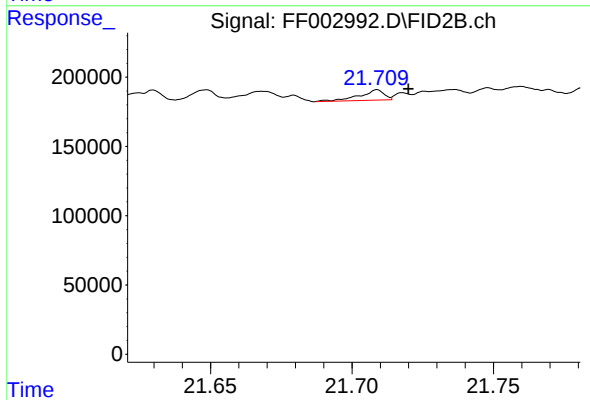

#18 N-TETRACONTANE

R.T.: 21.709 min
Delta R.T.: -0.011 min
Response: 44700
Conc: 0.43 ug/ml