

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121118\
Data File : FF002993.D
Signal(s) : FID2B.ch
Acq On : 11 Dec 2018 19:52
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 12 02:53:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.644	2149667	16.558 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.823	140745	0.974 ug/ml
13)	N-TRIACONTANE	17.713	71268	0.556 ug/ml
14)	N-DOTRIACONTANE	18.551	182582	1.529 ug/ml
16)	N-HEXATRIACONTANE	20.083	85981	0.797 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121118\
Data File : FF002993.D
Signal(s) : FID2B.ch
Acq On : 11 Dec 2018 19:52
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 12 02:53:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

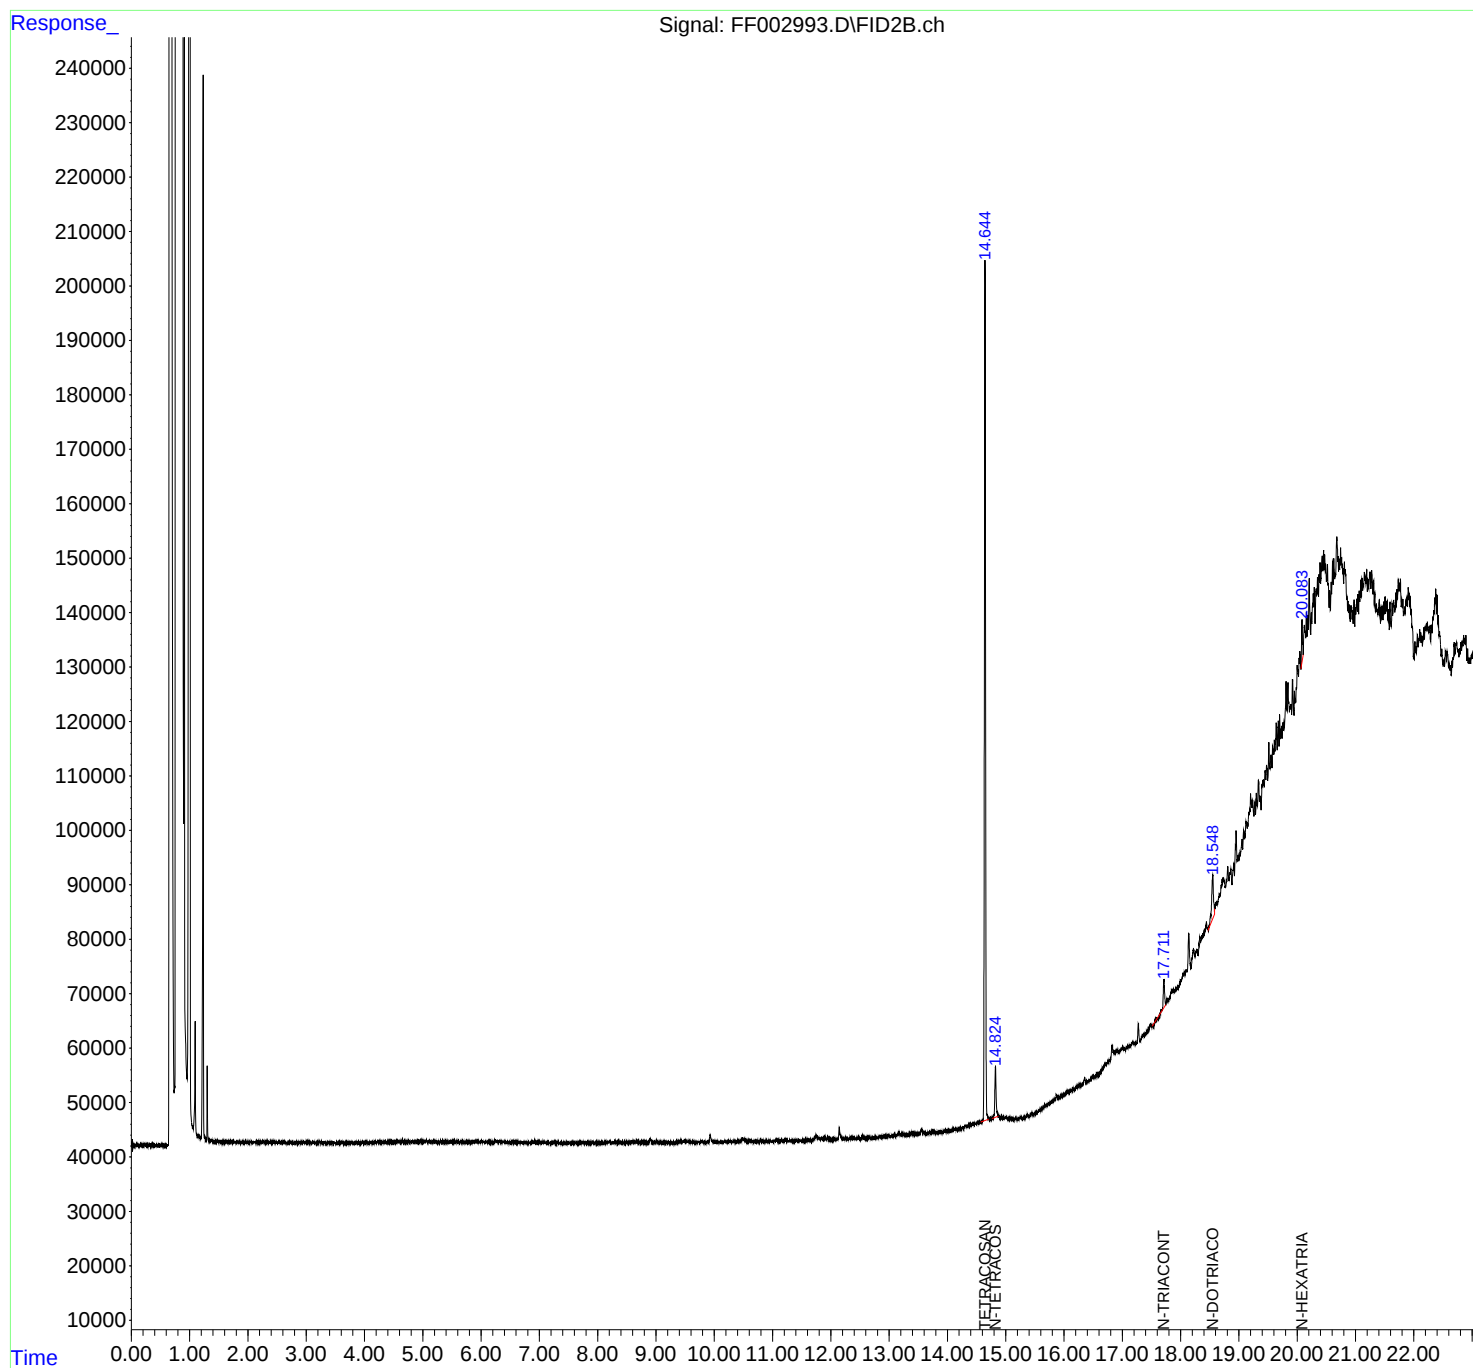

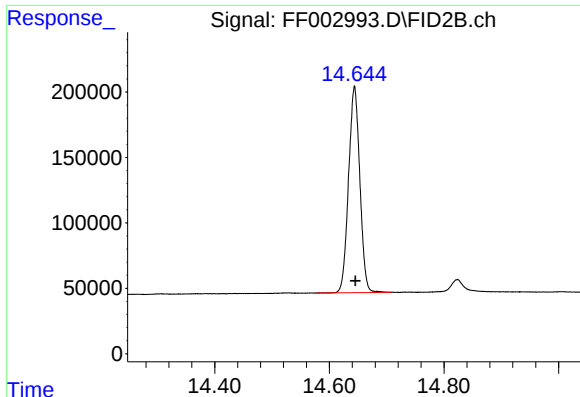


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.644 min
Delta R.T.: -0.001 min
Response: 2149667
Conc: 16.56 ug/ml

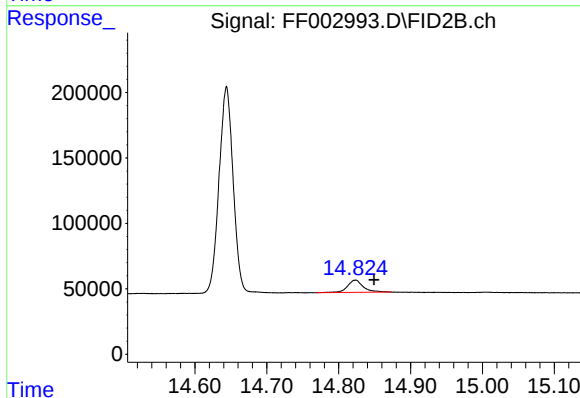


#10 N-TETRACOSANE

R.T.: 14.823 min
Delta R.T.: -0.026 min
Response: 140745
Conc: 0.97 ug/ml

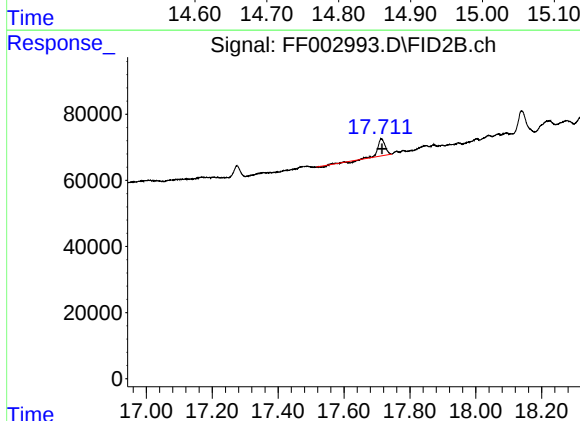


#13 N-TRIACONTANE

R.T.: 17.713 min
Delta R.T.: -0.002 min
Response: 71268
Conc: 0.56 ug/ml

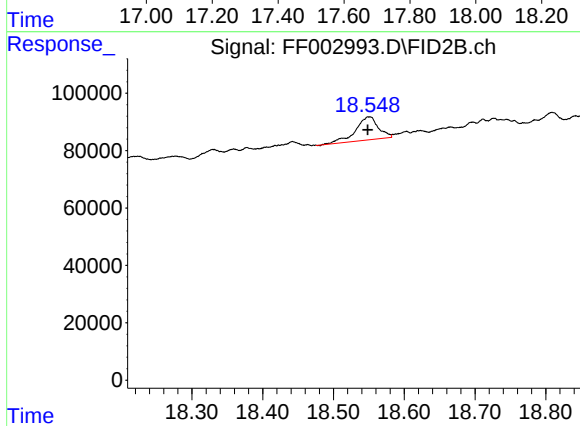

#14 N-DOTRIACONTANE

R.T.: 18.551 min
Delta R.T.: 0.002 min
Response: 182582
Conc: 1.53 ug/ml

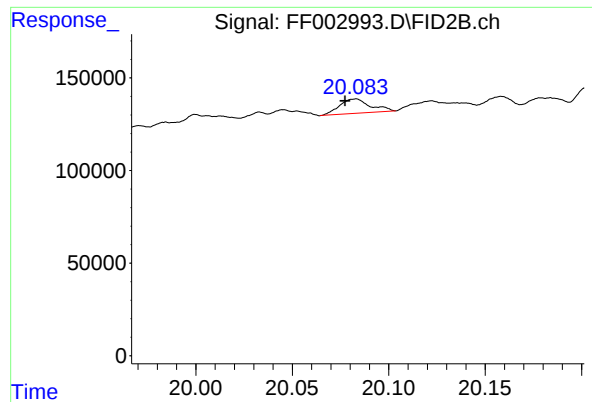

#16 N-HEXATRIACONTANE

R.T.: 20.083 min
Delta R.T.: 0.005 min
Response: 85981
Conc: 0.80 ug/ml