

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121120\
Data File : FF007960.D
Signal(s) : FID2B.ch
Acq On : 11 Dec 2020 14:07
Operator : DD\AJ
Sample : L5012-01
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WASTE

Integration File: autoint1.e
Quant Time: Dec 11 22:14:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120220.M
Quant Title :
QLast Update : Thu Dec 03 09:08:10 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.703	2079291	16.447 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.603	136342	1.230 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121120\
Data File : FF007960.D
Signal(s) : FID2B.ch
Acq On : 11 Dec 2020 14:07
Operator : DD\AJ
Sample : L5012-01
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WASTE

Integration File: autoint1.e
Quant Time: Dec 11 22:14:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120220.M
Quant Title :
QLast Update : Thu Dec 03 09:08:10 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

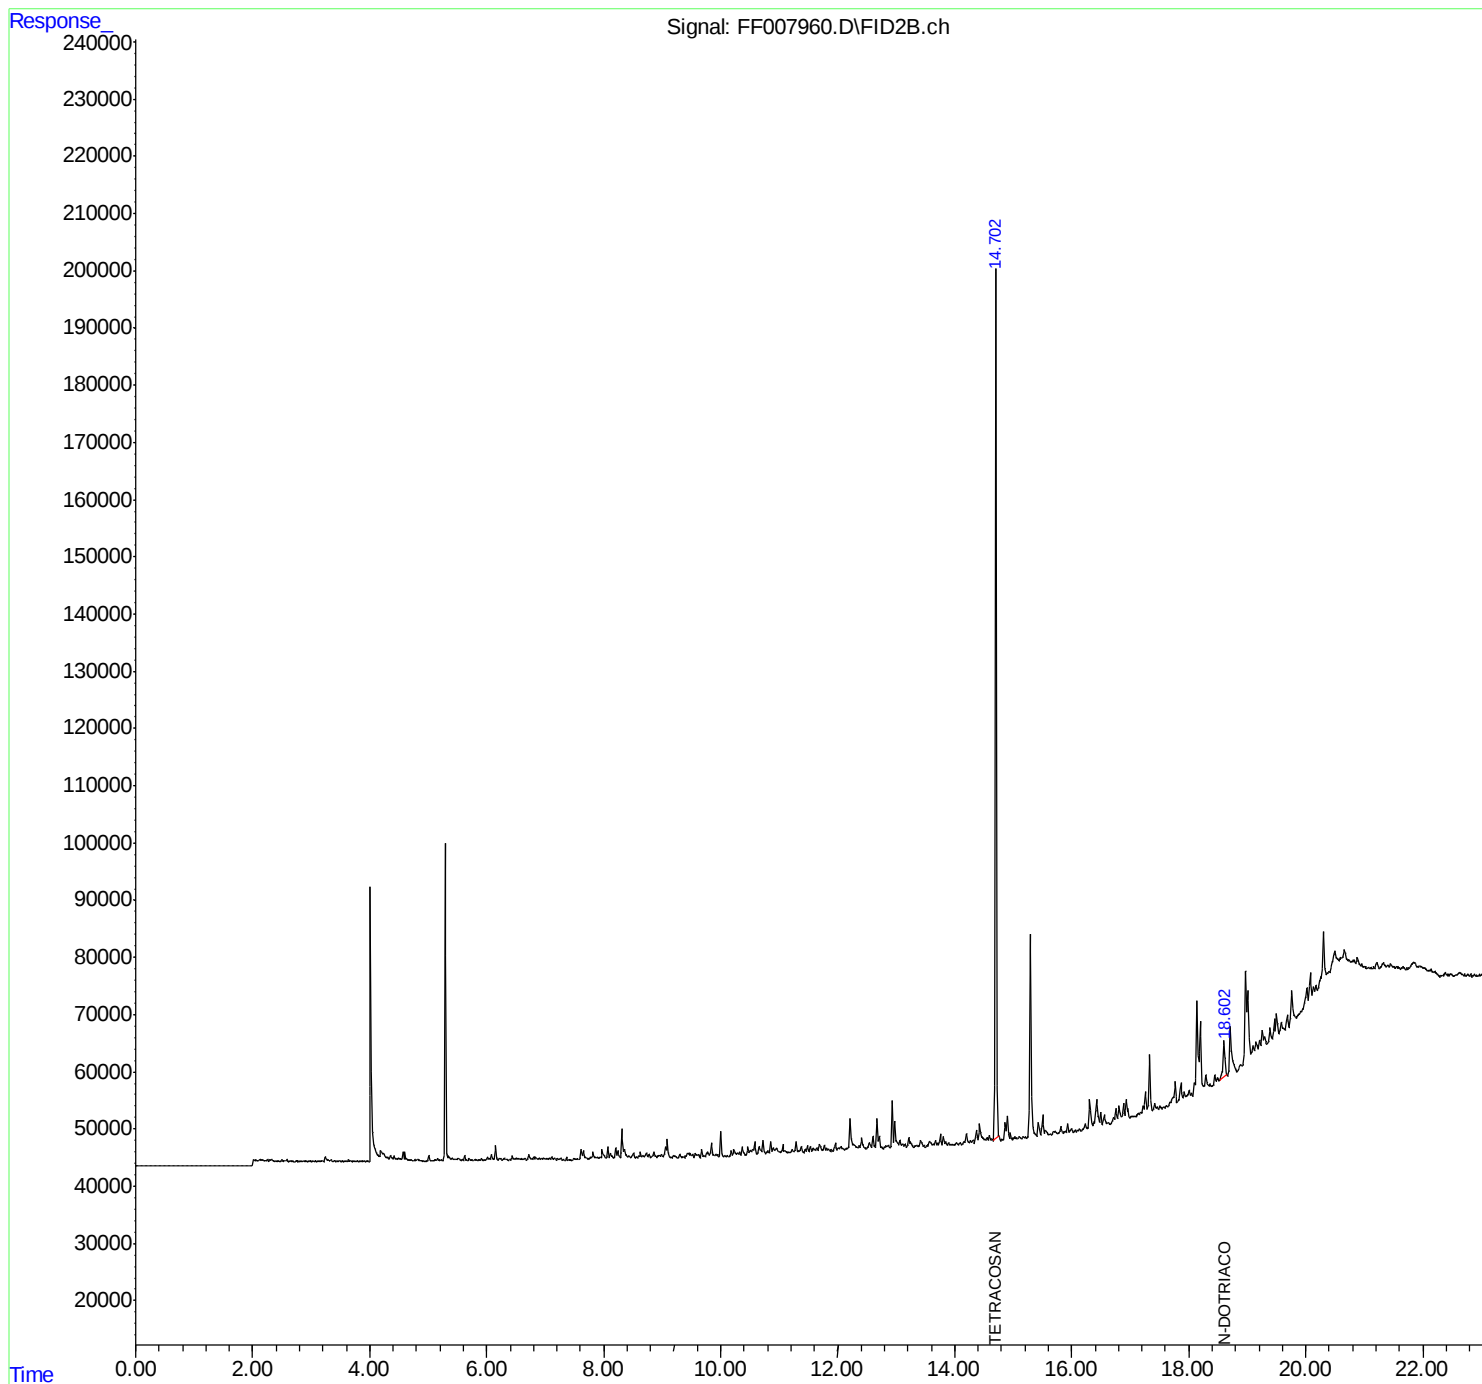


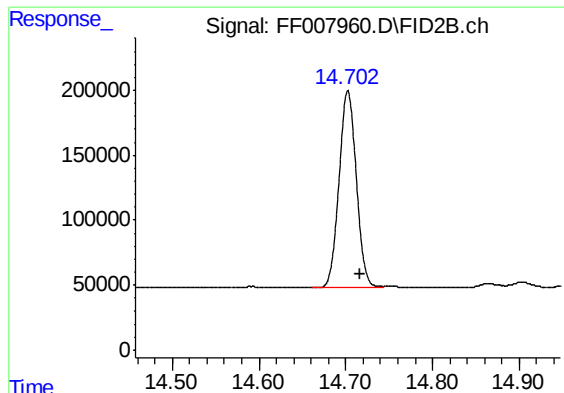

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.703 min
Delta R.T.: -0.014 min
Response: 2079291
Conc: 16.45 ug/ml

Instrument :
FID_F
ClientSampleId :
WASTE

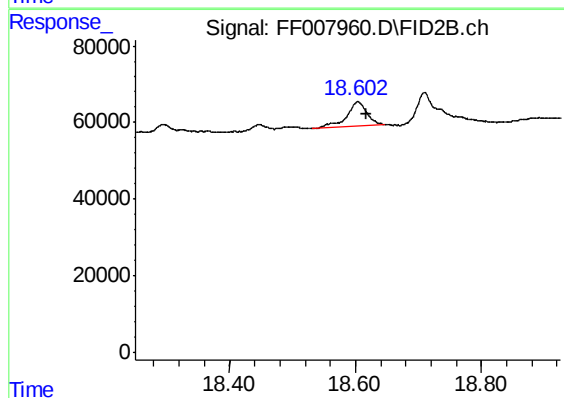

#14 N-DOTRIACONTANE

R.T.: 18.603 min
Delta R.T.: -0.015 min
Response: 136342
Conc: 1.23 ug/ml