

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121120\
Data File : FF007967.D
Signal(s) : FID2B.ch
Acq On : 11 Dec 2020 21:18
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 11 22:15:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120220.M
Quant Title :
QLast Update : Thu Dec 03 09:08:10 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.744	246197	1.947 ug/ml
Target Compounds			
11) N-HEXACOSANE	15.929	102365	0.726 ug/ml
12) N-OCTACOSANE	16.881	111712	0.825 ug/ml
13) N-TRIACONTANE	17.770	117348	0.927 ug/ml
14) N-DOTRIACONTANE	18.605	102297	0.923 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121120\
Data File : FF007967.D
Signal(s) : FID2B.ch
Acq On : 11 Dec 2020 21:18
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 11 22:15:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120220.M
Quant Title :
QLast Update : Thu Dec 03 09:08:10 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

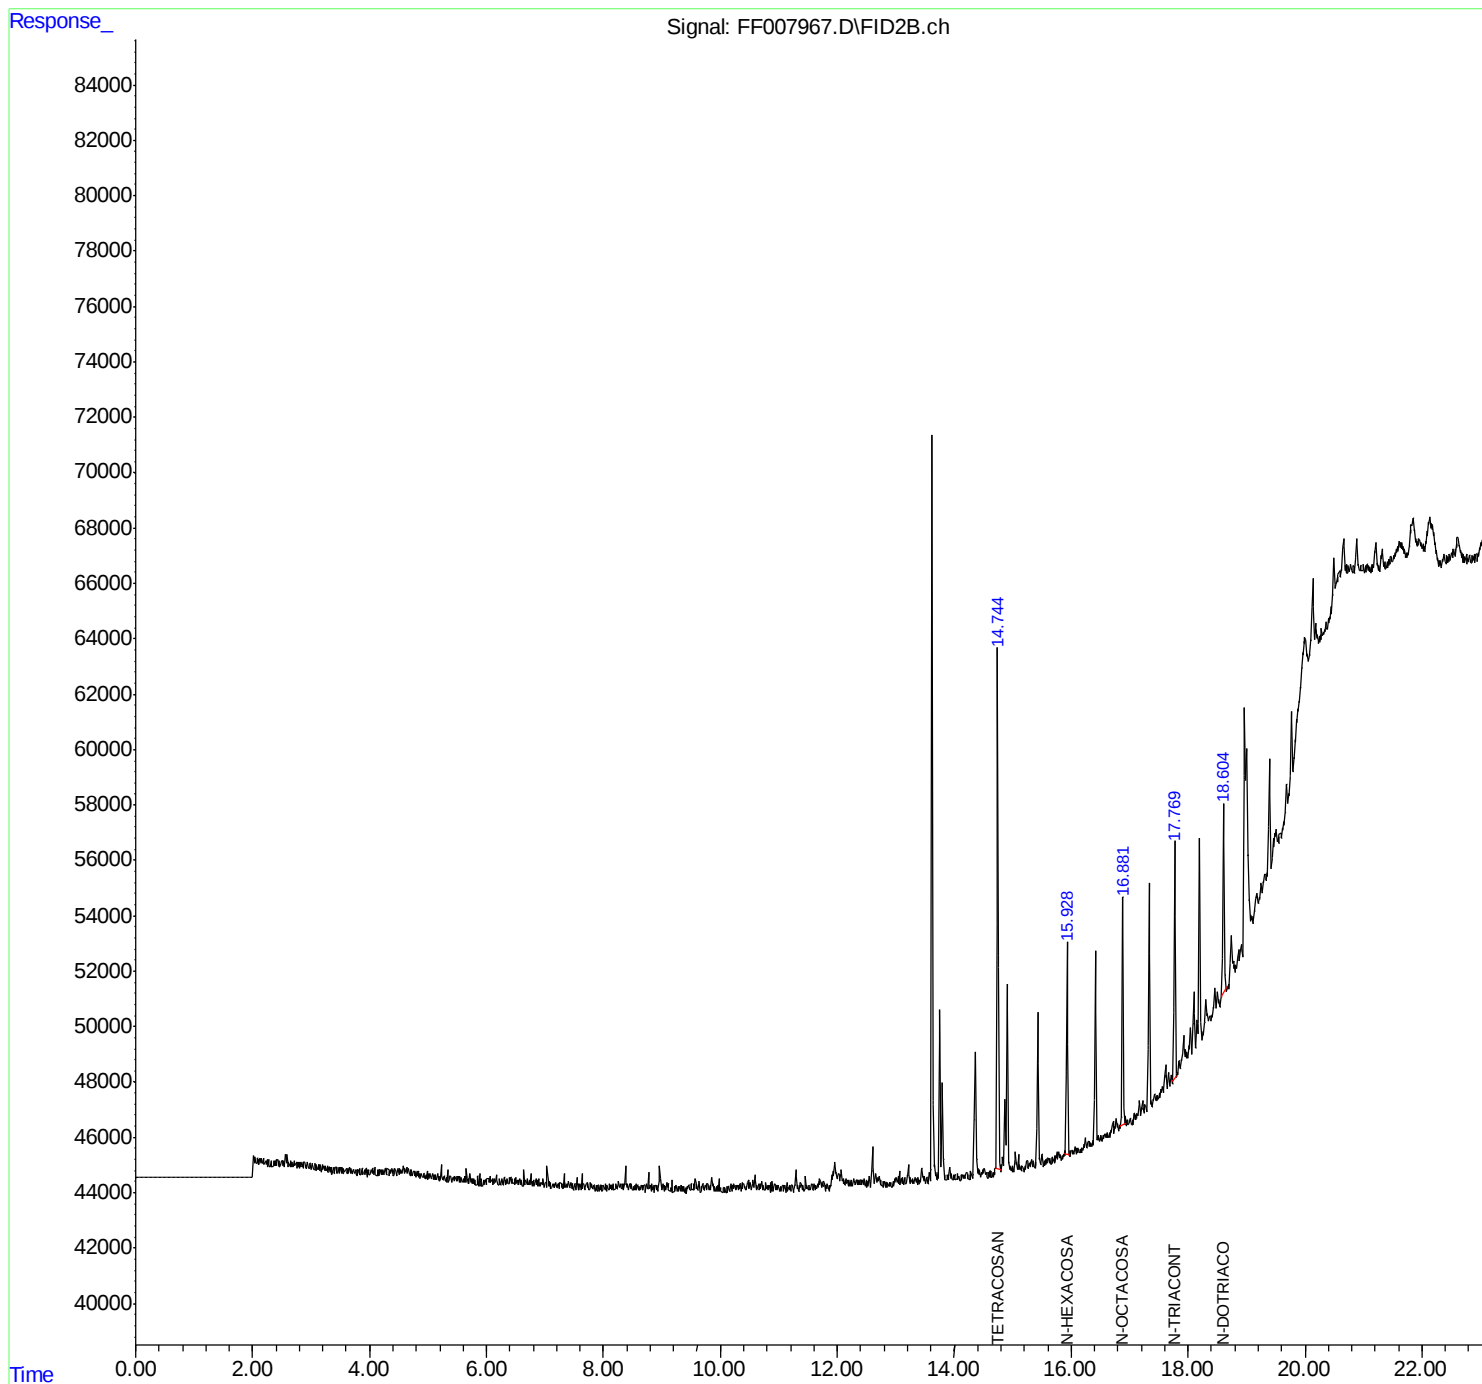


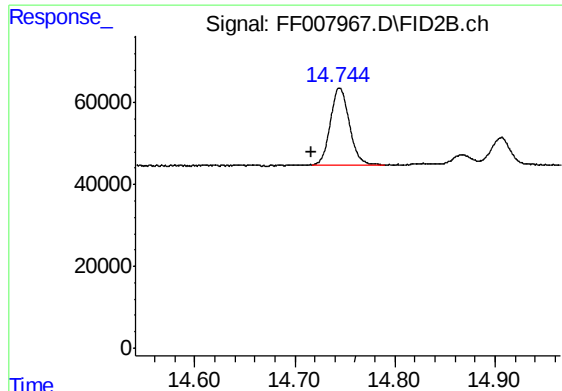

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.744 min
Delta R.T.: 0.028 min
Response: 246197
Conc: 1.95 ug/ml

Instrument :
FID_F
ClientSampleId :

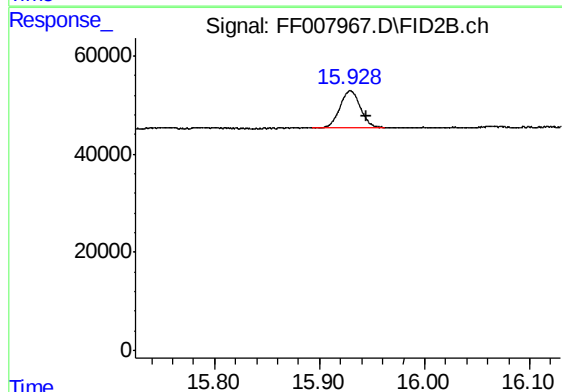


#11 N-HEXACOSANE

R.T.: 15.929 min
Delta R.T.: -0.016 min
Response: 102365
Conc: 0.73 ug/ml

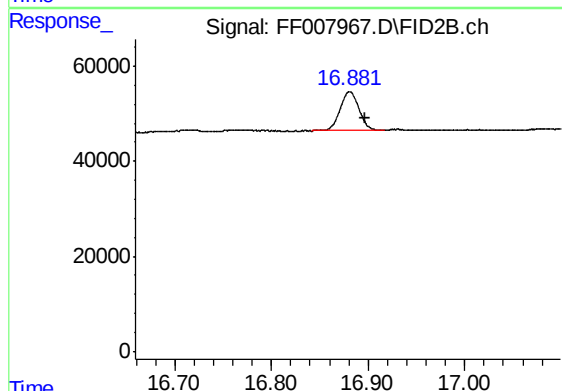


#12 N-OCTACOSANE

R.T.: 16.881 min
Delta R.T.: -0.016 min
Response: 111712
Conc: 0.83 ug/ml

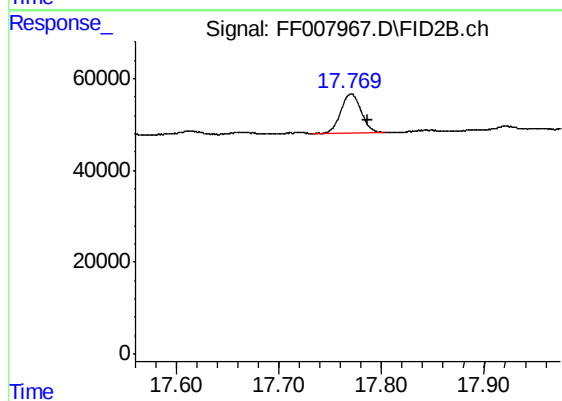

#13 N-TRIACONTANE

R.T.: 17.770 min
Delta R.T.: -0.016 min
Response: 117348
Conc: 0.93 ug/ml

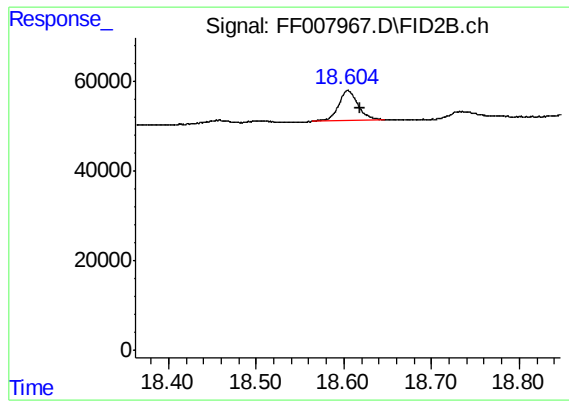

#14 N-DOTRIACONTANE

R.T.: 18.605 min

Delta R.T.: -0.014 min

Response: 102297

Conc: 0.92 ug/ml

Instrument :
FID_F
ClientSampleId :