

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB121218\
 Data File : FB019049.D
 Signal(s) : FID2B.CH
 Acq On : 12 Dec 2018 15:11
 Operator : MJ/SJ
 Sample : J6344-05MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 12 15:32:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
 Quant Title :
 QLast Update : Fri Dec 07 17:57:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.110	168345	19.260 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.960	378268	24.743 ng/ml
2) t	2,2,4-Trimethylpentane	7.728	356259	23.125 ng/ml
3) t	n-Heptane	8.067	117933	7.935 ng/ml
4) t	Benzene	8.205	181291	10.065 ng/ml
6) t	Toluene	10.959	435789	28.710 ng/ml
7) t	Ethylbenzene	13.409	142772	9.190 ng/ml
8) t	m-Xylene	13.541	299786	18.401 ng/ml
9) t	O-Xylene	14.273	301445	17.828 ng/ml
10) t	1,2,4-Trimethylbenzene	16.556	360081	17.793 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB121218\
Data File : FB019049.D
Signal(s) : FID2B.CH
Acq On : 12 Dec 2018 15:11
Operator : MJ/SJ
Sample : J6344-05MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 12 15:32:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
Quant Title :
QLast Update : Fri Dec 07 17:57:38 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

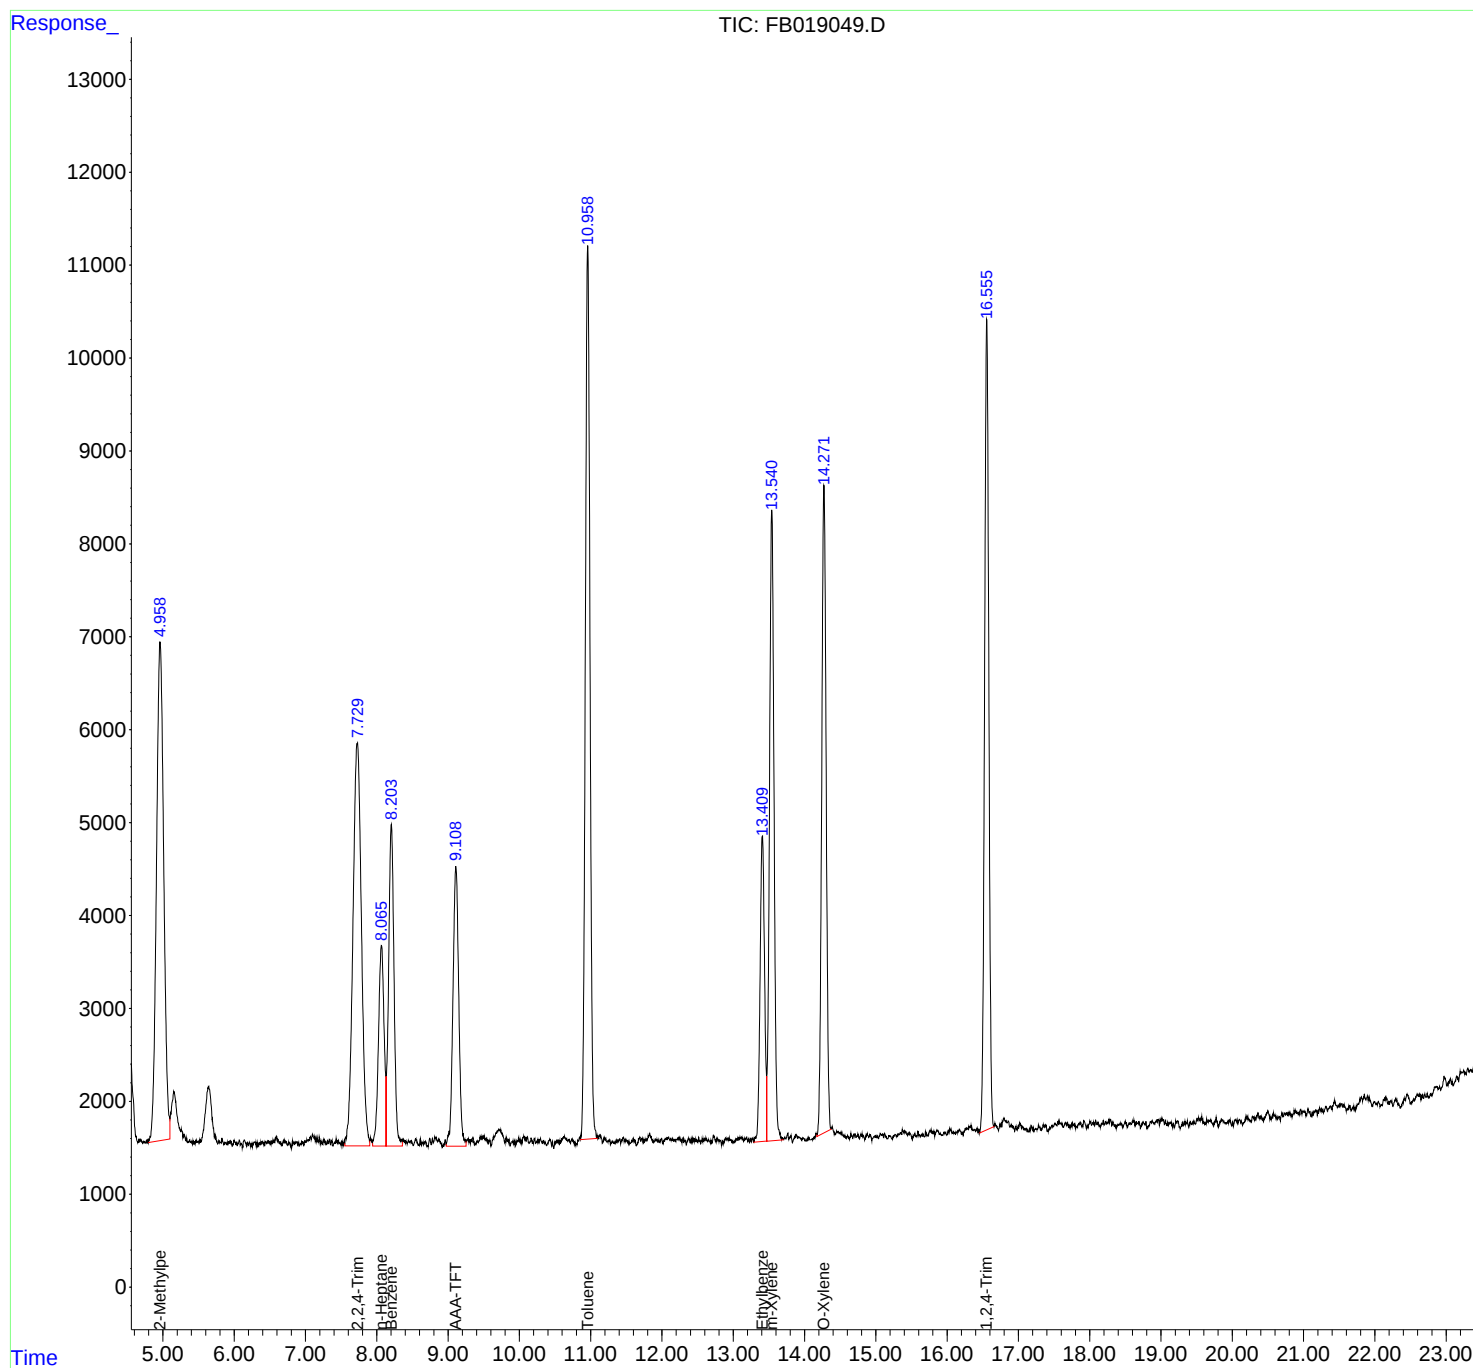

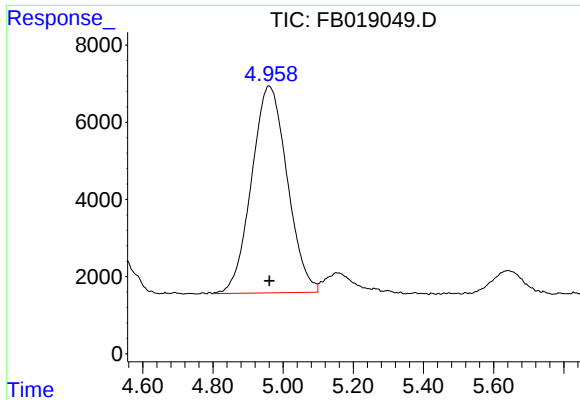


#1 2-Methylpentane

R.T.: 4.960 min
Delta R.T.: 0.000 min
Response: 378268
Conc: 24.74 ng/ml

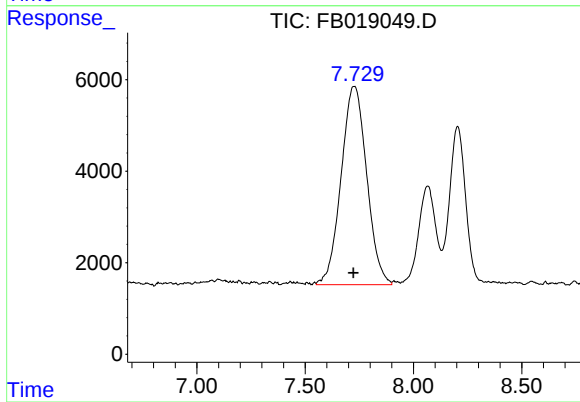


#2 2,2,4-Trimethylpentane

R.T.: 7.728 min
Delta R.T.: 0.005 min
Response: 356259
Conc: 23.12 ng/ml

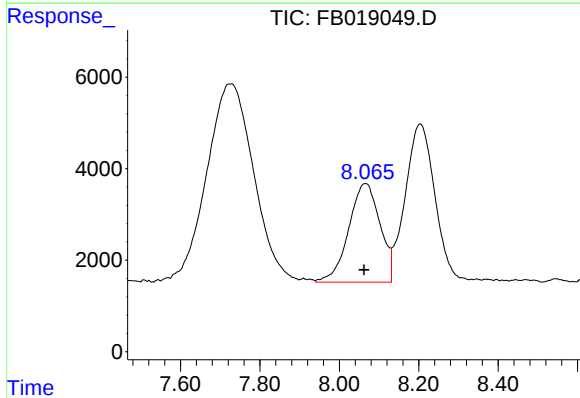


#3 n-Heptane

R.T.: 8.067 min
Delta R.T.: 0.004 min
Response: 117933
Conc: 7.93 ng/ml

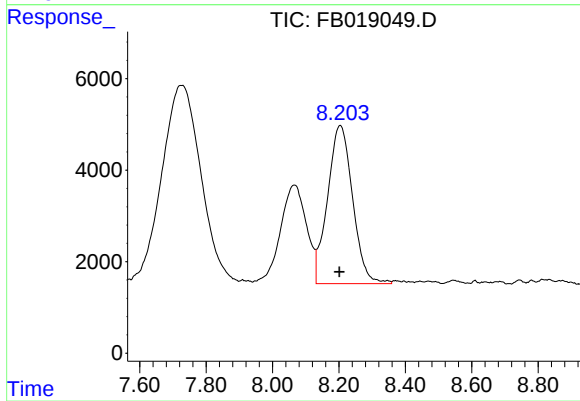


#4 Benzene

R.T.: 8.205 min
Delta R.T.: 0.004 min
Response: 181291
Conc: 10.06 ng/ml

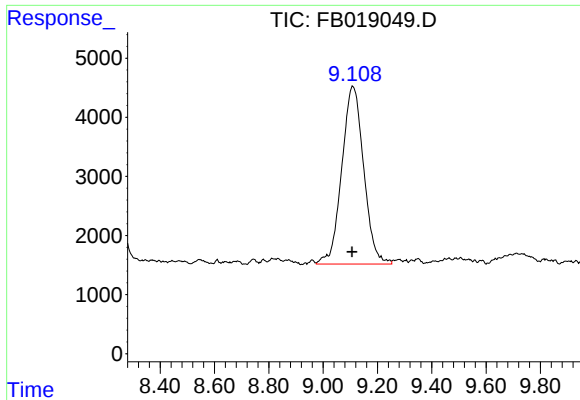


#5 AAA-TFT

R.T.: 9.110 min
 Delta R.T.: 0.003 min
 Response: 168345
 Conc: 19.26 ng/ml

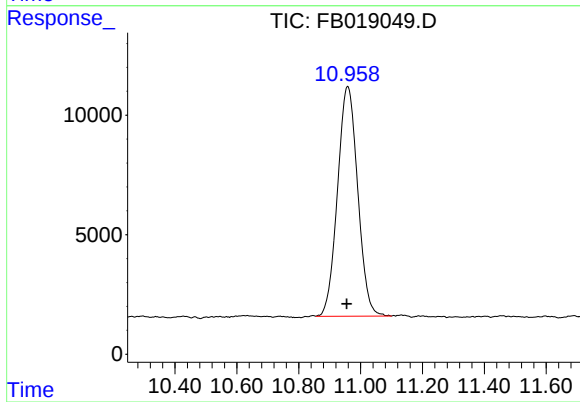


#6 Toluene

R.T.: 10.959 min
 Delta R.T.: 0.003 min
 Response: 435789
 Conc: 28.71 ng/ml

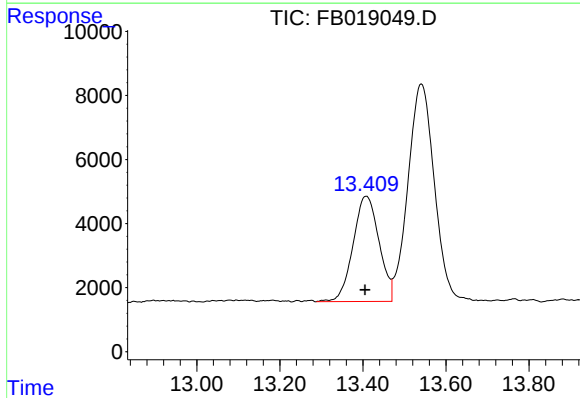


#7 Ethylbenzene

R.T.: 13.409 min
 Delta R.T.: 0.003 min
 Response: 142772
 Conc: 9.19 ng/ml

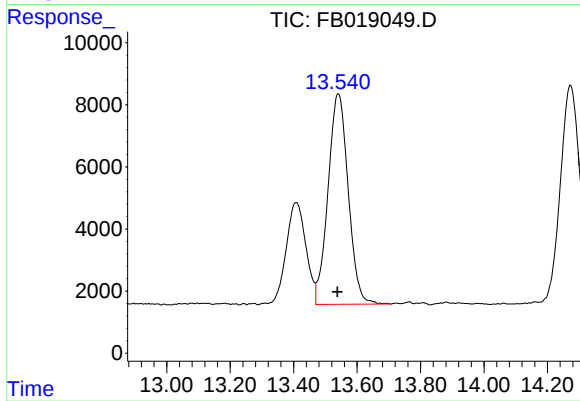


#8 m-Xylene

R.T.: 13.541 min
 Delta R.T.: 0.004 min
 Response: 299786
 Conc: 18.40 ng/ml

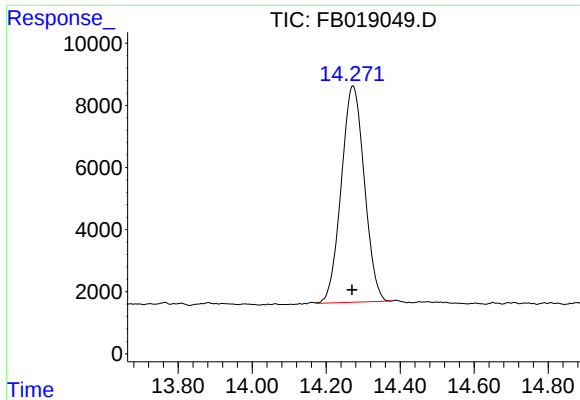

#9 O-Xylene

R.T.: 14.273 min
Delta R.T.: 0.003 min
Response: 301445
Conc: 17.83 ng/ml

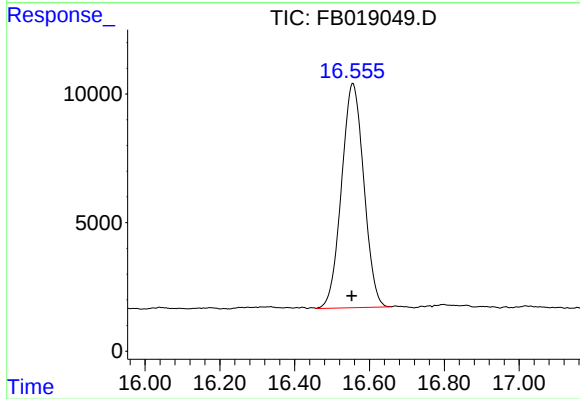

#10 1,2,4-Trimethylbenzene

R.T.: 16.556 min
Delta R.T.: 0.003 min
Response: 360081
Conc: 17.79 ng/ml