

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121218\
 Data File : FF003000.D
 Signal(s) : FID2B.ch
 Acq On : 12 Dec 2018 11:06
 Operator : AJ\SJ
 Sample : J6193-01MS 5X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Dec 12 14:05:02 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.643	471522	3.632 ug/ml
Target Compounds			
2) N-DECANE	4.365	512605	3.272 ug/ml
3) N-DODECANE	6.387	529819	3.336 ug/ml
4) N-TETRADECANE	8.181	504437	3.147 ug/ml
5) N-HEXADECANE	9.782	564986	3.528 ug/ml
6) N-OCTADECANE	11.226	529581	3.343 ug/ml
7) N-EICOSANE	12.538	529458	3.433 ug/ml
8) N-DOCOSANE	13.741	536647	3.589 ug/ml
10) N-TETRACOSANE	14.847	482513	3.339 ug/ml
11) N-HEXACOSANE	15.871	453730	3.251 ug/ml
12) N-OCTACOSANE	16.823	667257	4.980 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121218\
Data File : FF003000.D
Signal(s) : FID2B.ch
Acq On : 12 Dec 2018 11:06
Operator : AJ\SJ
Sample : J6193-01MS 5X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Dec 12 14:05:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

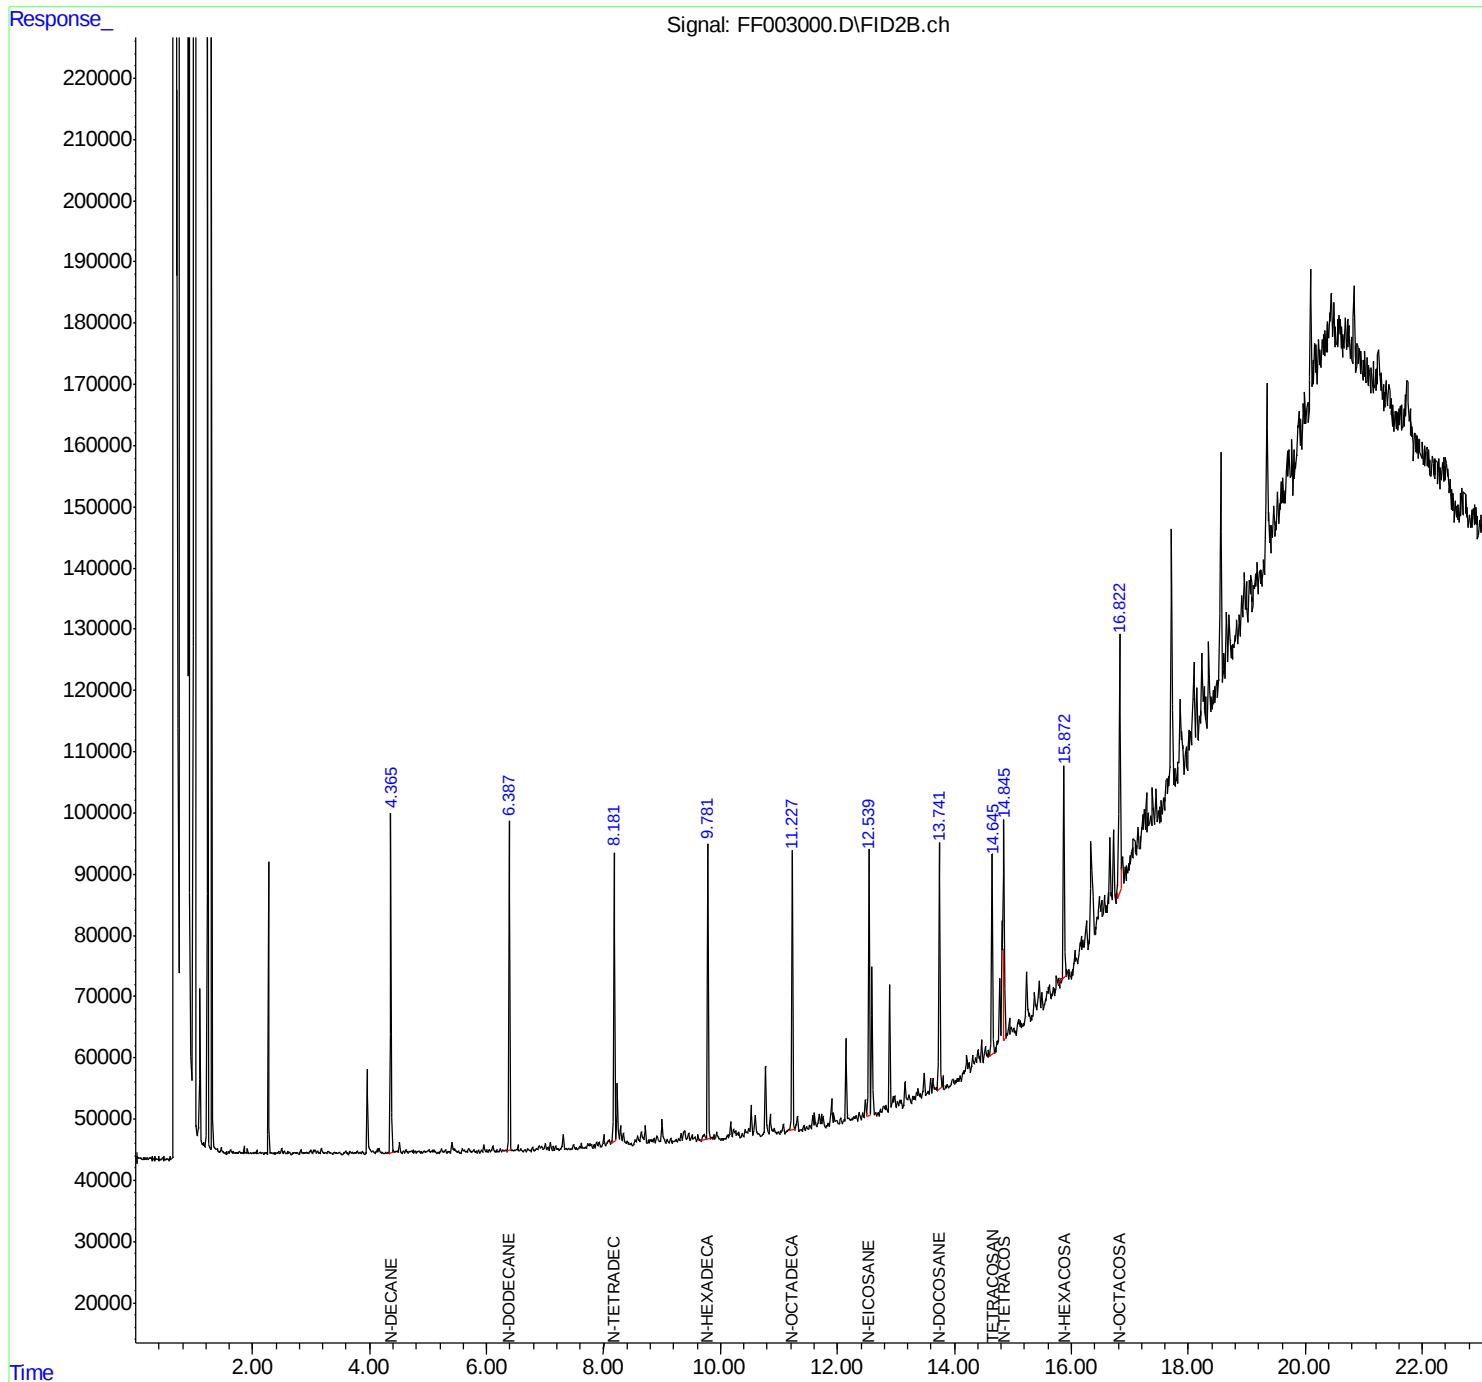

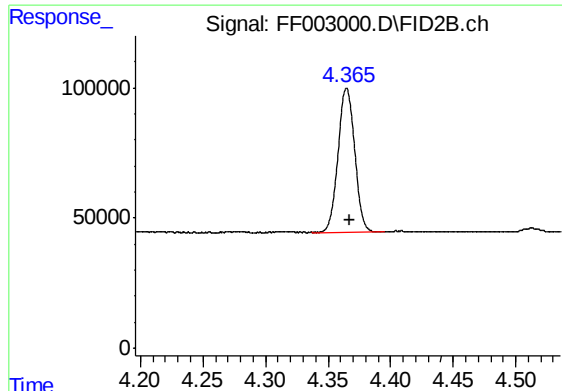


#2 N-DECANE

R.T.: 4.365 min
Delta R.T.: -0.003 min
Response: 512605
Conc: 3.27 ug/ml

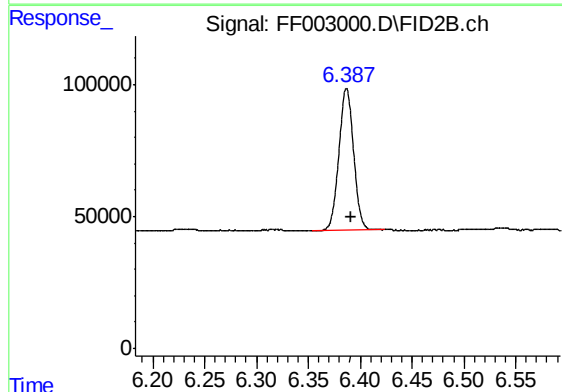


#3 N-DODECANE

R.T.: 6.387 min
Delta R.T.: -0.004 min
Response: 529819
Conc: 3.34 ug/ml

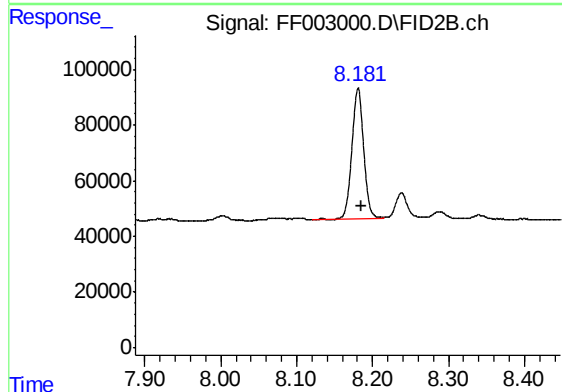


#4 N-TETRADECANE

R.T.: 8.181 min
Delta R.T.: -0.005 min
Response: 504437
Conc: 3.15 ug/ml

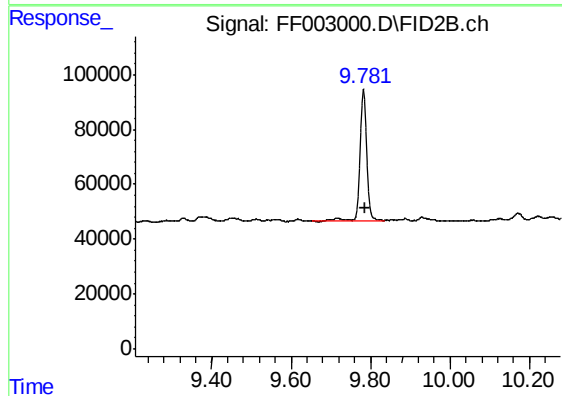


#5 N-HEXADECANE

R.T.: 9.782 min
Delta R.T.: -0.005 min
Response: 564986
Conc: 3.53 ug/ml

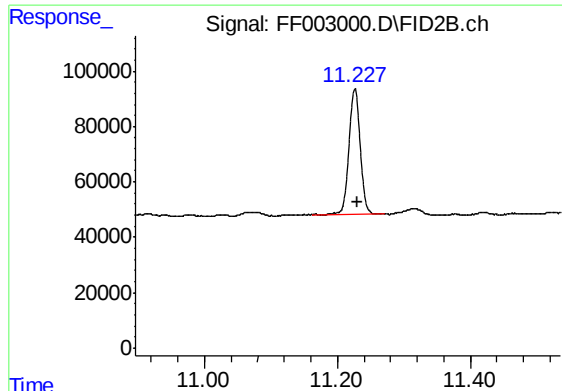


#6 N-OCTADECANE

R.T.: 11.226 min
Delta R.T.: -0.005 min
Response: 529581
Conc: 3.34 ug/ml

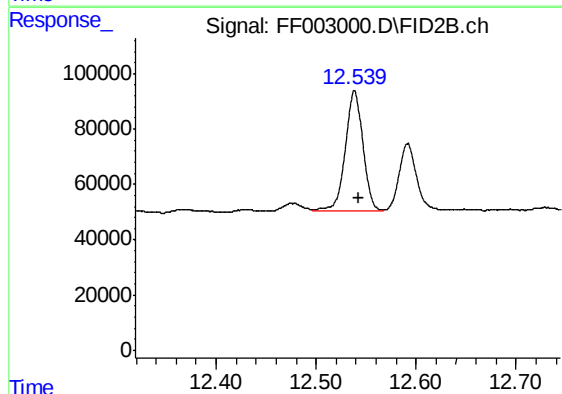


#7 N-EICOSANE

R.T.: 12.538 min
Delta R.T.: -0.005 min
Response: 529458
Conc: 3.43 ug/ml

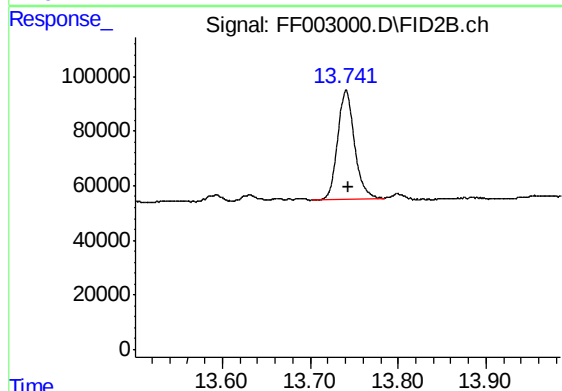


#8 N-DOCOSANE

R.T.: 13.741 min
Delta R.T.: -0.003 min
Response: 536647
Conc: 3.59 ug/ml

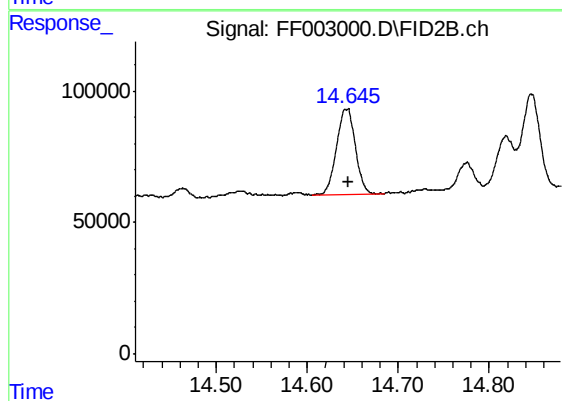


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.643 min
Delta R.T.: -0.002 min
Response: 471522
Conc: 3.63 ug/ml

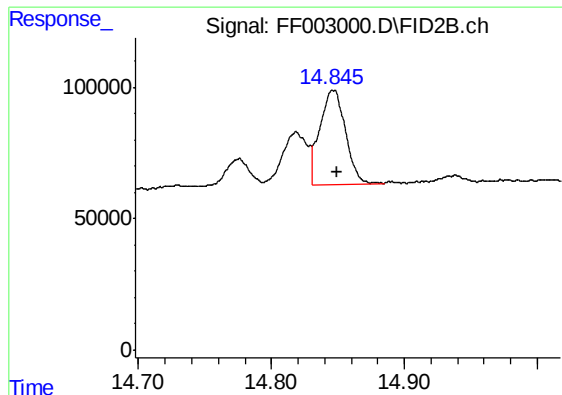


#10 N-TETRACOSANE

R.T.: 14.847 min
Delta R.T.: -0.003 min
Response: 482513
Conc: 3.34 ug/ml

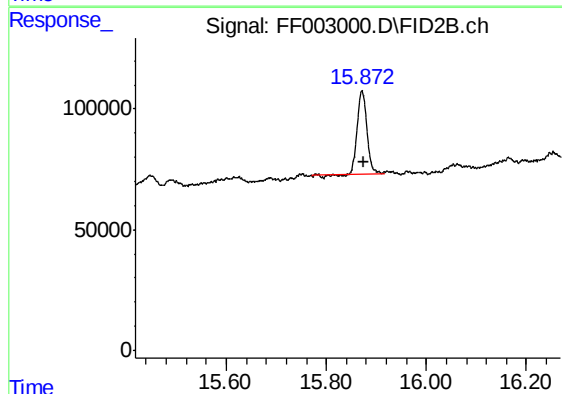

#11 N-HEXACOSANE

R.T.: 15.871 min
Delta R.T.: -0.003 min
Response: 453730
Conc: 3.25 ug/ml

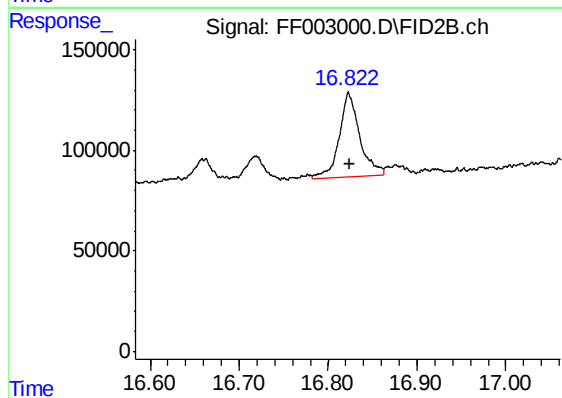

#12 N-OCTACOSANE

R.T.: 16.823 min
Delta R.T.: -0.002 min
Response: 667257
Conc: 4.98 ug/ml