

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121218\
 Data File : FF003003.D
 Signal(s) : FID2B.ch
 Acq On : 12 Dec 2018 12:37
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Dec 12 14:05:19 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.647	5967491	45.966 ug/ml
Target Compounds			
2) N-DECANE	4.367	7930153	50.618 ug/ml
3) N-DODECANE	6.391	7857232	49.480 ug/ml
4) N-TETRADECANE	8.186	7718833	48.156 ug/ml
5) N-HEXADECANE	9.787	7574244	47.296 ug/ml
6) N-OCTADECANE	11.231	7399477	46.709 ug/ml
7) N-EICOSANE	12.543	7135427	46.265 ug/ml
8) N-DOCOSANE	13.745	6875798	45.983 ug/ml
10) N-TETRACOSANE	14.851	6784787	46.949 ug/ml
11) N-HEXACOSANE	15.875	6529993	46.784 ug/ml
12) N-OCTACOSANE	16.828	6479346	48.358 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121218\
Data File : FF003003.D
Signal(s) : FID2B.ch
Acq On : 12 Dec 2018 12:37
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Dec 12 14:05:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

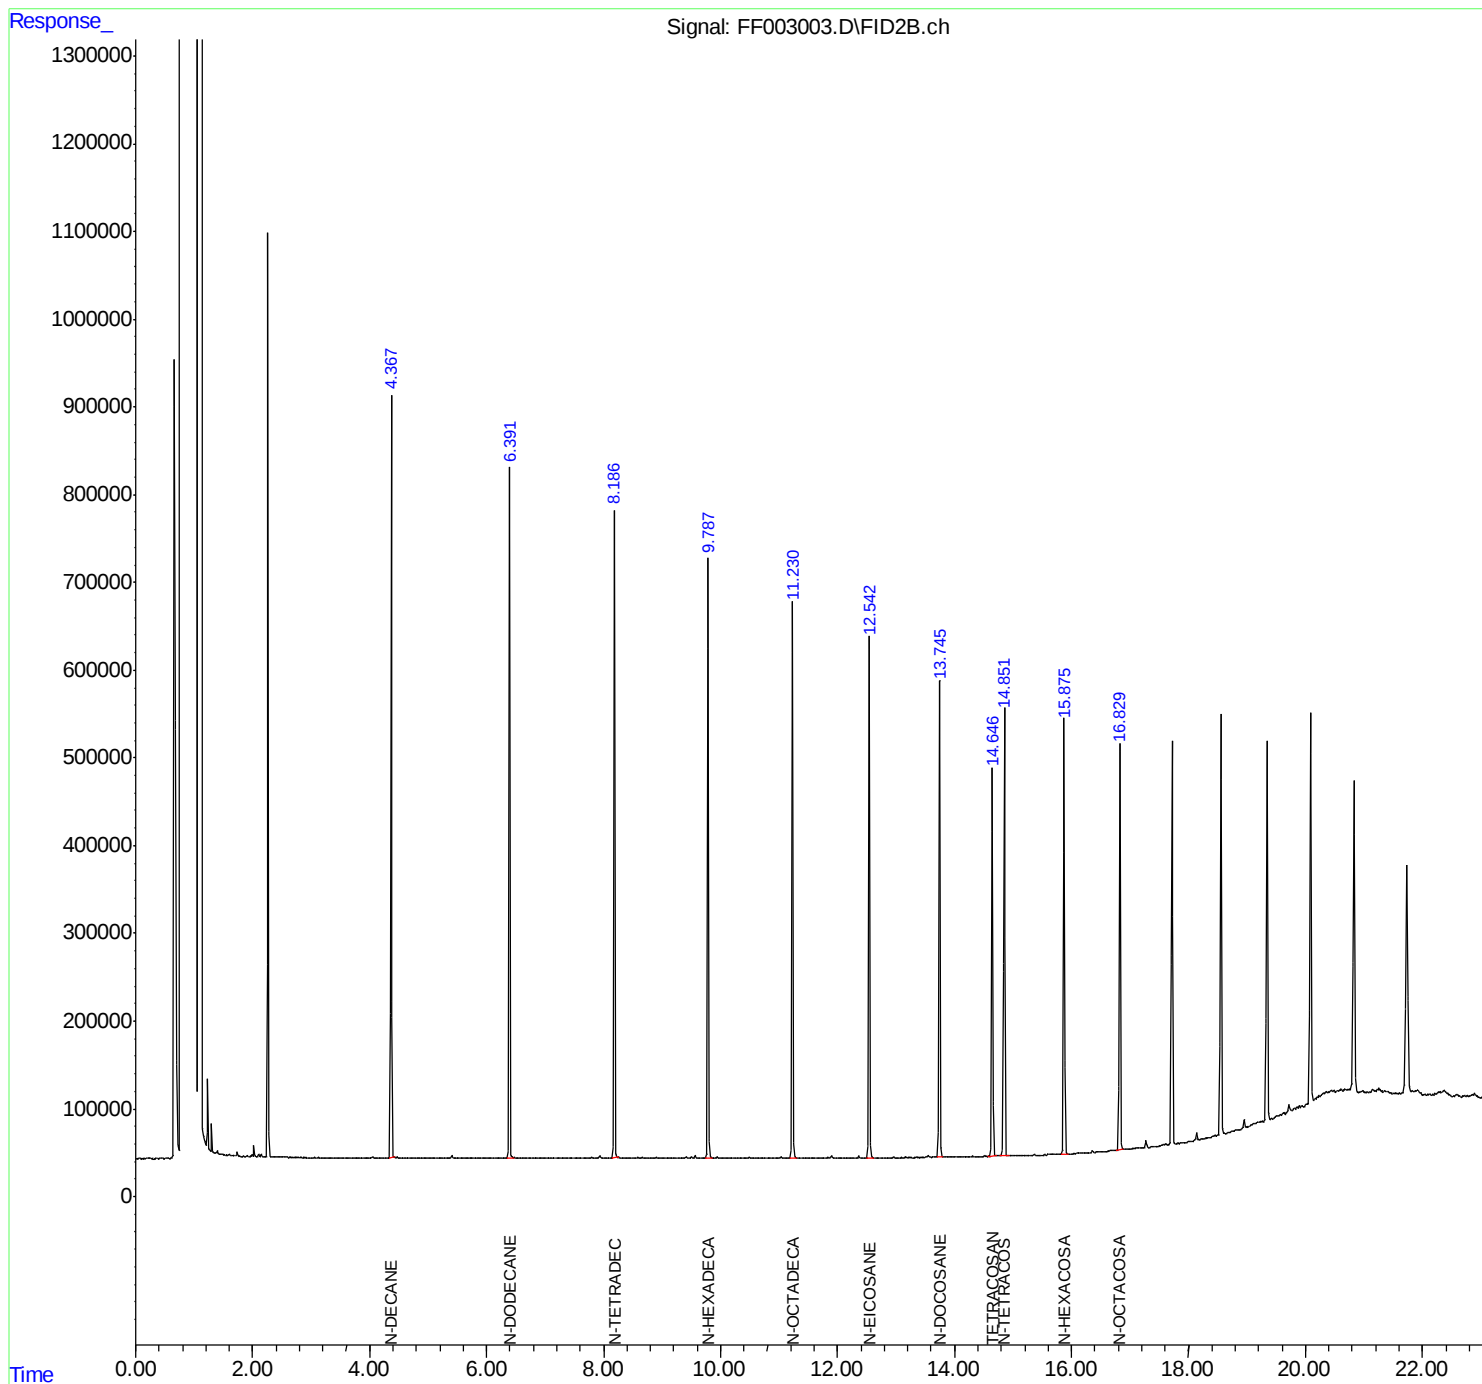

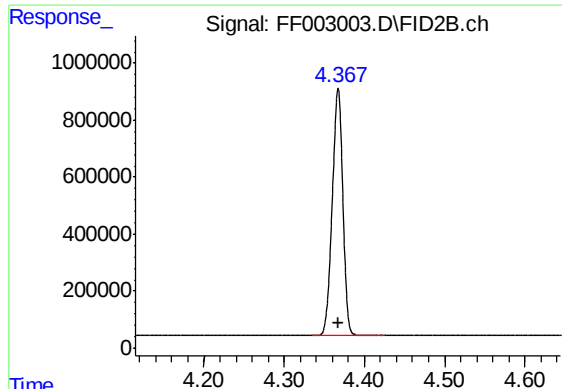


#2 N-DECANE

R.T.: 4.367 min
Delta R.T.: 0.000 min
Response: 7930153
Conc: 50.62 ug/ml

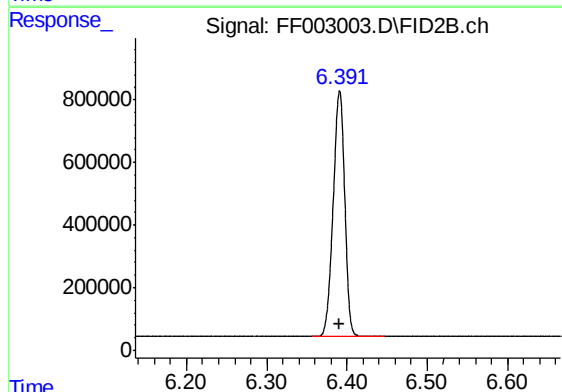


#3 N-DODECANE

R.T.: 6.391 min
Delta R.T.: 0.000 min
Response: 7857232
Conc: 49.48 ug/ml

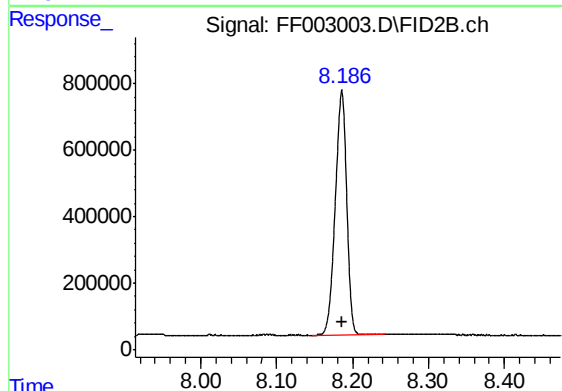


#4 N-TETRADECANE

R.T.: 8.186 min
Delta R.T.: 0.000 min
Response: 7718833
Conc: 48.16 ug/ml

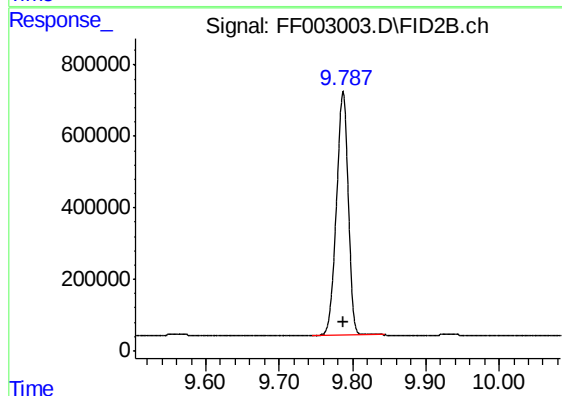


#5 N-HEXADECANE

R.T.: 9.787 min
Delta R.T.: 0.000 min
Response: 7574244
Conc: 47.30 ug/ml

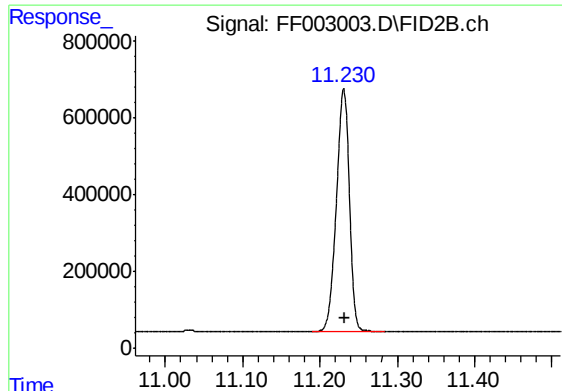


#6 N-OCTADECANE

R.T.: 11.231 min
Delta R.T.: 0.000 min
Response: 7399477
Conc: 46.71 ug/ml

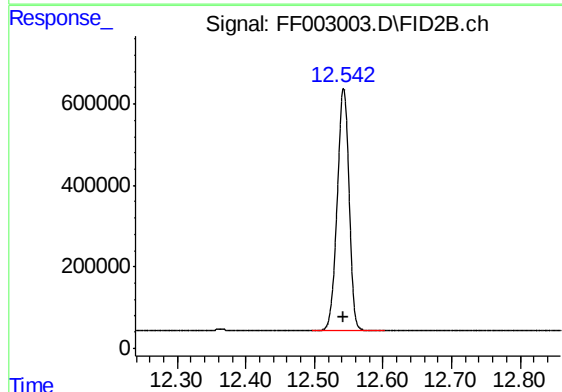


#7 N-EICOSANE

R.T.: 12.543 min
Delta R.T.: 0.000 min
Response: 7135427
Conc: 46.26 ug/ml

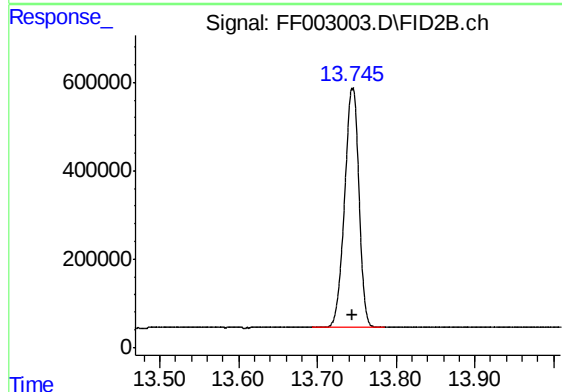


#8 N-DOCOSANE

R.T.: 13.745 min
Delta R.T.: 0.001 min
Response: 6875798
Conc: 45.98 ug/ml

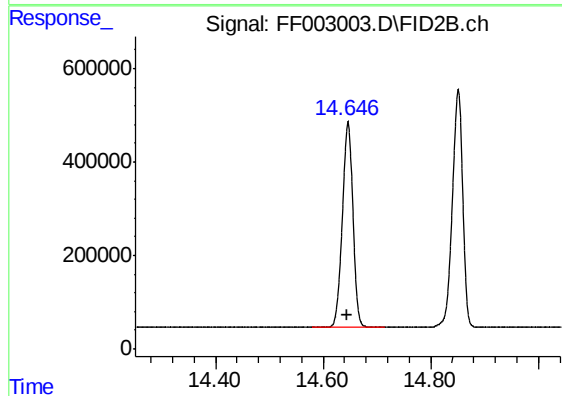


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.647 min
Delta R.T.: 0.001 min
Response: 5967491
Conc: 45.97 ug/ml

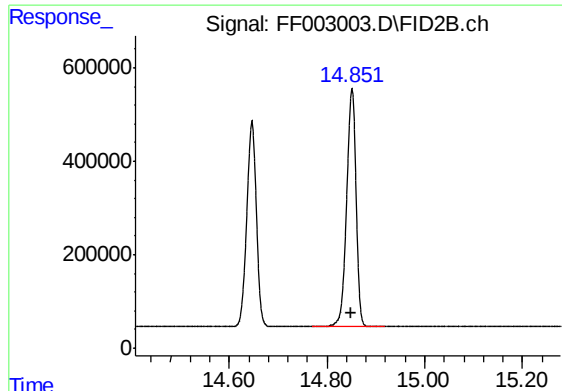


#10 N-TETRACOSANE

R.T.: 14.851 min
Delta R.T.: 0.002 min
Response: 6784787
Conc: 46.95 ug/ml

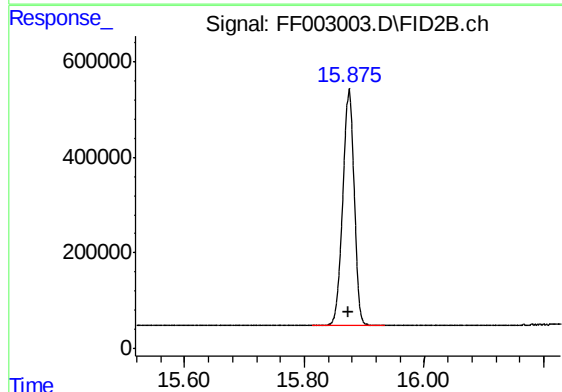

#11 N-HEXACOSANE

R.T.: 15.875 min
Delta R.T.: 0.000 min
Response: 6529993
Conc: 46.78 ug/ml

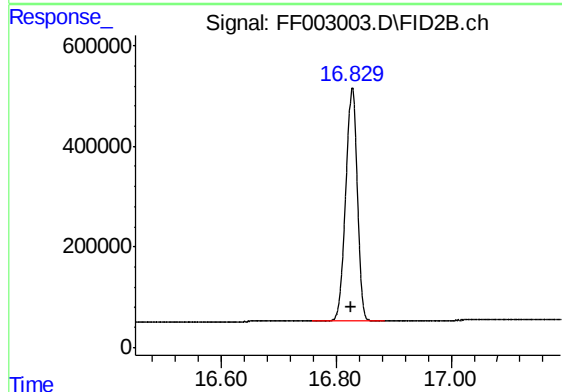

#12 N-OCTACOSANE

R.T.: 16.828 min
Delta R.T.: 0.003 min
Response: 6479346
Conc: 48.36 ug/ml