

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112321\
Data File : FF009383.D
Signal(s) : FID2B.ch
Acq On : 13 Dec 2021 14:52
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 14 01:13:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112321.M
Quant Title :
QLast Update : Wed Nov 24 00:27:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.434	2989464	21.505 ug/ml
12)	N-OCTACOSANE	16.842	2517888	19.768 ug/ml
13)	N-TRIACONTANE	17.729	452556	3.697 ug/ml
14)	N-DOTRIACONTANE	18.561	223248	1.944 ug/ml
15)	N-TETRATRIACONTANE	19.349	37318	0.348 ug/ml
16)	N-HEXATRIACONTANE	20.108	2783	0.028 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121321\
Data File : FF009383.D
Signal(s) : FID2B.ch
Acq On : 13 Dec 2021 14:52
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 14 01:13:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112321.M
Quant Title :
QLast Update : Wed Nov 24 00:27:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

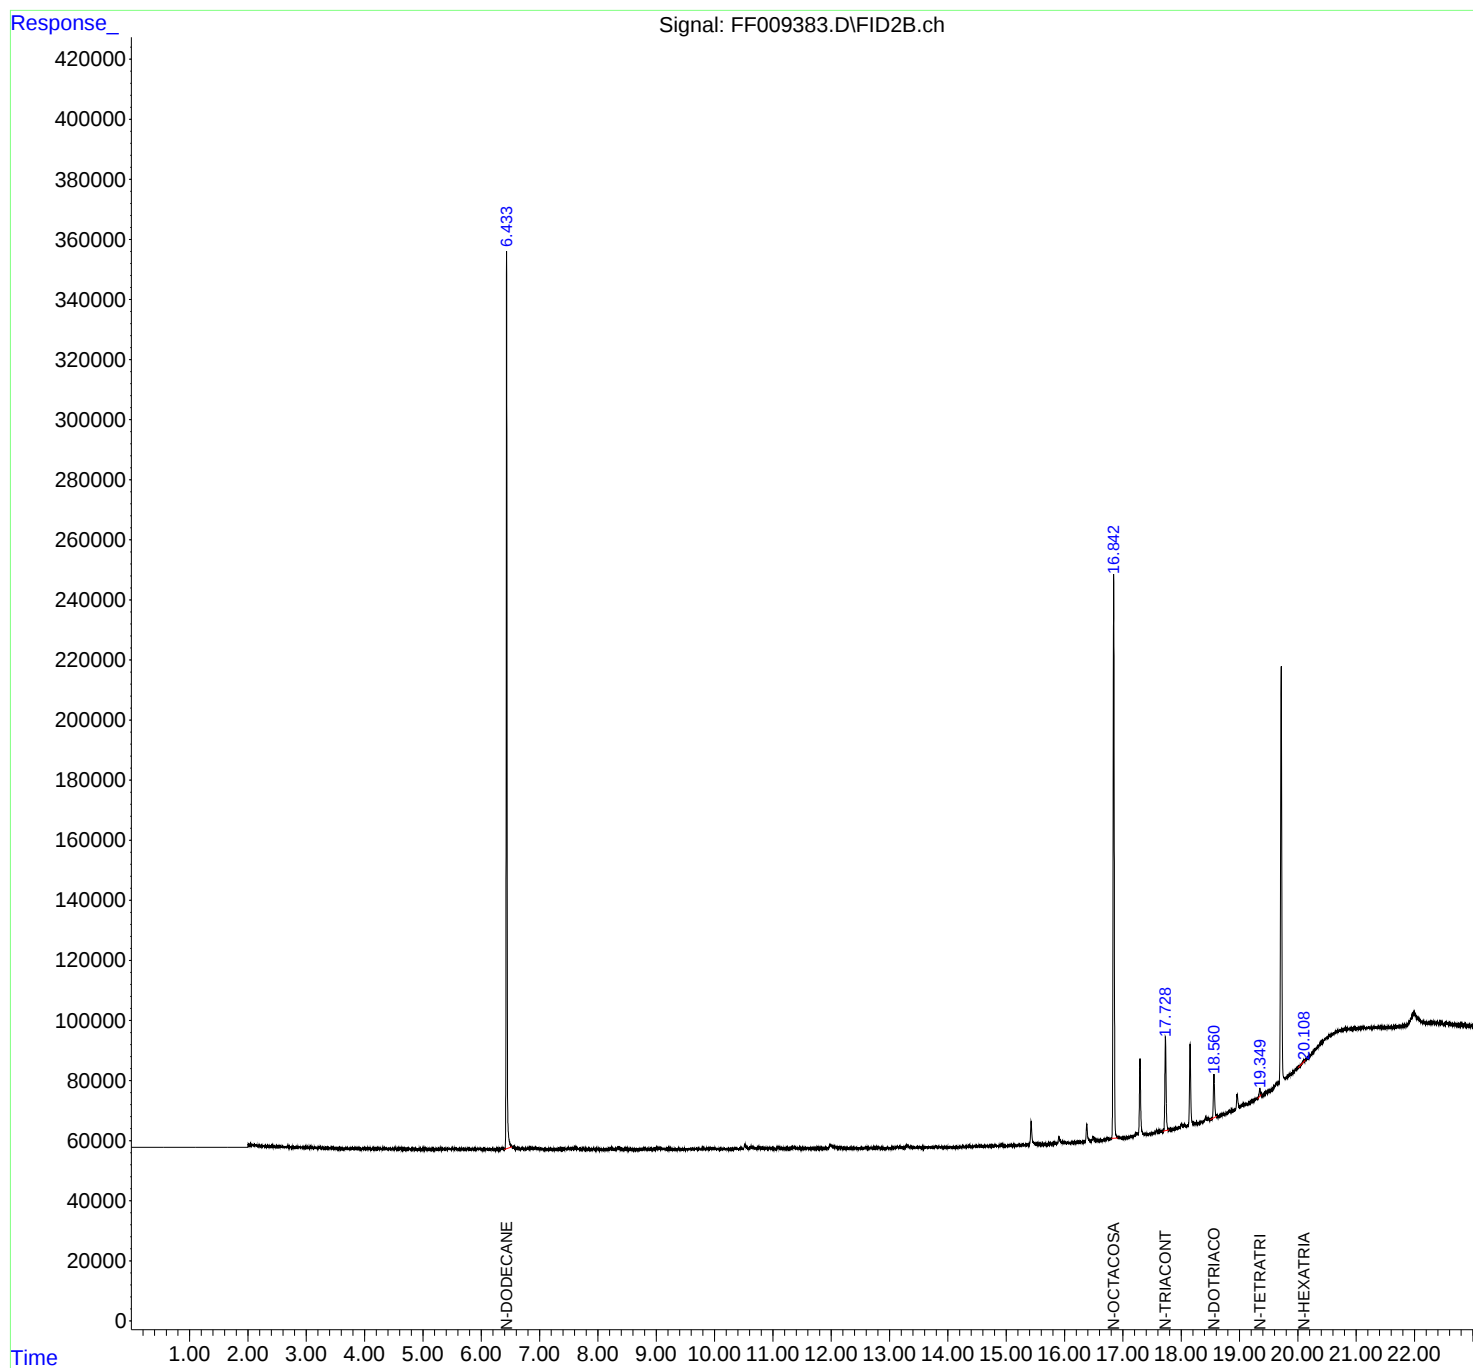


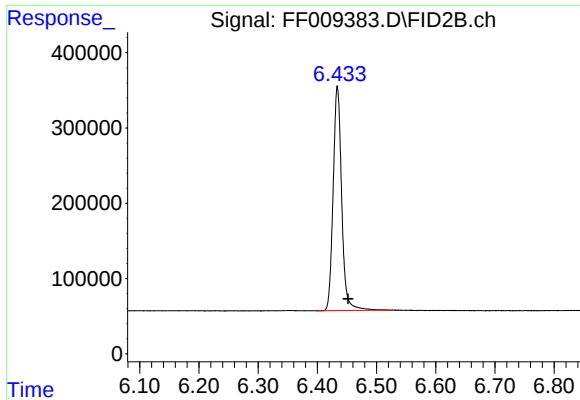

#3 N-DODECANE


R.T.: 6.434 min
Delta R.T.: -0.018 min
Response: 2989464
Conc: 21.50 ug/ml

Instrument :
FID_F
ClientSampleId :

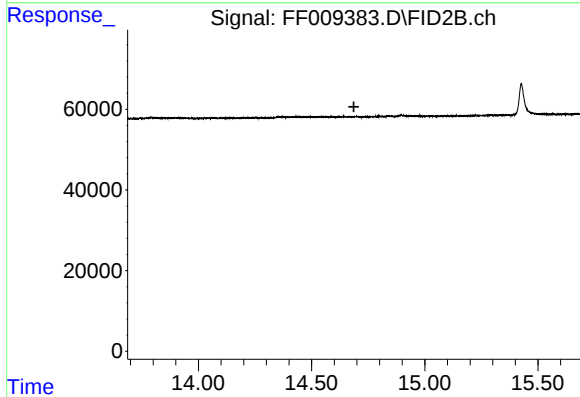


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.687 min
Response: 0
Conc: N.D.

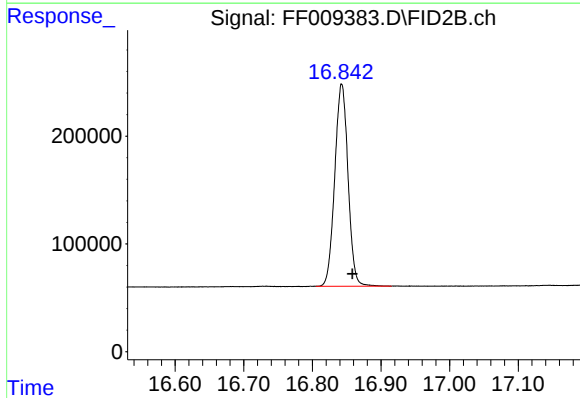


#12 N-OCTACOSANE

R.T.: 16.842 min
Delta R.T.: -0.016 min
Response: 2517888
Conc: 19.77 ug/ml

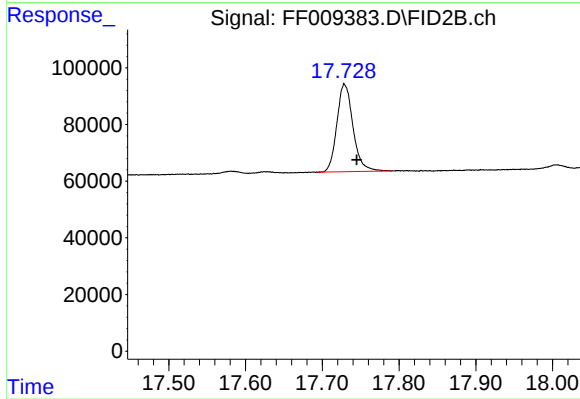

#13 N-TRIACONTANE


R.T.: 17.729 min
Delta R.T.: -0.016 min
Response: 452556
Conc: 3.70 ug/ml

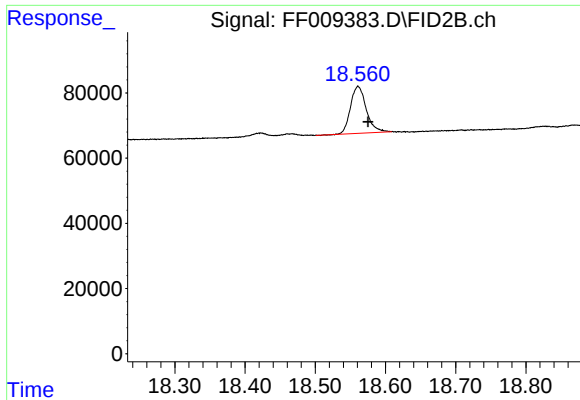

#14 N-DOTRIACONTANE


R.T.: 18.561 min
Delta R.T.: -0.014 min
Response: 223248
Conc: 1.94 ug/ml

Instrument :
FID_F
ClientSampleId :

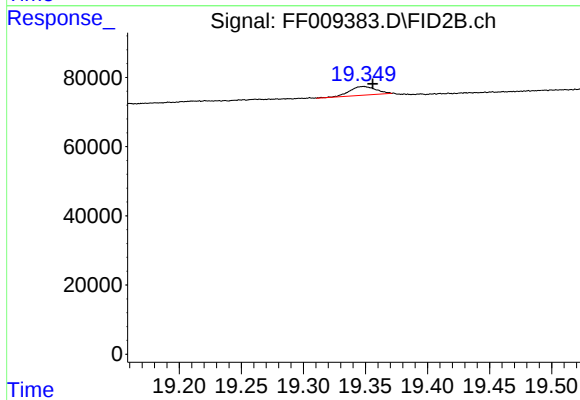

#15 N-TETRATRIACONTANE

R.T.: 19.349 min
Delta R.T.: -0.007 min
Response: 37318
Conc: 0.35 ug/ml

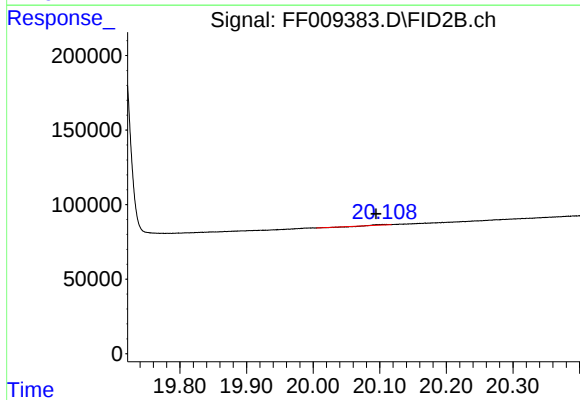

#16 N-HEXATRIACONTANE

R.T.: 20.108 min
Delta R.T.: 0.013 min
Response: 2783
Conc: 0.03 ug/ml