

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121322\
 Data File : FF011788.D
 Signal(s) : FID2B.ch
 Acq On : 13 Dec 2022 08:11
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 14 03:02:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
 Quant Title :
 QLast Update : Tue Dec 06 04:24:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.014f	68826	0.603 ug/ml
Target Compounds			
7) N-EICOSANE	12.940	289815	2.141 ug/ml
8) N-DOCOSANE	14.144	339709	2.564 ug/ml
10) N-TETRACOSANE	15.234	1812156	13.783 ug/ml
11) N-HEXACOSANE	16.275	226166	1.784 ug/ml
12) N-OCTACOSANE	17.226	124084	1.007 ug/ml
13) N-TRIACONTANE	18.113	126367	1.043 ug/ml
14) N-DOTRIACONTANE	18.949	245006	2.036 ug/ml
15) N-TETRATRIACONTANE	19.715	253386	2.138 ug/ml
16) N-HEXATRIACONTANE	20.469	33836	0.291 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121322\
Data File : FF011788.D
Signal(s) : FID2B.ch
Acq On : 13 Dec 2022 08:11
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 14 03:02:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

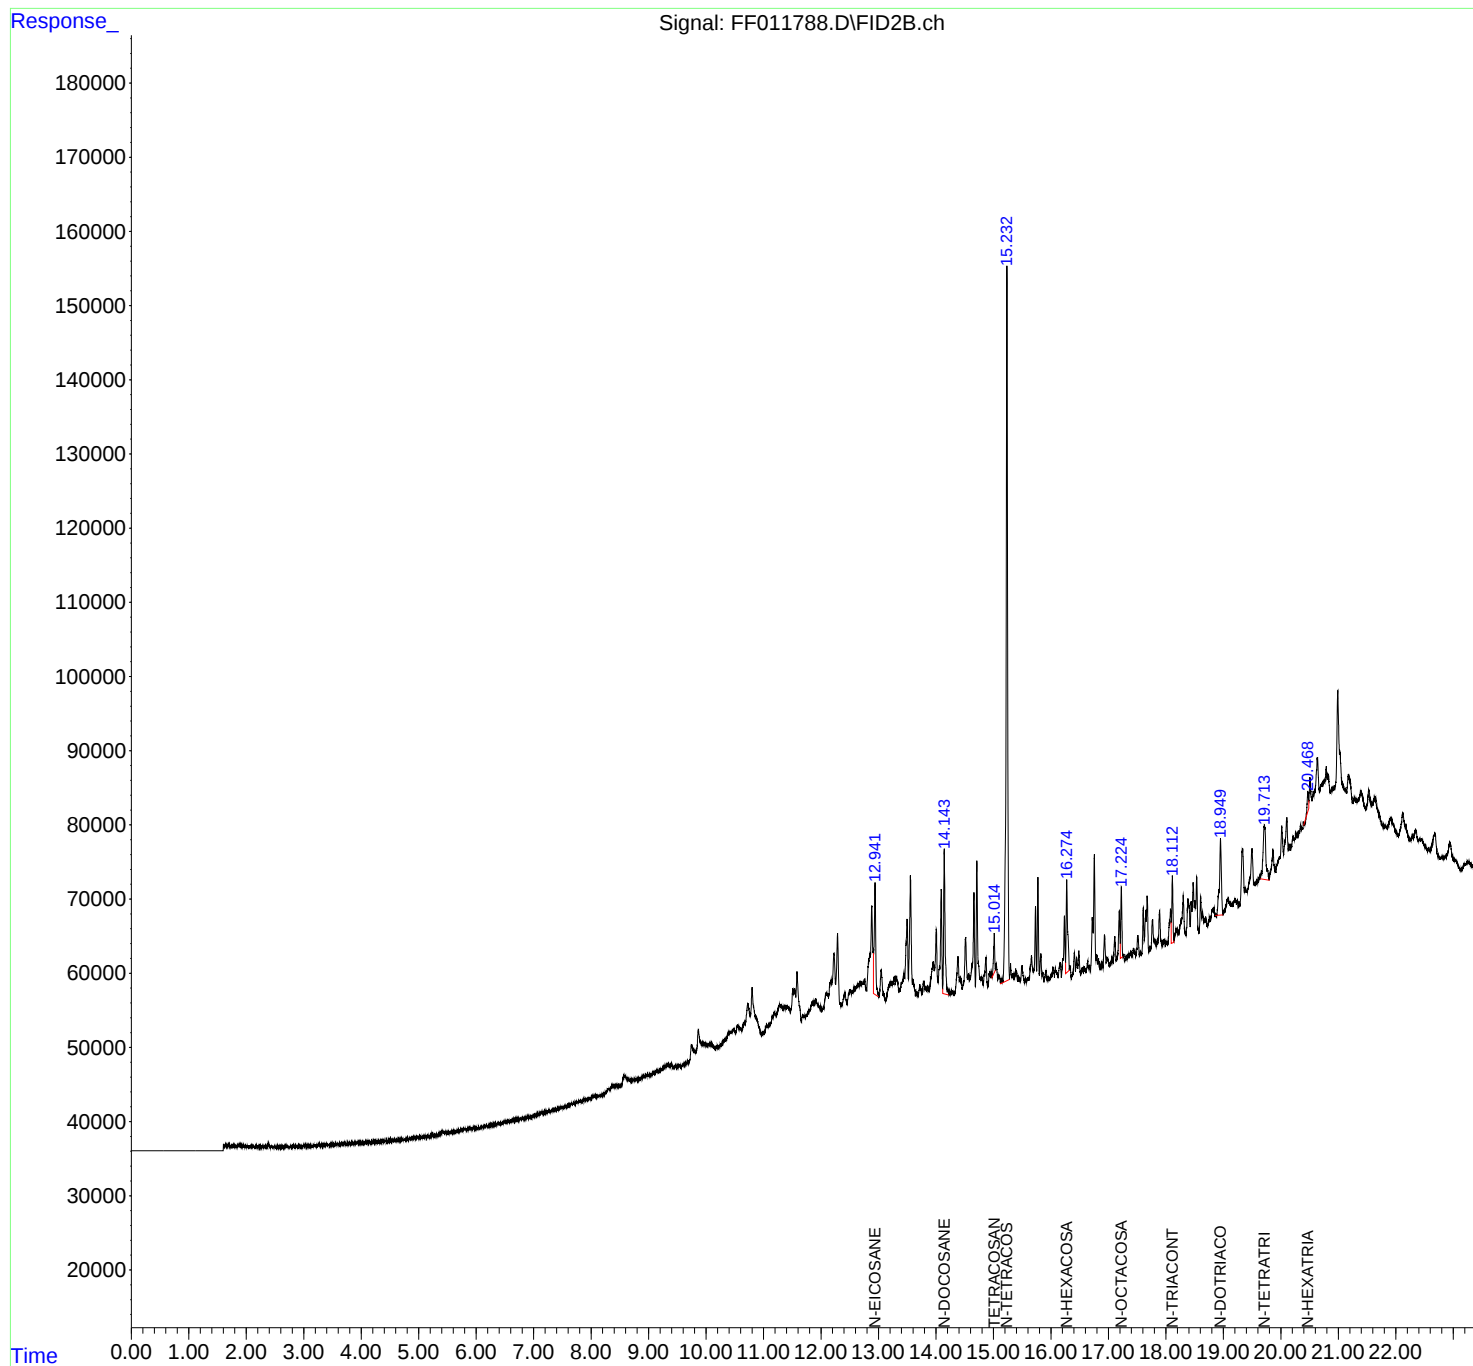


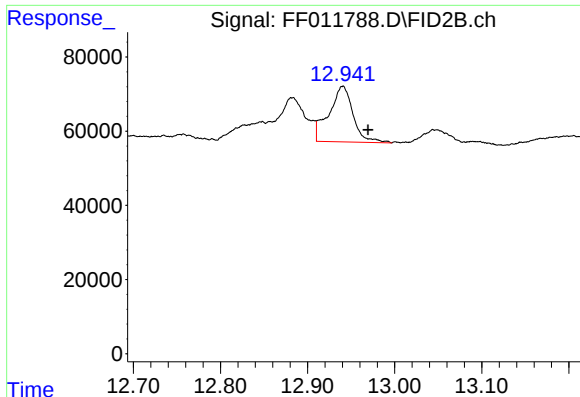

#7 N-EICOSANE


R.T.: 12.940 min
Delta R.T.: -0.029 min
Response: 289815
Conc: 2.14 ug/ml

Instrument :
FID_F
ClientSampleId :

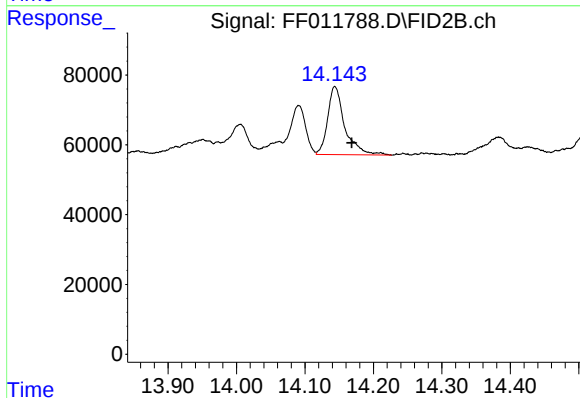


#8 N-DOCOSANE

R.T.: 14.144 min
Delta R.T.: -0.025 min
Response: 339709
Conc: 2.56 ug/ml

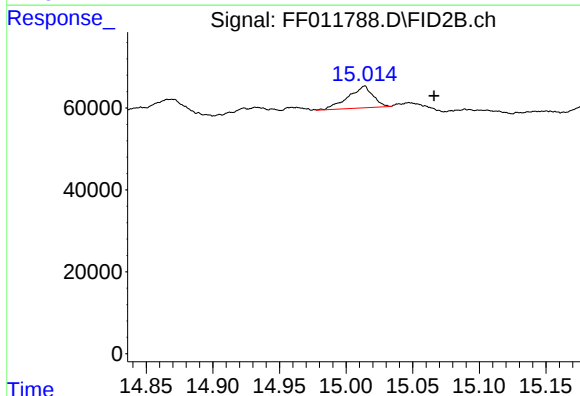


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.014 min
Delta R.T.: -0.052 min
Response: 68826
Conc: 0.60 ug/ml

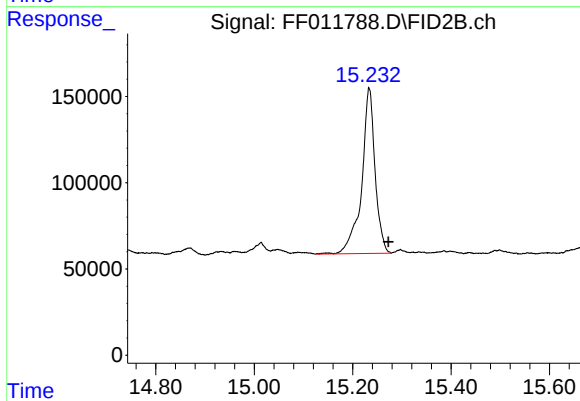

#10 N-TETRACOSANE


R.T.: 15.234 min
Delta R.T.: -0.039 min
Response: 1812156
Conc: 13.78 ug/ml

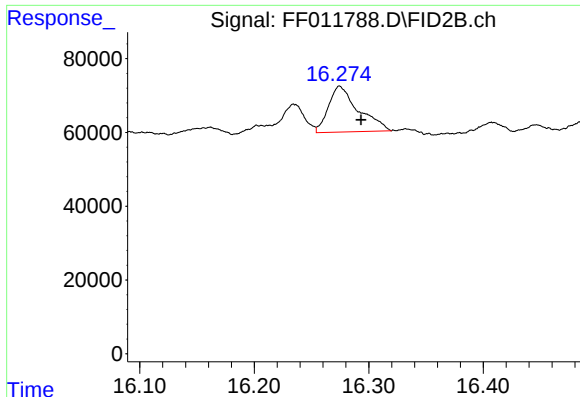

#11 N-HEXACOSANE


R.T.: 16.275 min
Delta R.T.: -0.019 min
Response: 226166
Conc: 1.78 ug/ml

Instrument :
FID_F
ClientSampleId :

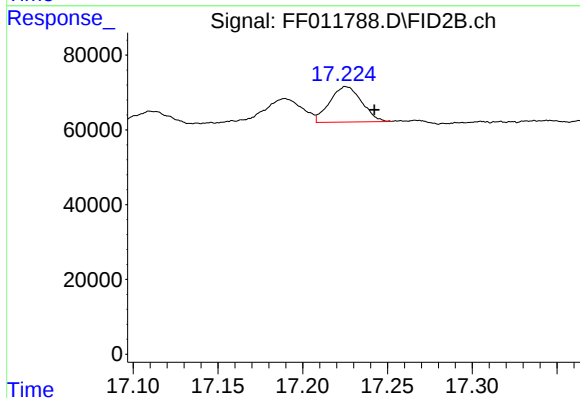


#12 N-OCTACOSANE

R.T.: 17.226 min
Delta R.T.: -0.017 min
Response: 124084
Conc: 1.01 ug/ml

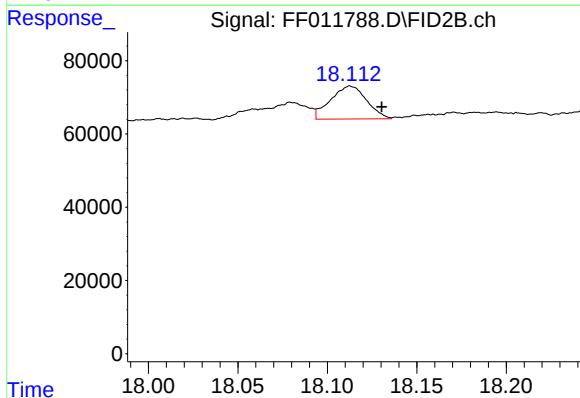


#13 N-TRIACONTANE

R.T.: 18.113 min
Delta R.T.: -0.018 min
Response: 126367
Conc: 1.04 ug/ml

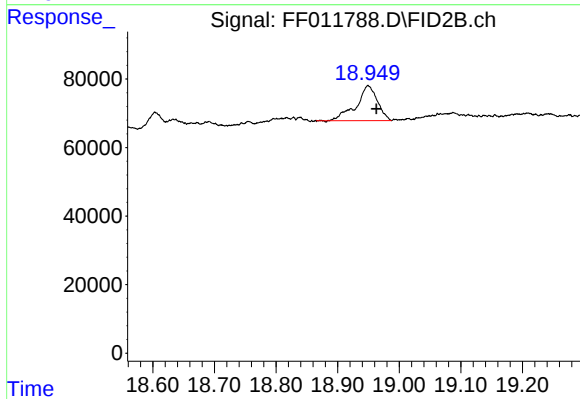

#14 N-DOTRIACONTANE


R.T.: 18.949 min
Delta R.T.: -0.013 min
Response: 245006
Conc: 2.04 ug/ml

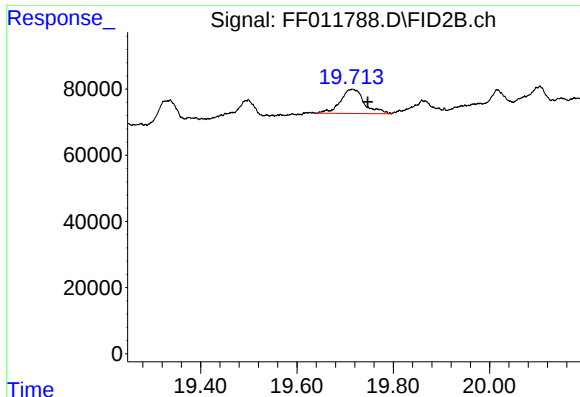

#15 N-TETRATRIACONTANE

R.T.: 19.715 min
Delta R.T.: -0.032 min
Response: 253386
Conc: 2.14 ug/ml

Instrument :
FID_F
ClientSampleId :

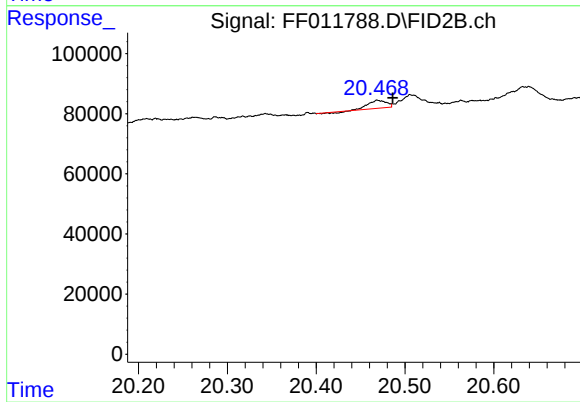

#16 N-HEXATRIACONTANE

R.T.: 20.469 min
Delta R.T.: -0.017 min
Response: 33836
Conc: 0.29 ug/ml