

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121322\
Data File : FF011789.D
Signal(s) : FID2B.ch
Acq On : 13 Dec 2022 08:40
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 14 03:02:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.052	2208282	19.340 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.113	94637	0.781 ug/ml
14) N-DOTRIACONTANE	18.945	132163	1.098 ug/ml
15) N-TETRATRIACONTANE	19.729	115480	0.974 ug/ml
16) N-HEXATRIACONTANE	20.470	52746	0.453 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121322\
Data File : FF011789.D
Signal(s) : FID2B.ch
Acq On : 13 Dec 2022 08:40
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 14 03:02:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

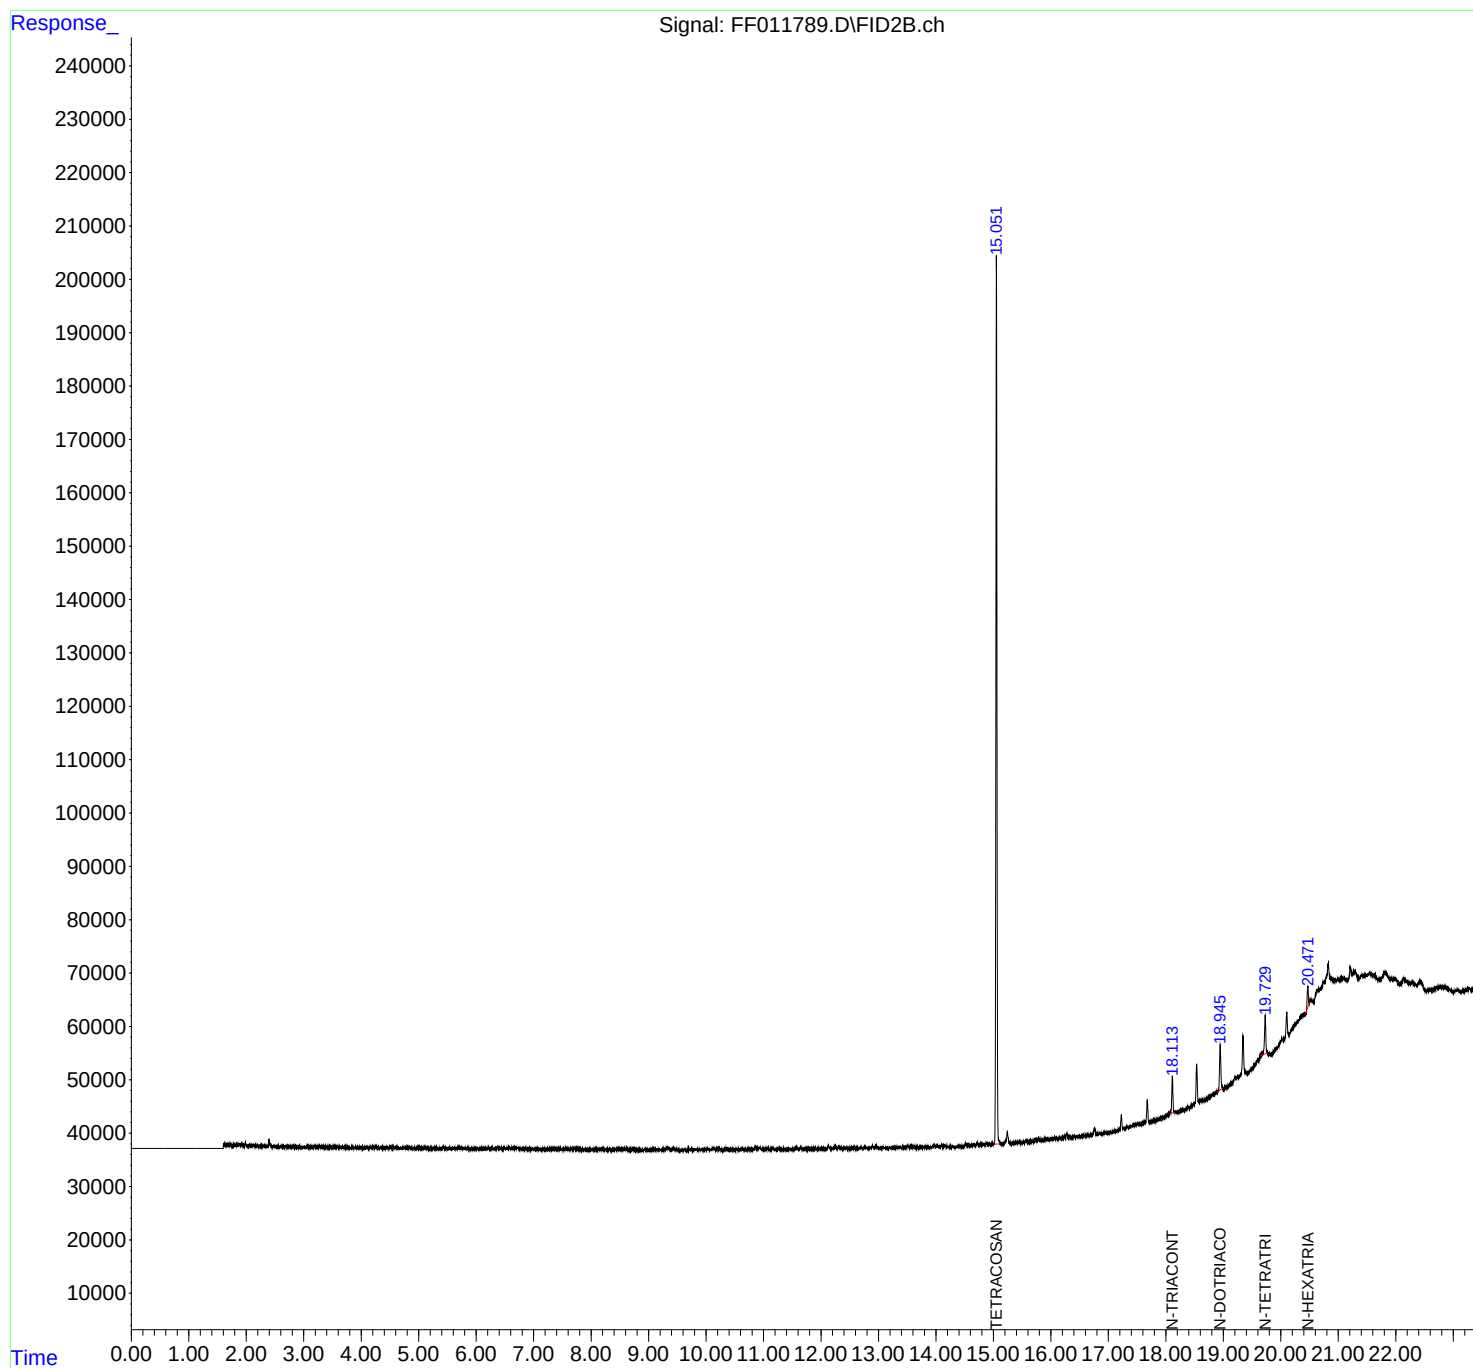


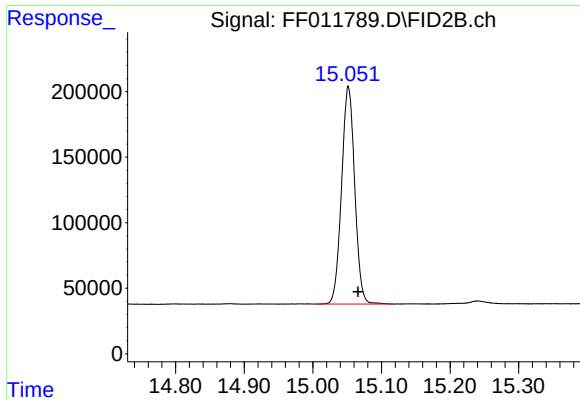

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.052 min
Delta R.T.: -0.014 min
Response: 2208282
Conc: 19.34 ug/ml

Instrument :
FID_F
ClientSampleId :

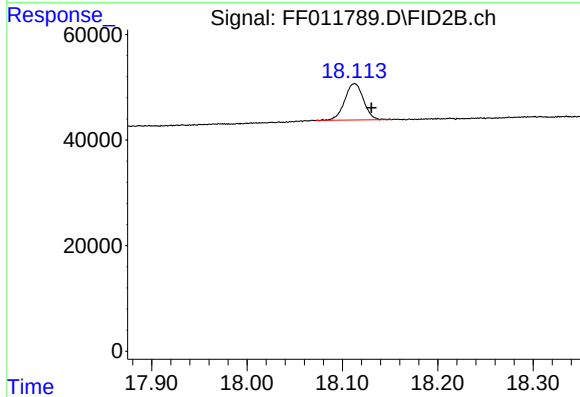


#13 N-TRIACONTANE

R.T.: 18.113 min
Delta R.T.: -0.018 min
Response: 94637
Conc: 0.78 ug/ml

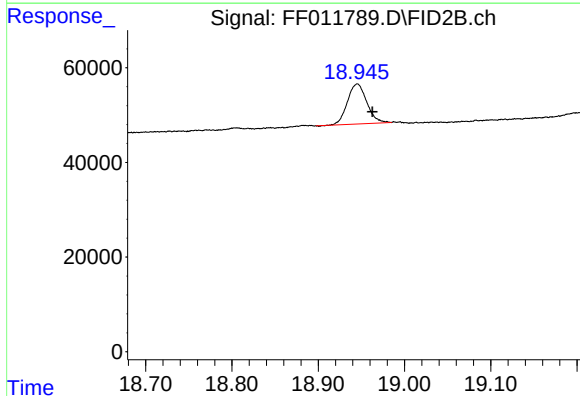


#14 N-DOTRIACONTANE

R.T.: 18.945 min
Delta R.T.: -0.017 min
Response: 132163
Conc: 1.10 ug/ml

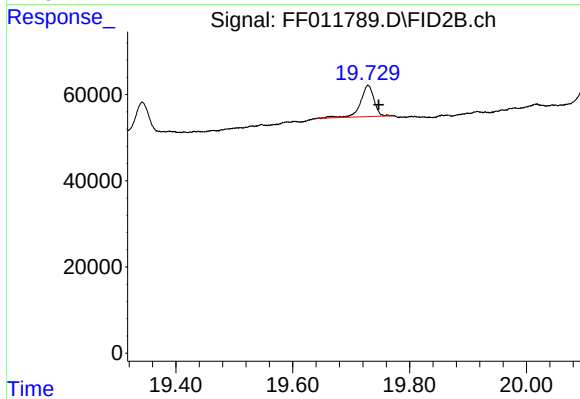

#15 N-TETRATRIACONTANE

R.T.: 19.729 min
Delta R.T.: -0.018 min
Response: 115480
Conc: 0.97 ug/ml

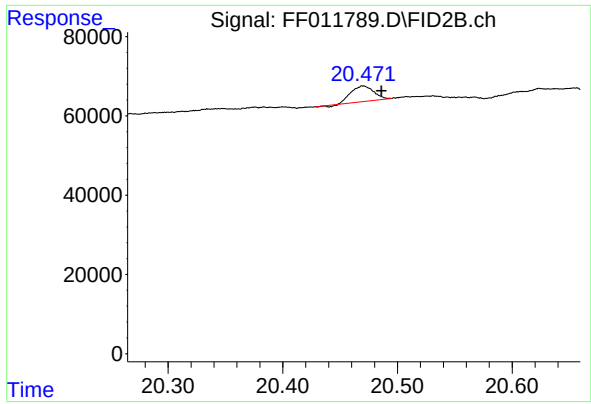

#16 N-HEXATRIACONTANE

R.T.: 20.470 min
Delta R.T.: -0.016 min
Response: 52746
Conc: 0.45 ug/ml

Instrument :

FID_F

ClientSampleId :