

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121322\
 Data File : FF011791.D
 Signal(s) : FID2B.ch
 Acq On : 13 Dec 2022 09:38
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 14 03:02:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
 Quant Title :
 QLast Update : Tue Dec 06 04:24:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.773	2535499	18.360 ug/ml
12)	N-OCTACOSANE	17.227	2348308	19.051 ug/ml
13)	N-TRIACONTANE	18.113	314321	2.594 ug/ml
14)	N-DOTRIACONTANE	18.946	415153	3.450 ug/ml
15)	N-TETRATRIACONTANE	19.729	347465	2.932 ug/ml
16)	N-HEXATRIACONTANE	20.468	226476	1.947 ug/ml
17)	N-OCTATRIACONTANE	21.208	158569	1.312 ug/ml
18)	N-TETRACONTANE	22.132	239562	1.837 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121322\
Data File : FF011791.D
Signal(s) : FID2B.ch
Acq On : 13 Dec 2022 09:38
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 14 03:02:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

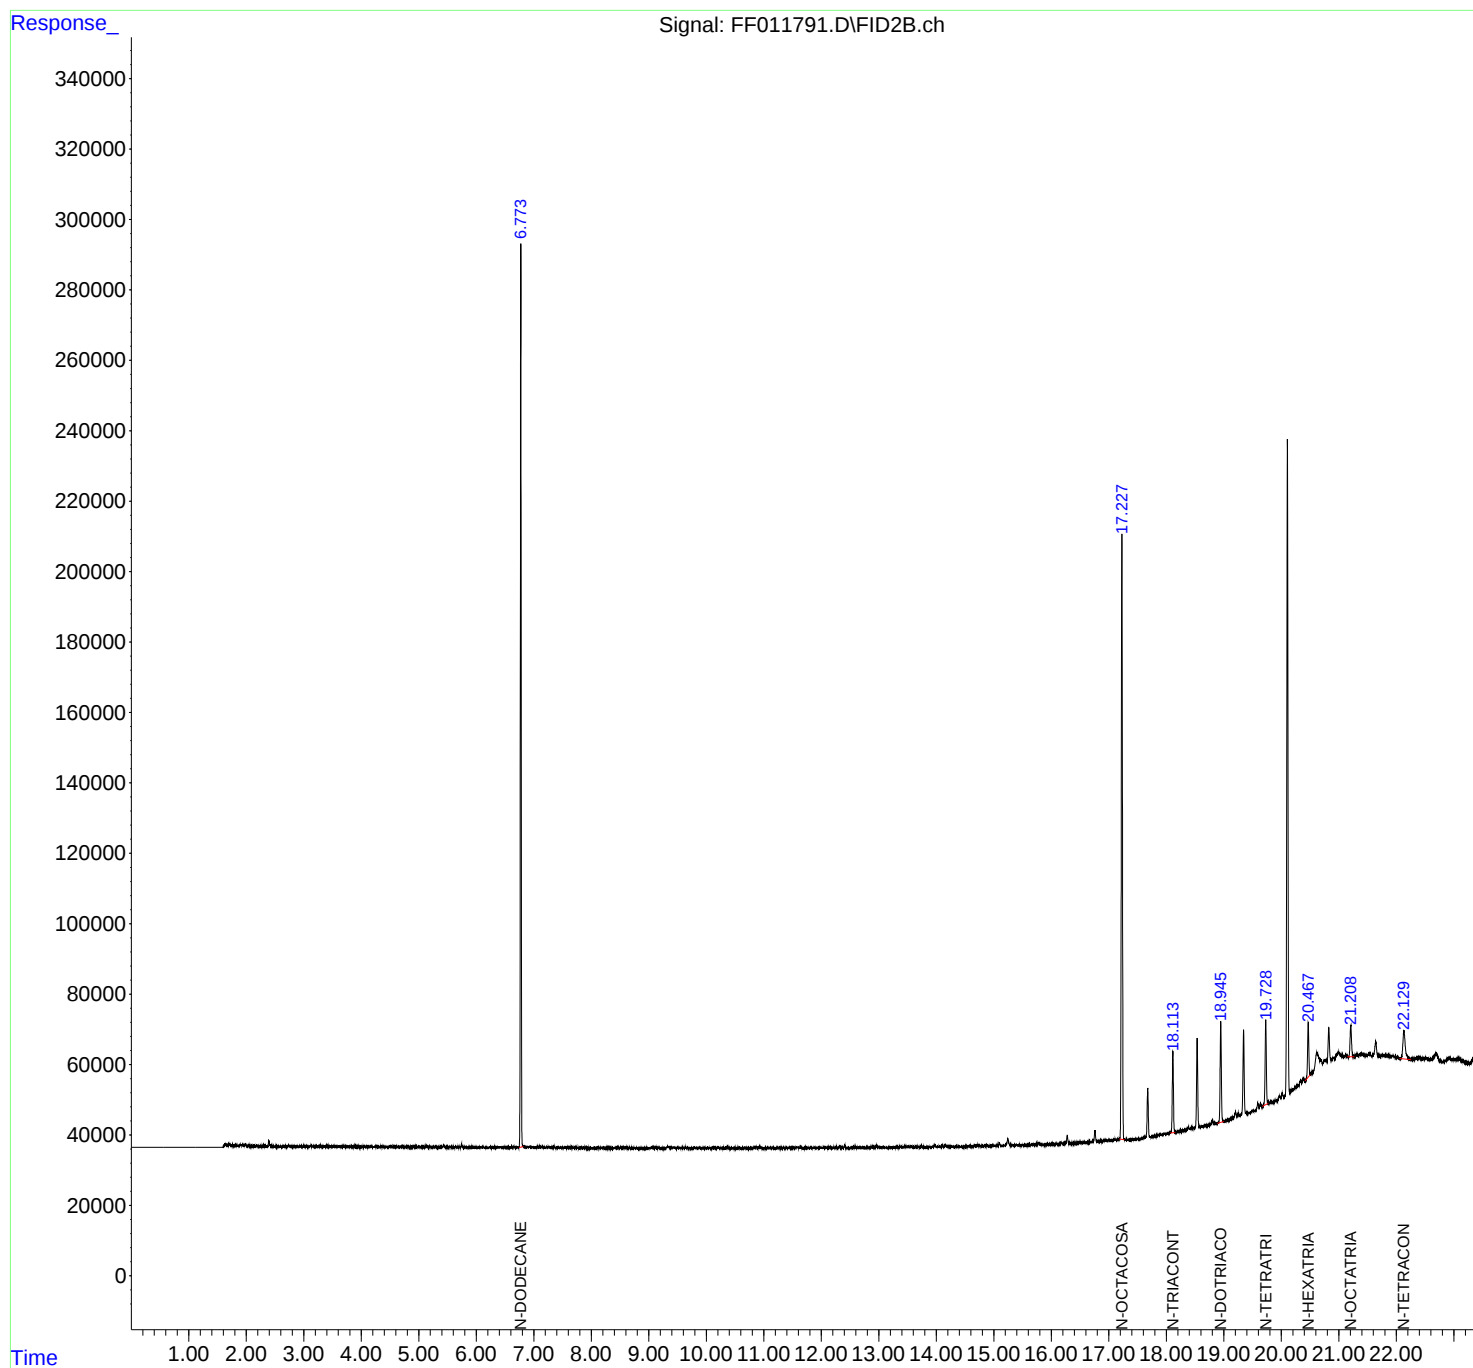


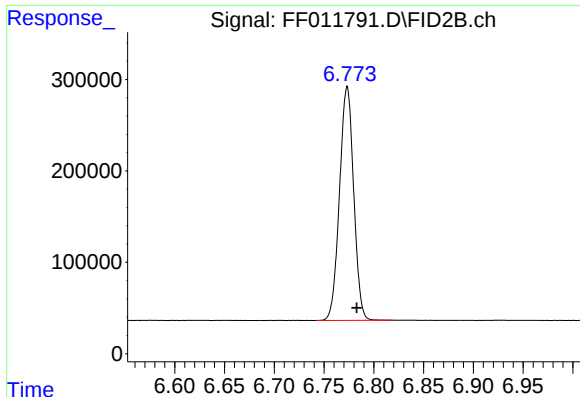

#3 N-DODECANE


R.T.: 6.773 min
Delta R.T.: -0.010 min
Response: 2535499
Conc: 18.36 ug/ml

Instrument :
FID_F
ClientSampleId :

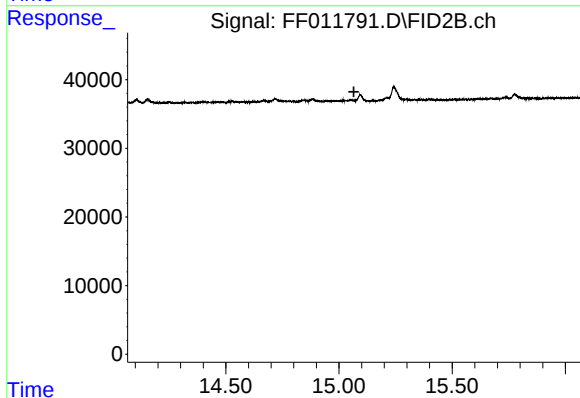


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.066 min
Response: 0
Conc: N.D.

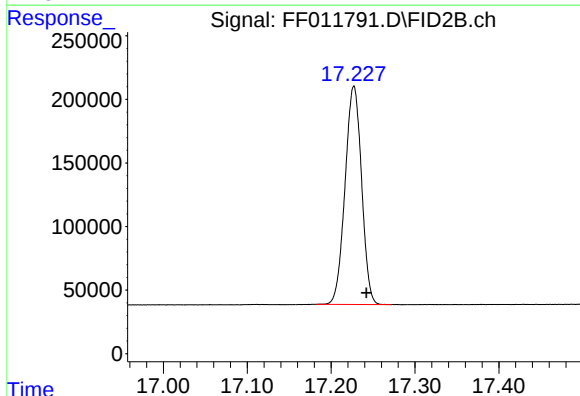


#12 N-OCTACOSANE

R.T.: 17.227 min
Delta R.T.: -0.015 min
Response: 2348308
Conc: 19.05 ug/ml

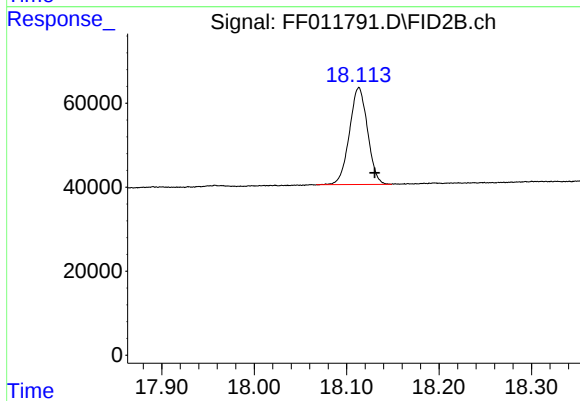

#13 N-TRIACONTANE


R.T.: 18.113 min
Delta R.T.: -0.017 min
Response: 314321
Conc: 2.59 ug/ml

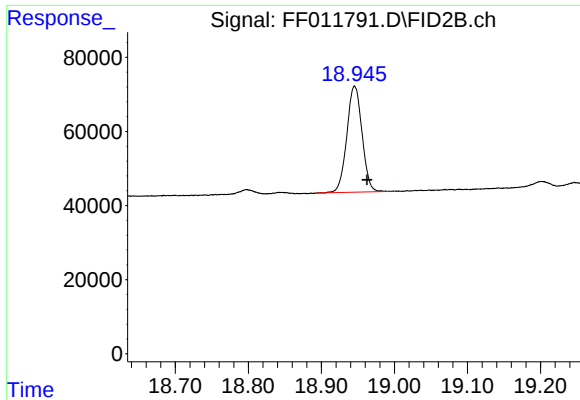

#14 N-DOTRIACONTANE


R.T.: 18.946 min
Delta R.T.: -0.017 min
Response: 415153
Conc: 3.45 ug/ml

Instrument :
FID_F
ClientSampleId :

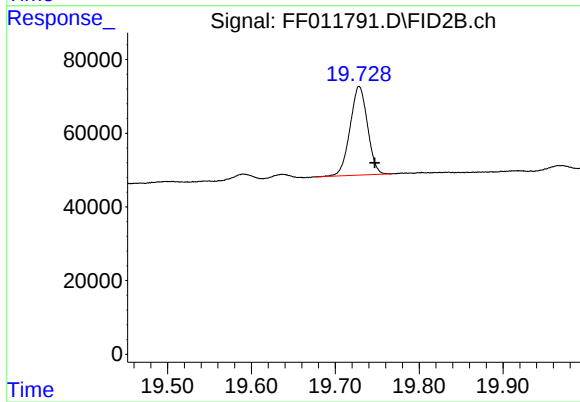


#15 N-TETRATRIACONTANE

R.T.: 19.729 min
Delta R.T.: -0.019 min
Response: 347465
Conc: 2.93 ug/ml

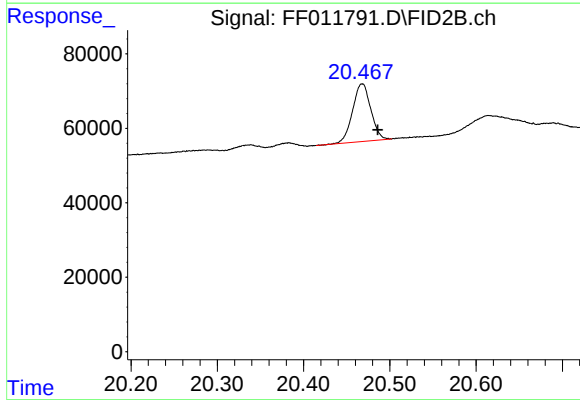


#16 N-HEXATRIACONTANE

R.T.: 20.468 min
Delta R.T.: -0.018 min
Response: 226476
Conc: 1.95 ug/ml

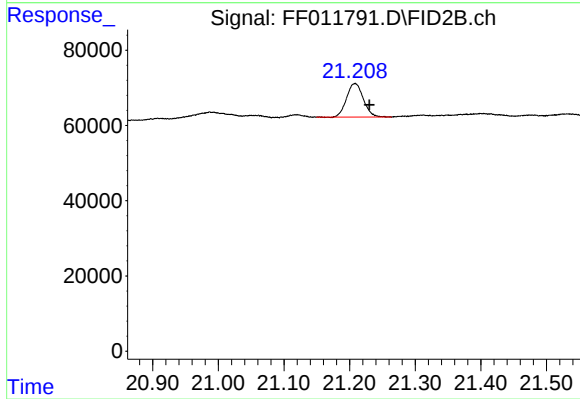

#17 N-OCTATRIACONTANE

R.T.: 21.208 min
Delta R.T.: -0.022 min
Response: 158569
Conc: 1.31 ug/ml

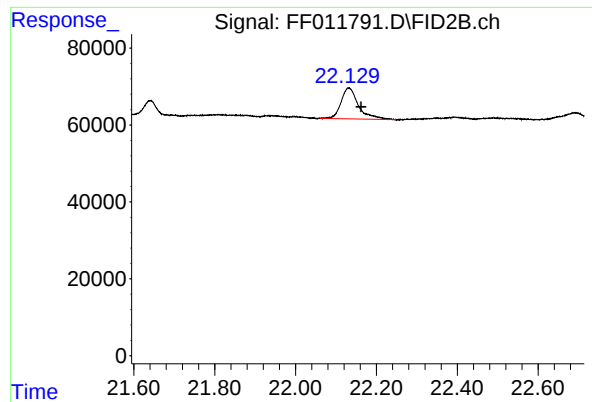

#18 N-TETRACONTANE

R.T.: 22.132 min
Delta R.T.: -0.030 min
Response: 239562
Conc: 1.84 ug/ml

Instrument :

FID_F

ClientSampleId :