

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121322\
Data File : FF011804.D
Signal(s) : FID2B.ch
Acq On : 13 Dec 2022 16:10
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 14 03:05:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.772	2347140	16.996 ug/ml
12)	N-OCTACOSANE	17.226	2226481	18.063 ug/ml
13)	N-TRIACONTANE	18.112	372925	3.078 ug/ml
14)	N-DOTRIACONTANE	18.944	487192	4.048 ug/ml
15)	N-TETRATRIACONTANE	19.727	400345	3.378 ug/ml
16)	N-HEXATRIACONTANE	20.466	266984	2.295 ug/ml
17)	N-OCTATRIACONTANE	21.207	205427	1.700 ug/ml
18)	N-TETRACONTANE	22.128	236244	1.811 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121322\
Data File : FF011804.D
Signal(s) : FID2B.ch
Acq On : 13 Dec 2022 16:10
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 14 03:05:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

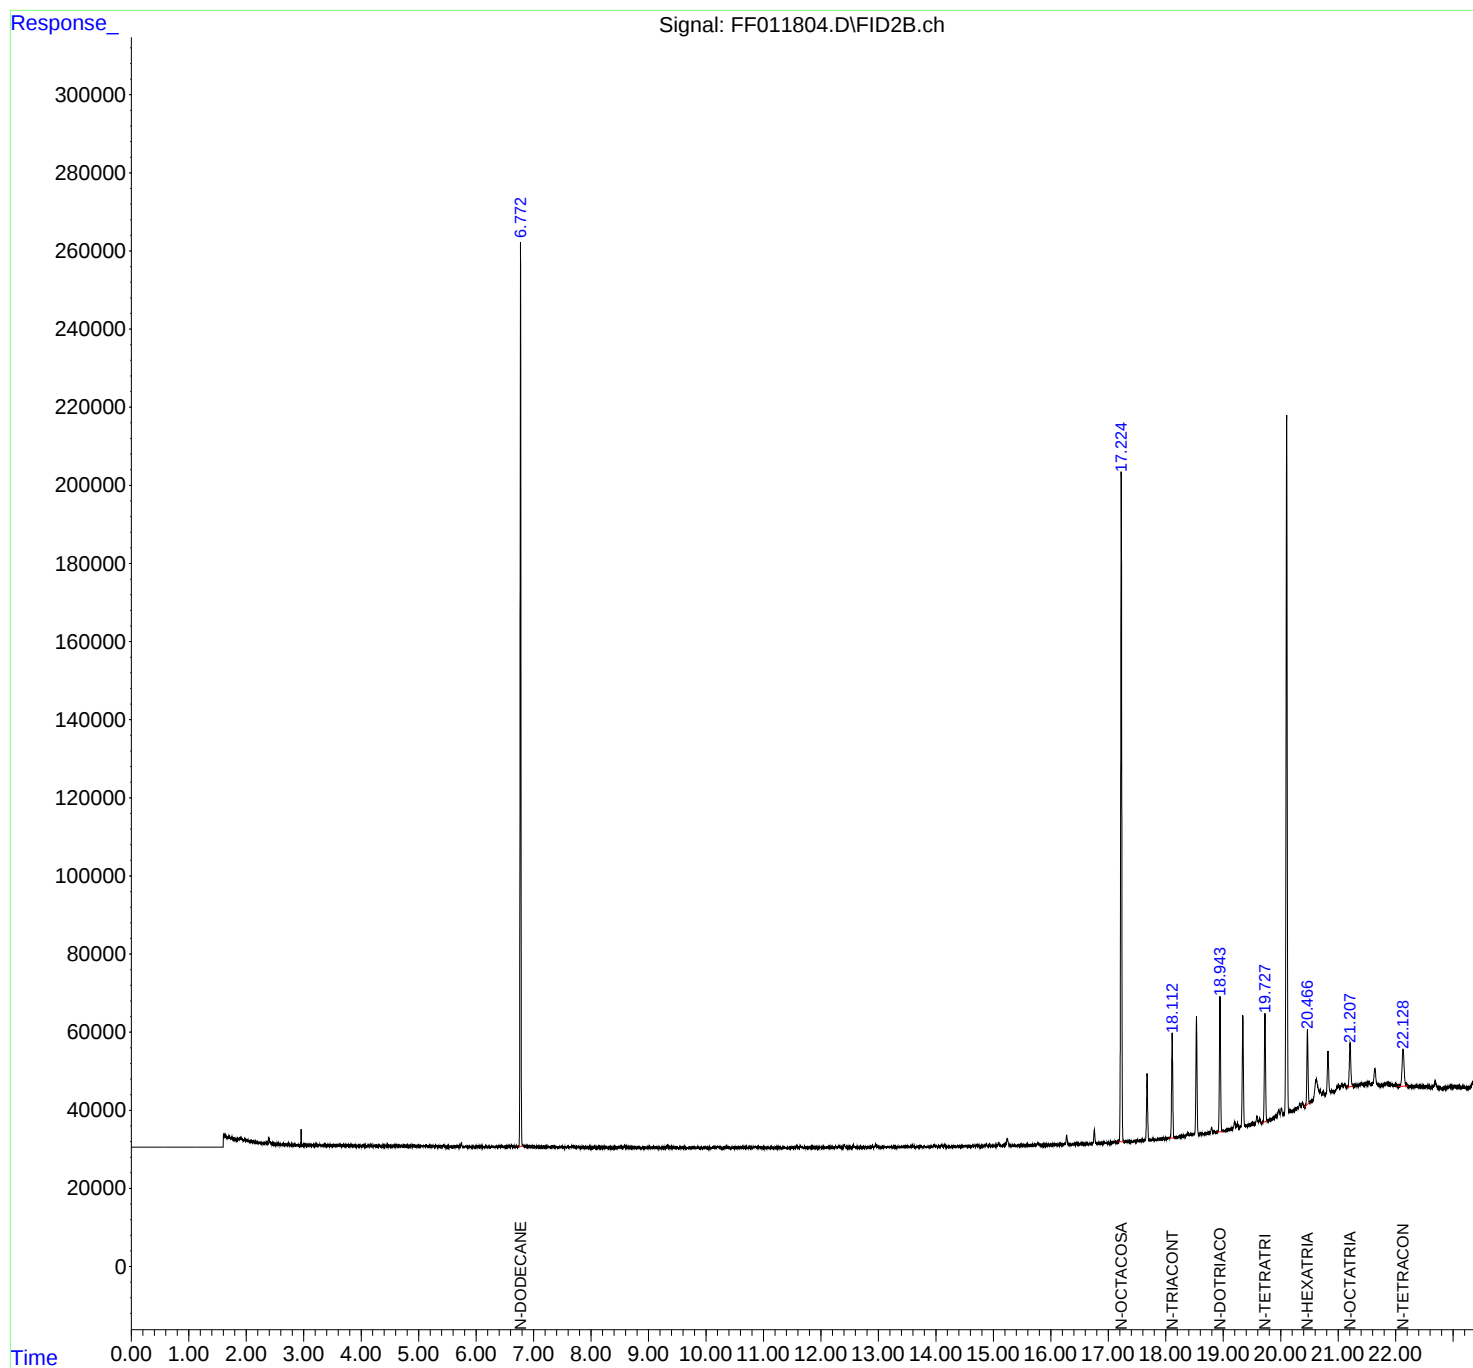


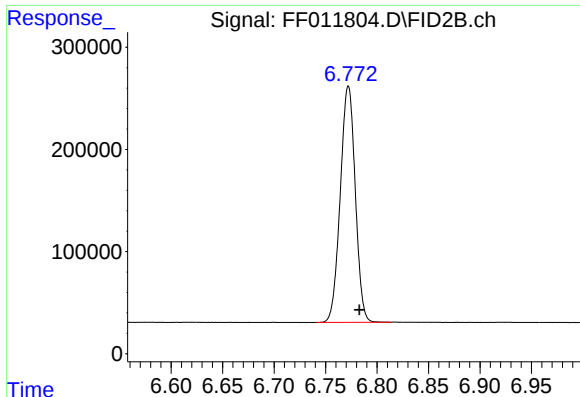

#3 N-DODECANE


R.T.: 6.772 min
Delta R.T.: -0.011 min
Response: 2347140
Conc: 17.00 ug/ml

Instrument :
FID_F
ClientSampleId :

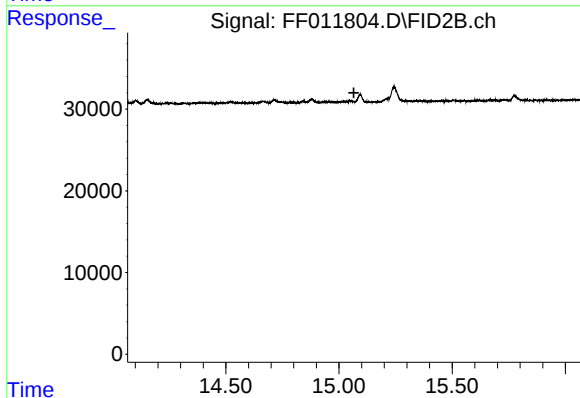


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.066 min
Response: 0
Conc: N.D.

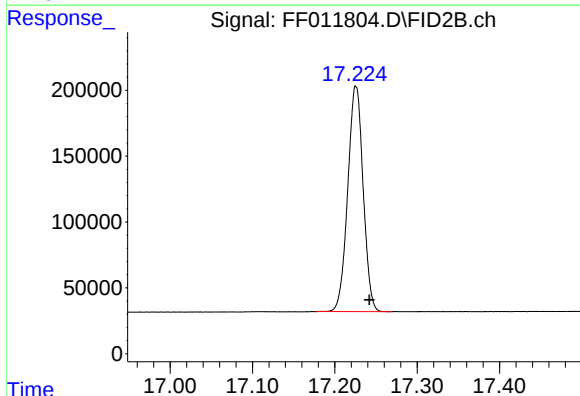


#12 N-OCTACOSANE

R.T.: 17.226 min
Delta R.T.: -0.017 min
Response: 2226481
Conc: 18.06 ug/ml

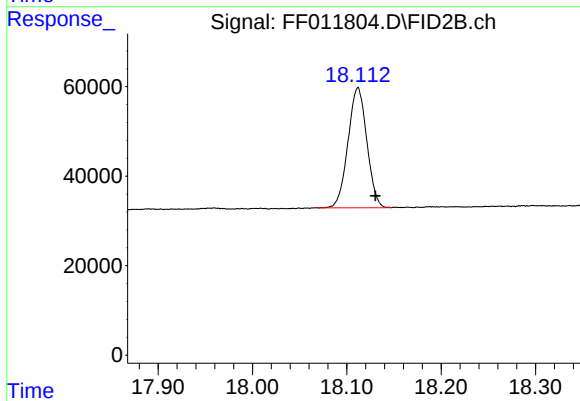

#13 N-TRIACONTANE

R.T.: 18.112 min
Delta R.T.: -0.019 min
Response: 372925
Conc: 3.08 ug/ml

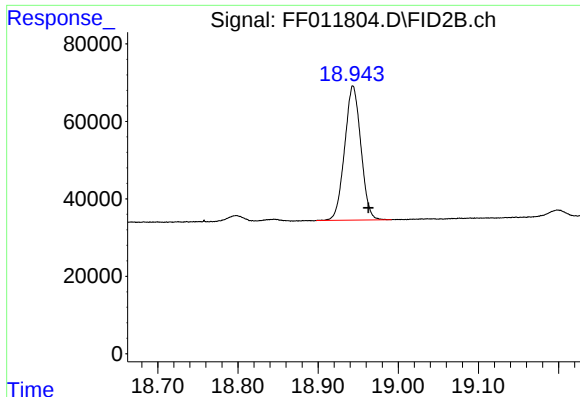


#14 N-DOTRIACONTANE

R.T.: 18.944 min
Delta R.T.: -0.019 min
Response: 487192
Conc: 4.05 ug/ml

Instrument :


FID_F

ClientSampleId :

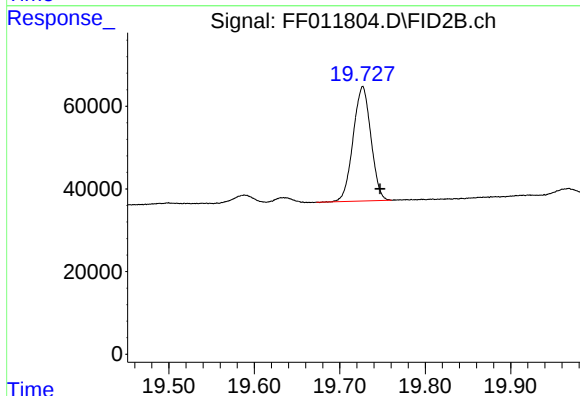


#15 N-TETRATRIACONTANE

R.T.: 19.727 min
Delta R.T.: -0.020 min
Response: 400345
Conc: 3.38 ug/ml

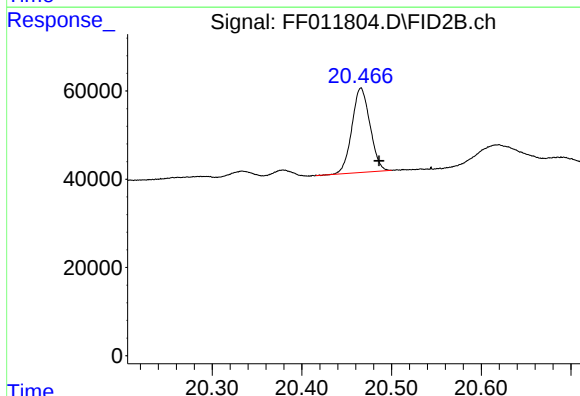


#16 N-HEXATRIACONTANE

R.T.: 20.466 min
Delta R.T.: -0.020 min
Response: 266984
Conc: 2.30 ug/ml

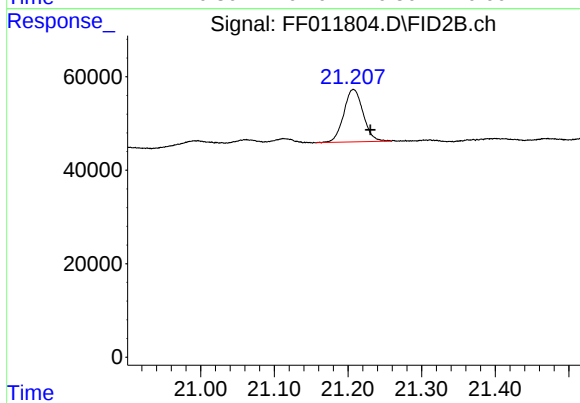

#17 N-OCTATRIACONTANE

R.T.: 21.207 min
Delta R.T.: -0.023 min
Response: 205427
Conc: 1.70 ug/ml

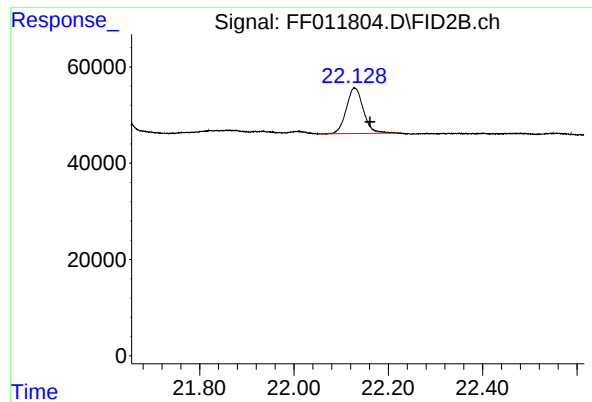

#18 N-TETRACONTANE

R.T.: 22.128 min
Delta R.T.: -0.033 min
Response: 236244
Conc: 1.81 ug/ml

Instrument :

FID_F

ClientSampleId :