

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF121322\  
 Data File : FF011805.D  
 Signal(s) : FID2B.ch  
 Acq On : 13 Dec 2022 16:40  
 Operator : YP\AJ  
 Sample : PB149571BL  
 Misc :  
 ALS Vial : 63 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Dec 14 03:05:16 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF120522.M  
 Quant Title :  
 QLast Update : Tue Dec 06 04:24:35 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.051	1858695	16.278 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.112	92458	0.763 ug/ml
14) N-DOTRIACONTANE	18.944	126041	1.047 ug/ml
15) N-TETRATRIACONTANE	19.727	101819	0.859 ug/ml
16) N-HEXATRIACONTANE	20.467	62065	0.534 ug/ml
-----			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF121322\  
 Data File : FF011805.D  
 Signal(s) : FID2B.ch  
 Acq On : 13 Dec 2022 16:40  
 Operator : YP\AJ  
 Sample : PB149571BL  
 Misc :  
 ALS Vial : 63 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Dec 14 03:05:16 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF120522.M  
 Quant Title :  
 QLast Update : Tue Dec 06 04:24:35 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

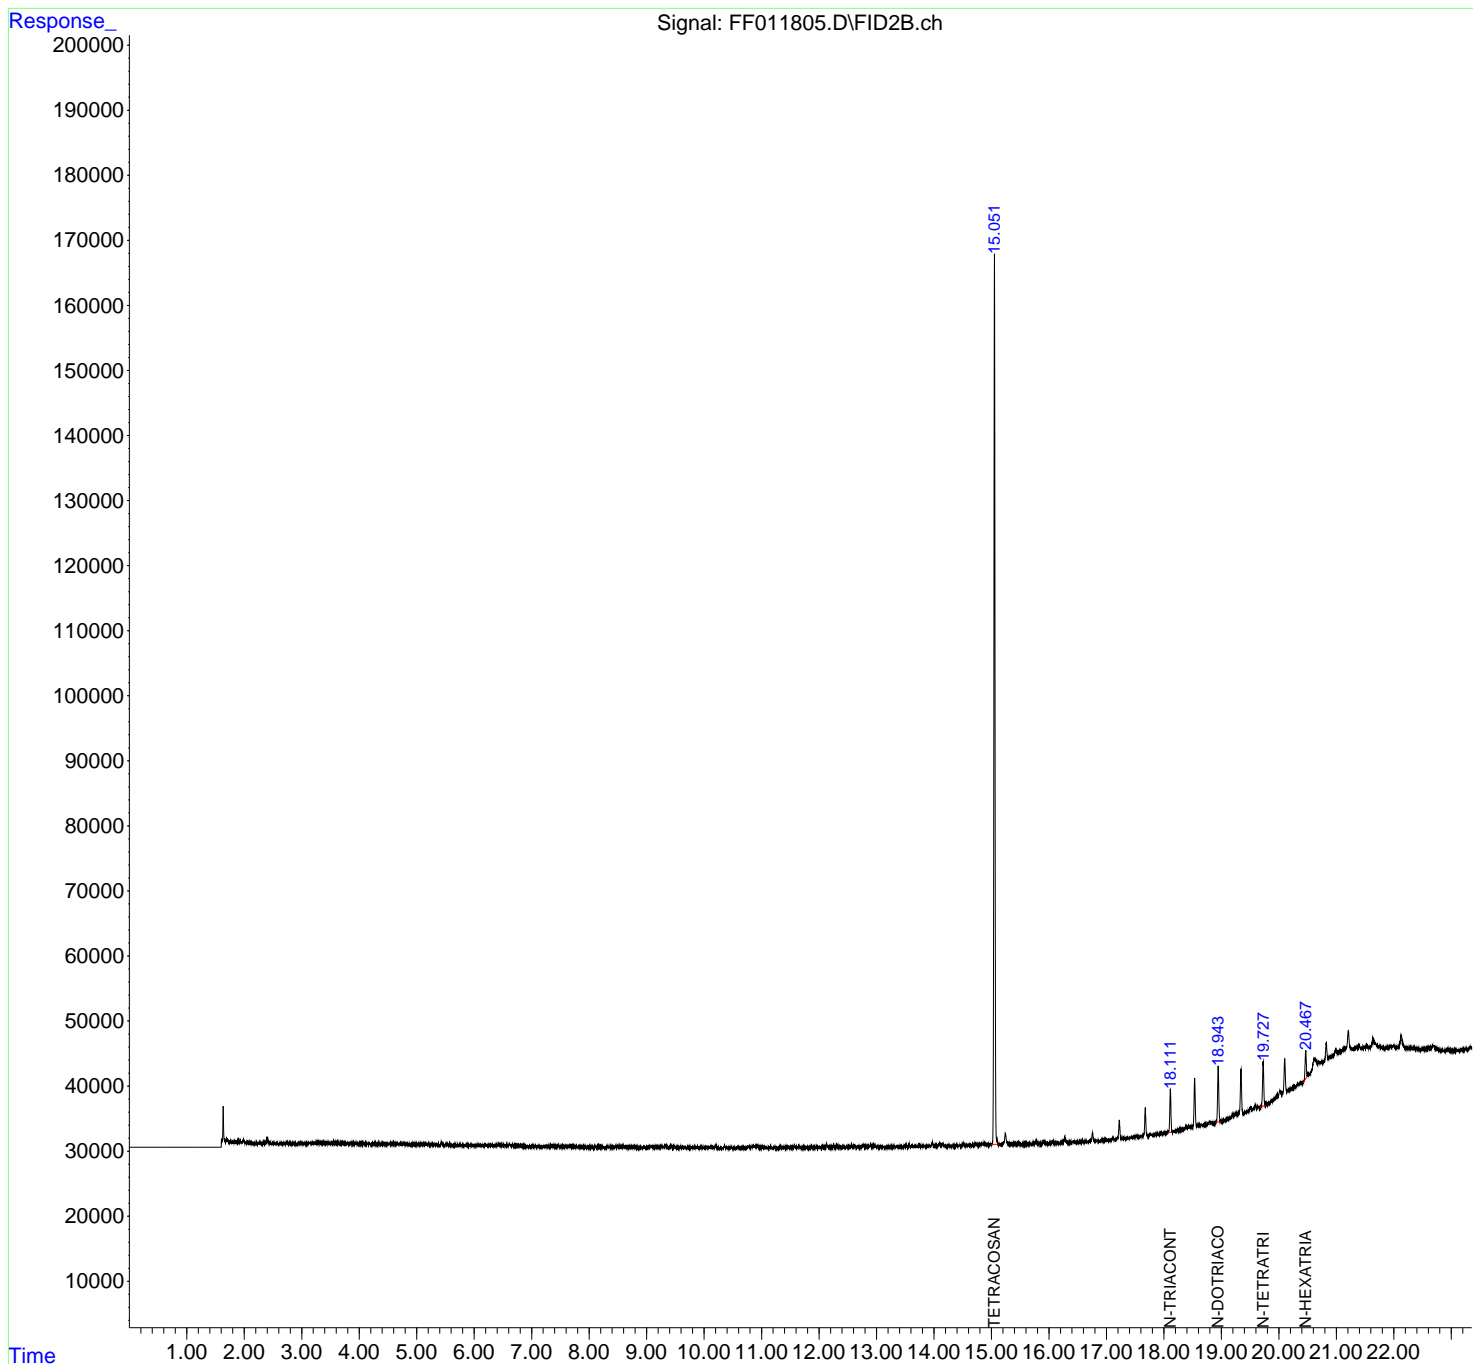


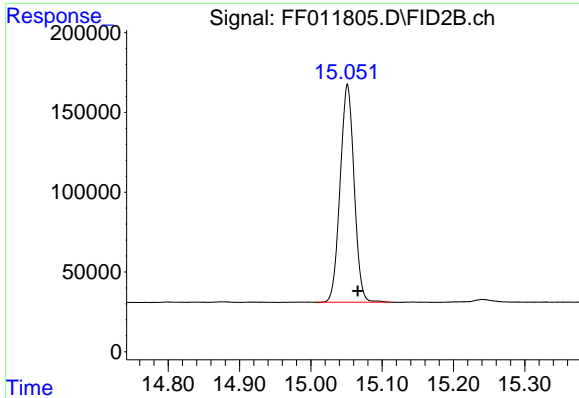

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.051 min  
 Delta R.T.: -0.015 min  
 Response: 1858695  
 Conc: 16.28 ug/ml

Instrument :  
 FID\_F  
 ClientSampleId :

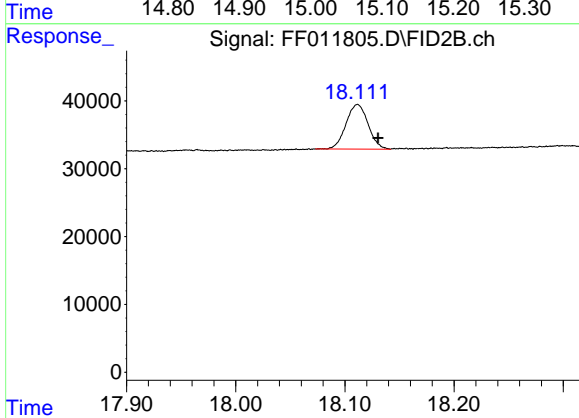


#13 N-TRIACONTANE

R.T.: 18.112 min  
 Delta R.T.: -0.019 min  
 Response: 92458  
 Conc: 0.76 ug/ml

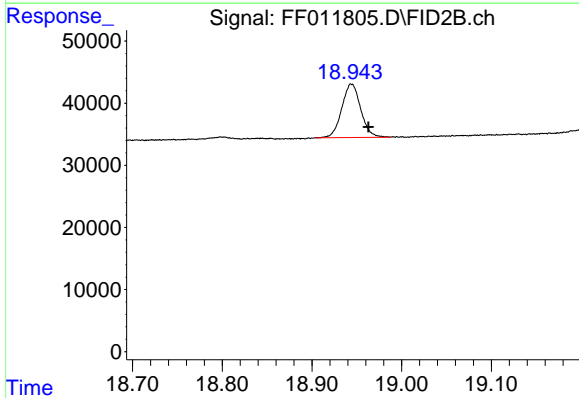


#14 N-DOTRIACONTANE

R.T.: 18.944 min  
 Delta R.T.: -0.019 min  
 Response: 126041  
 Conc: 1.05 ug/ml

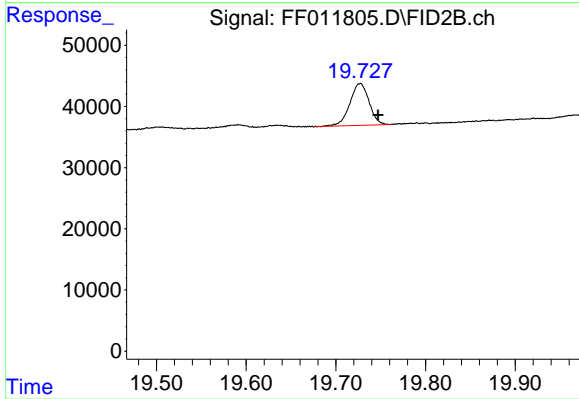

#15 N-TETRATRIACONTANE

R.T.: 19.727 min  
 Delta R.T.: -0.020 min  
 Response: 101819  
 Conc: 0.86 ug/ml

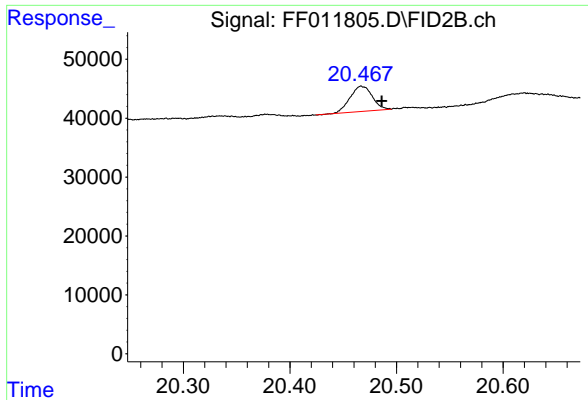

#16 N-HEXATRIACONTANE

R.T.: 20.467 min  
Delta R.T.: -0.019 min  
Response: 62065  
Conc: 0.53 ug/ml

Instrument :  
FID\_F  
ClientSampleId :