

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF121322\  
Data File : FF011791.D  
Signal(s) : FID2B.ch  
Acq On : 13 Dec 2022 09:38  
Operator : YP\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
RT MARKER

Integration File: autoint1.e  
Quant Time: Dec 14 03:02:55 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF120522.M  
Quant Title :  
QLast Update : Tue Dec 06 04:24:35 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |              | R.T.   | Response | Conc Units   |
|-----------------------------|--------------|--------|----------|--------------|
| -----                       |              |        |          |              |
| System Monitoring Compounds |              |        |          |              |
| Target Compounds            |              |        |          |              |
| 3)                          | N-DODECANE   | 6.773  | 2535499  | 18.360 ug/ml |
| 12)                         | N-OCTACOSANE | 17.227 | 2348308  | 19.051 ug/ml |
| -----                       |              |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF121322\  
Data File : FF011791.D  
Signal(s) : FID2B.ch  
Acq On : 13 Dec 2022 09:38  
Operator : YP\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
RT MARKER

Integration File: autoint1.e  
Quant Time: Dec 14 03:02:55 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF120522.M  
Quant Title :  
QLast Update : Tue Dec 06 04:24:35 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

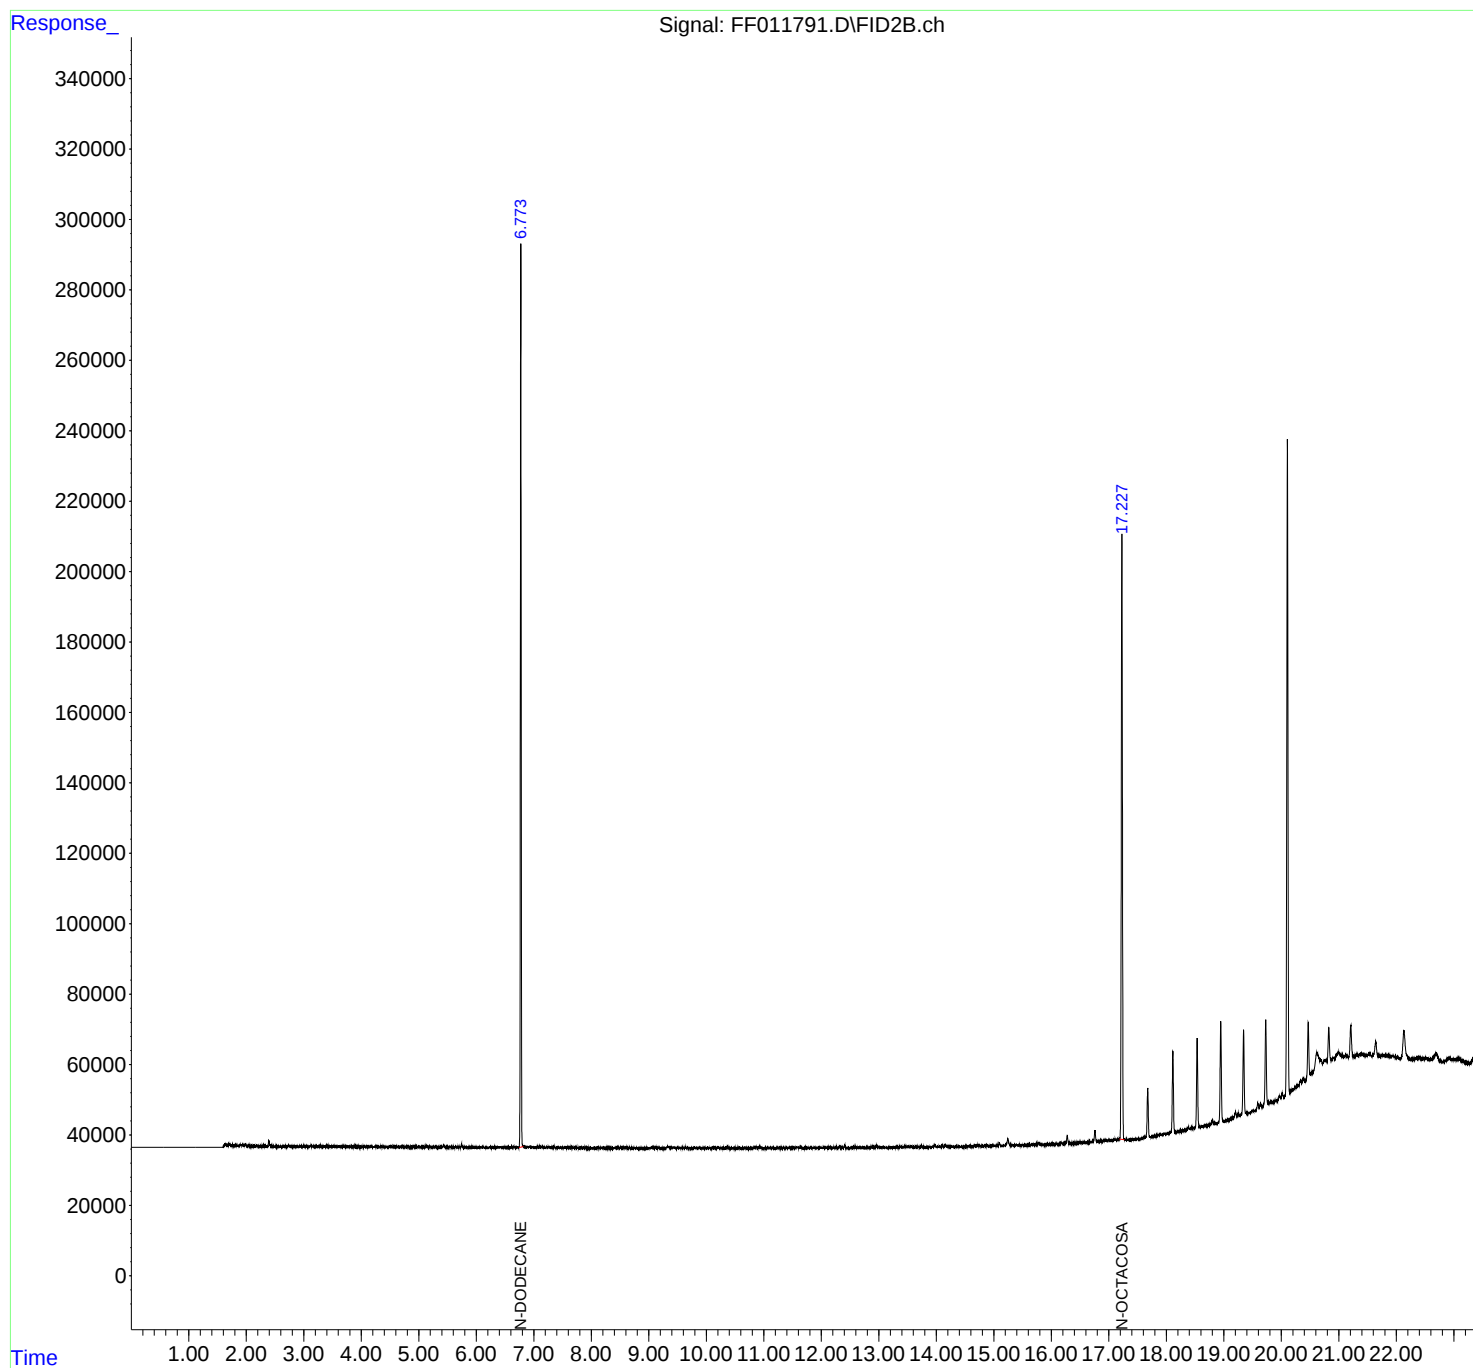


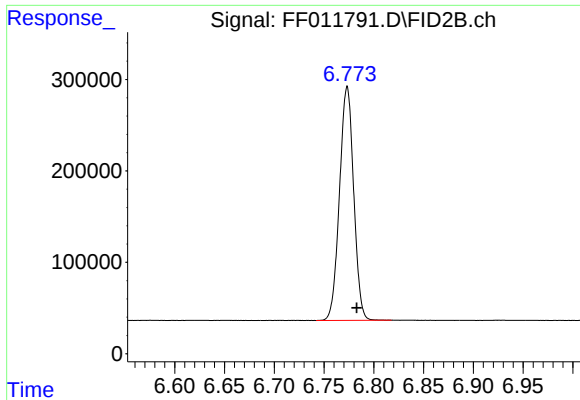

#3 N-DODECANE


R.T.: 6.773 min  
Delta R.T.: -0.010 min  
Response: 2535499  
Conc: 18.36 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
RT MARKER

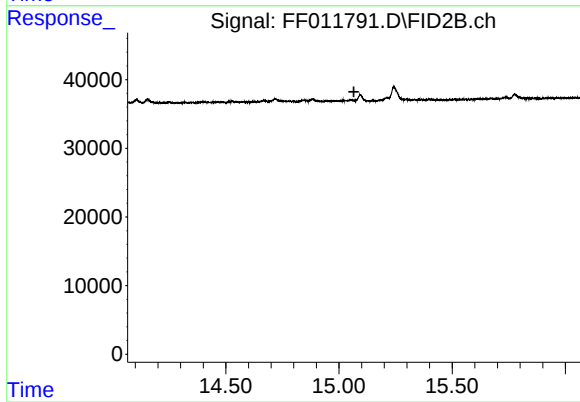

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 15.066 min  
Response: 0  
Conc: N.D.

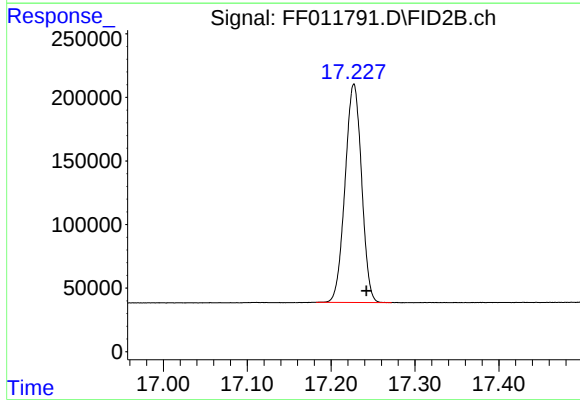

#12 N-OCTACOSANE

R.T.: 17.227 min  
Delta R.T.: -0.015 min  
Response: 2348308  
Conc: 19.05 ug/ml