

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121420\
 Data File : FF007996.D
 Signal(s) : FID2B.ch
 Acq On : 15 Dec 2020 00:19
 Operator : DD\AJ
 Sample : L5038-01
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 15 01:56:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120220.M
 Quant Title :
 QLast Update : Thu Dec 03 09:08:10 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.703	3018391	23.875 ug/ml
Target Compounds			
3) N-DODECANE	6.467	284878	1.978 ug/ml
4) N-TETRADECANE	8.216	2782930	18.959 ug/ml
12) N-OCTACOSANE	16.909	371420	2.744 ug/ml
18) N-TETRACONTANE	21.768f	1873513	33.403 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121420\
Data File : FF007996.D
Signal(s) : FID2B.ch
Acq On : 15 Dec 2020 00:19
Operator : DD\AJ
Sample : L5038-01
Misc :
ALS Vial : 78 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 15 01:56:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120220.M
Quant Title :
QLast Update : Thu Dec 03 09:08:10 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

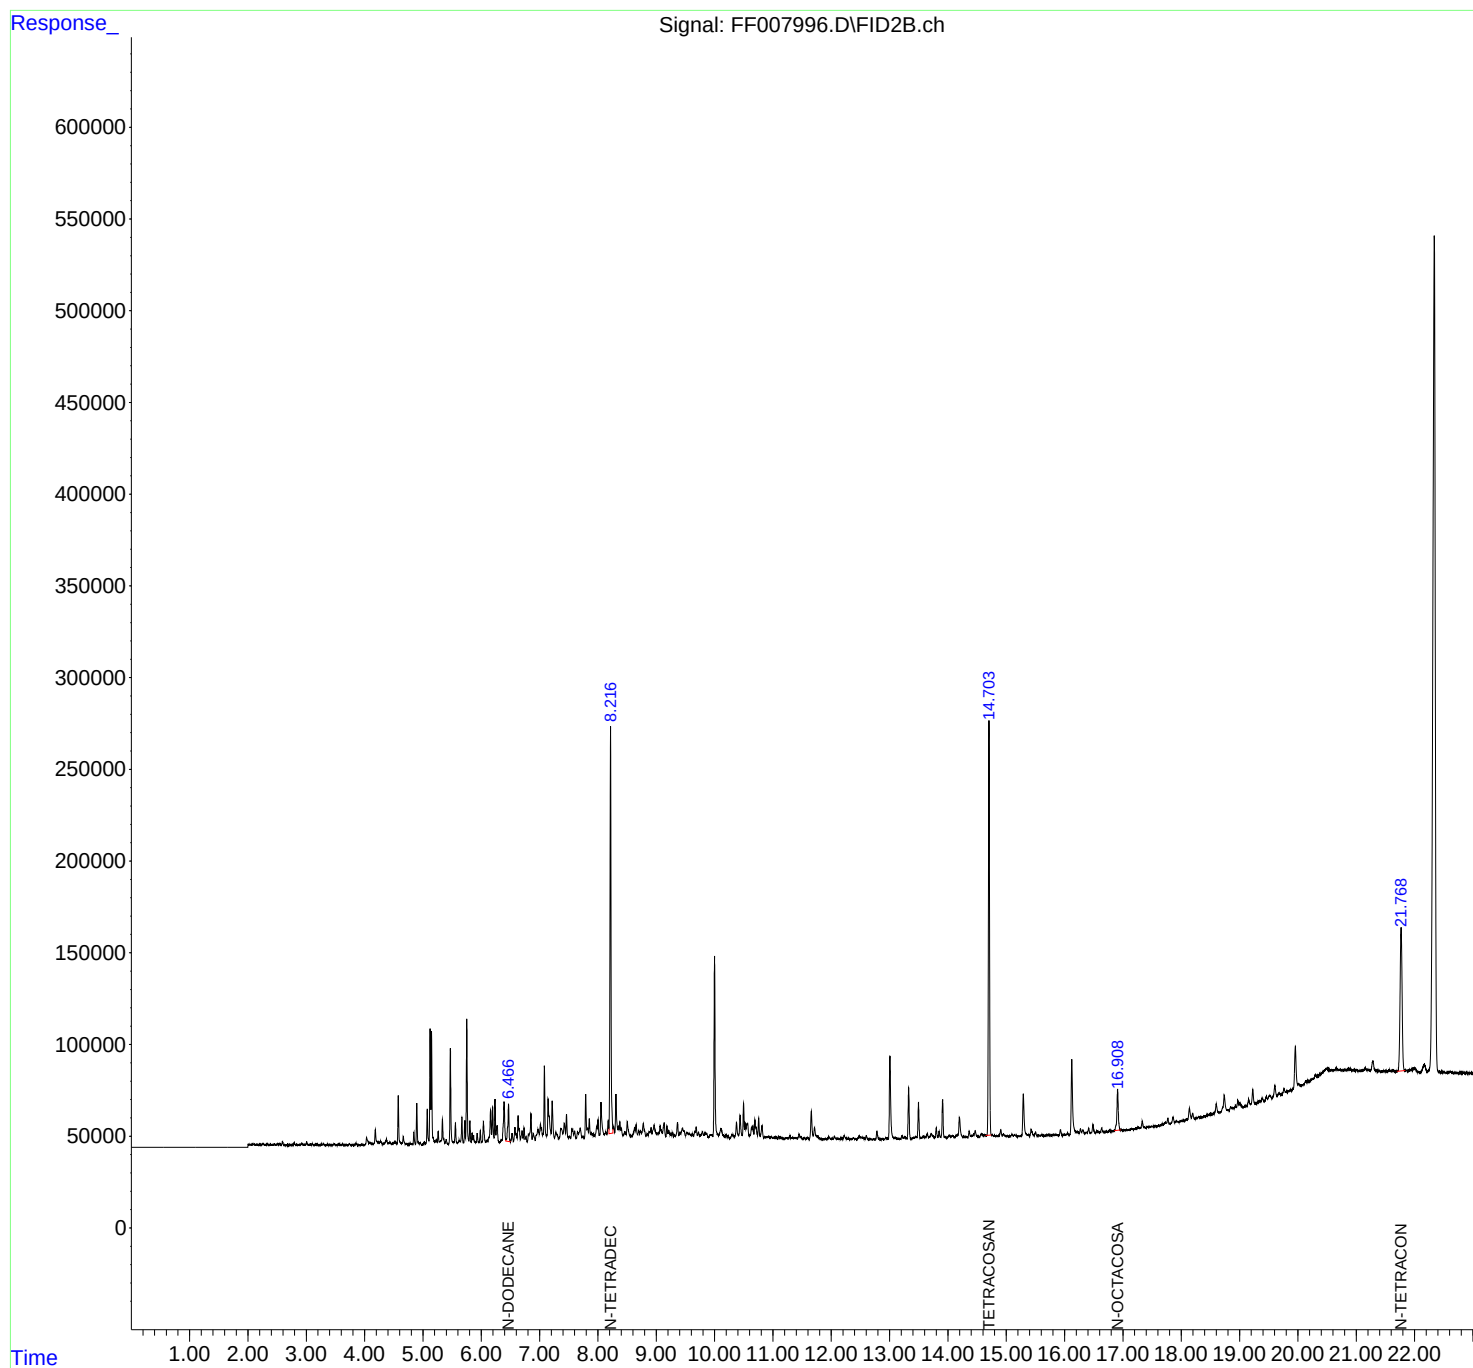

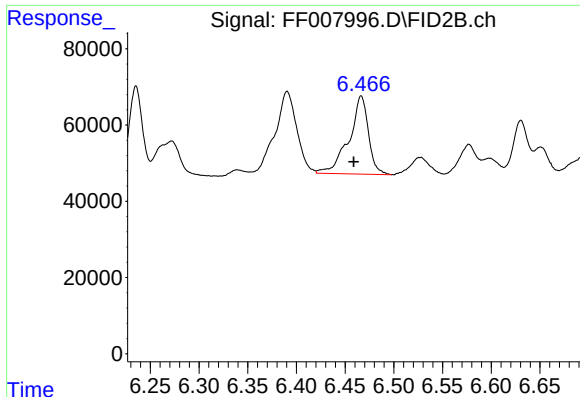


#3 N-DODECANE

R.T.: 6.467 min
Delta R.T.: 0.007 min
Response: 284878
Conc: 1.98 ug/ml

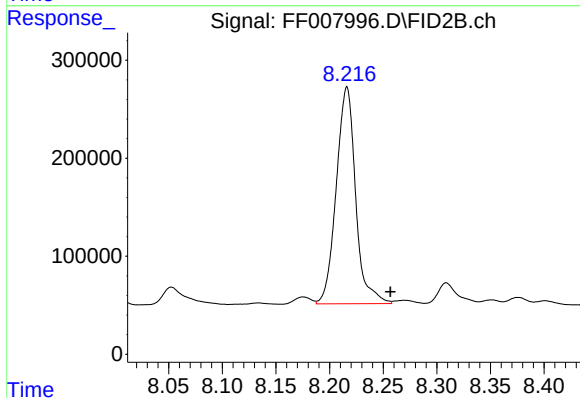


#4 N-TETRADECANE

R.T.: 8.216 min
Delta R.T.: -0.040 min
Response: 2782930
Conc: 18.96 ug/ml

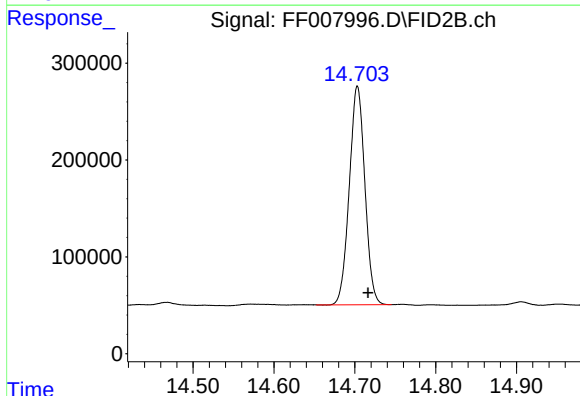


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.703 min
Delta R.T.: -0.013 min
Response: 3018391
Conc: 23.87 ug/ml

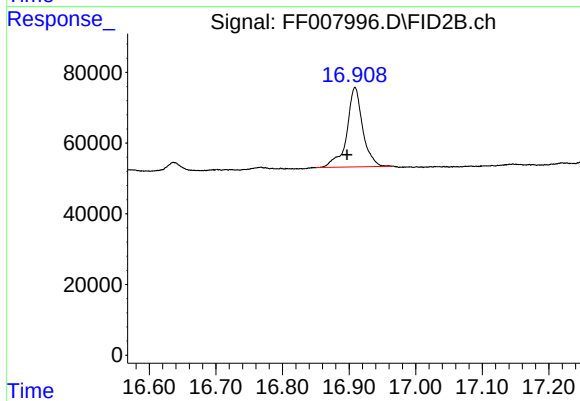

#12 N-OCTACOSANE

R.T.: 16.909 min
Delta R.T.: 0.012 min
Response: 371420
Conc: 2.74 ug/ml

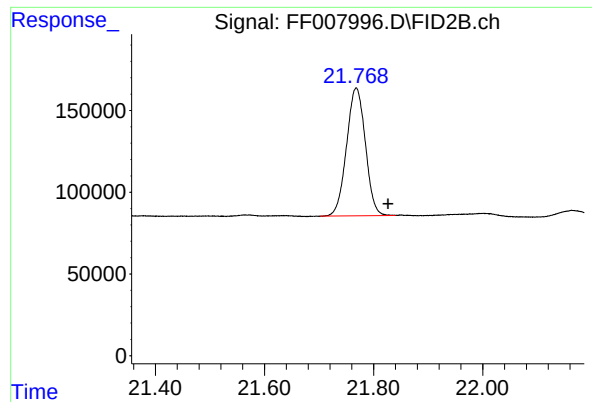

#18 N-TETRACONTANE

R.T.: 21.768 min
Delta R.T.: -0.058 min
Response: 1873513
Conc: 33.40 ug/ml