

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121422\
Data File : FF011818.D
Signal(s) : FID2B.ch
Acq On : 14 Dec 2022 09:42
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 14 14:58:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.767	2015441	14.594 ug/ml
12)	N-OCTACOSANE	17.223	1920026	15.577 ug/ml
13)	N-TRIACONTANE	18.110	392510	3.240 ug/ml
14)	N-DOTRIACONTANE	18.942	518100	4.305 ug/ml
15)	N-TETRATRIACONTANE	19.726	427490	3.607 ug/ml
16)	N-HEXATRIACONTANE	20.465	277644	2.387 ug/ml
17)	N-OCTATRIACONTANE	21.207	227357	1.881 ug/ml
18)	N-TETRACONTANE	22.126	275066	2.109 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121422\
Data File : FF011818.D
Signal(s) : FID2B.ch
Acq On : 14 Dec 2022 09:42
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 14 14:58:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

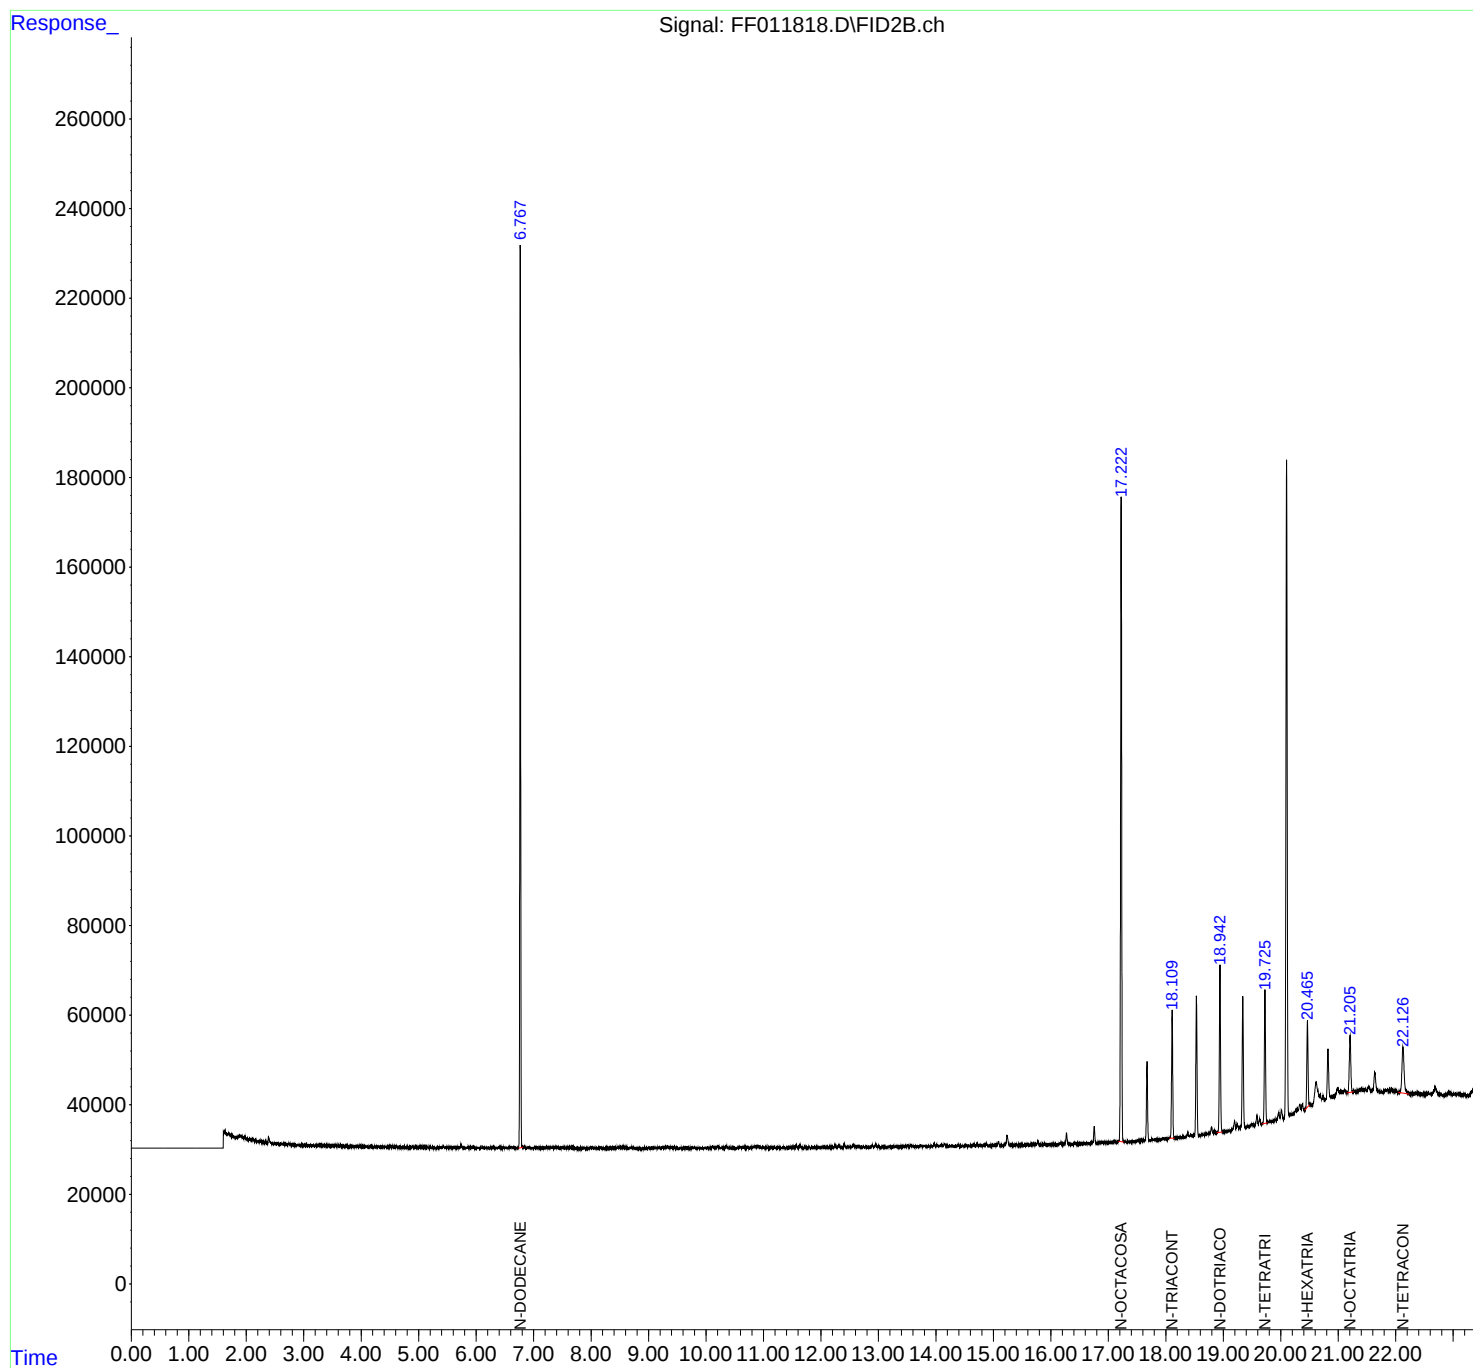


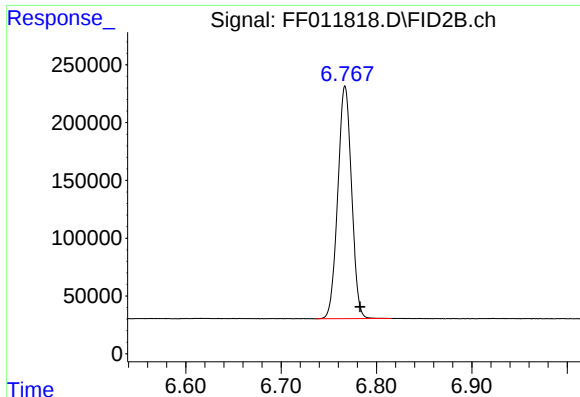

#3 N-DODECANE


R.T.: 6.767 min
Delta R.T.: -0.016 min
Response: 2015441
Conc: 14.59 ug/ml

Instrument :
FID_F
ClientSampleId :

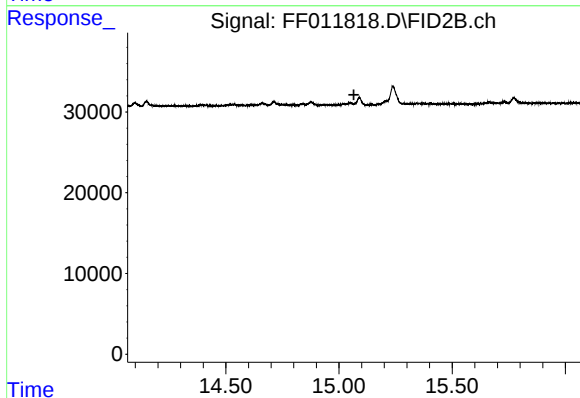


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.066 min
Response: 0
Conc: N.D.

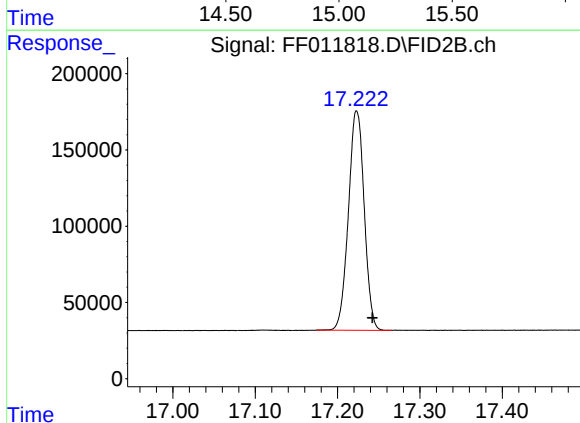


#12 N-OCTACOSANE

R.T.: 17.223 min
Delta R.T.: -0.019 min
Response: 1920026
Conc: 15.58 ug/ml

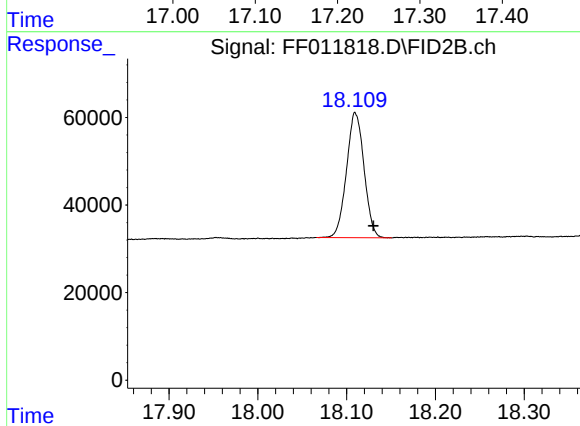

#13 N-TRIACONTANE


R.T.: 18.110 min
Delta R.T.: -0.021 min
Response: 392510
Conc: 3.24 ug/ml

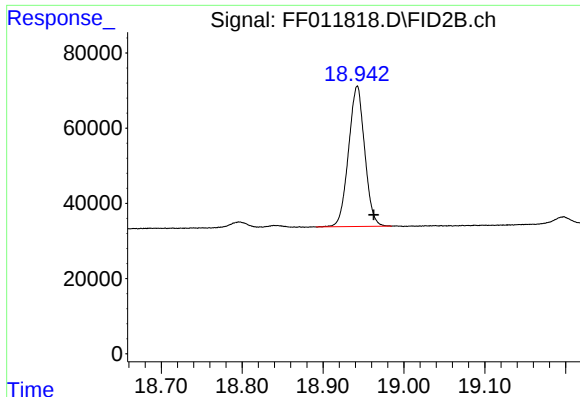

#14 N-DOTRIACONTANE


R.T.: 18.942 min
Delta R.T.: -0.020 min
Response: 518100
Conc: 4.31 ug/ml

Instrument :
FID_F
ClientSampleId :

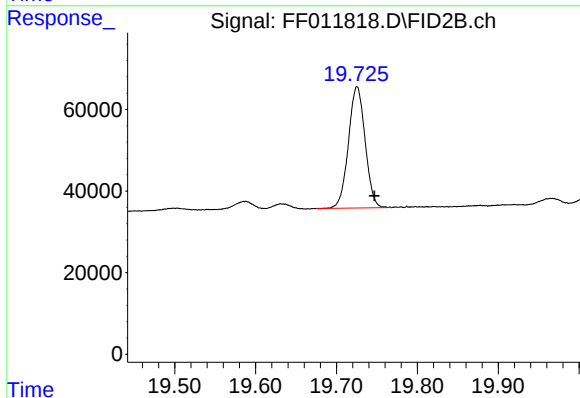


#15 N-TETRATRIACONTANE

R.T.: 19.726 min
Delta R.T.: -0.022 min
Response: 427490
Conc: 3.61 ug/ml

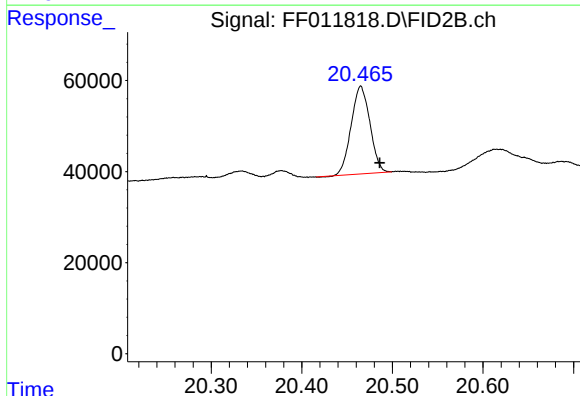


#16 N-HEXATRIACONTANE

R.T.: 20.465 min
Delta R.T.: -0.021 min
Response: 277644
Conc: 2.39 ug/ml

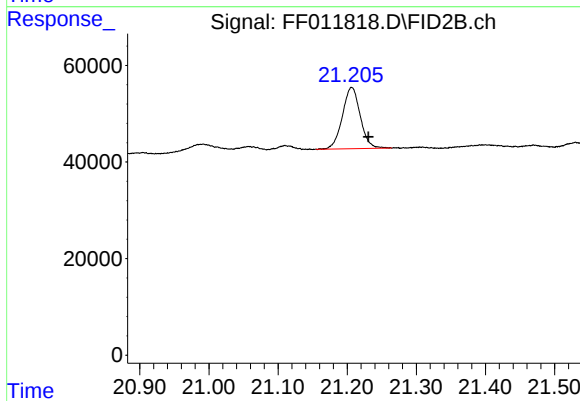

#17 N-OCTATRIACONTANE

R.T.: 21.207 min
Delta R.T.: -0.024 min
Response: 227357
Conc: 1.88 ug/ml

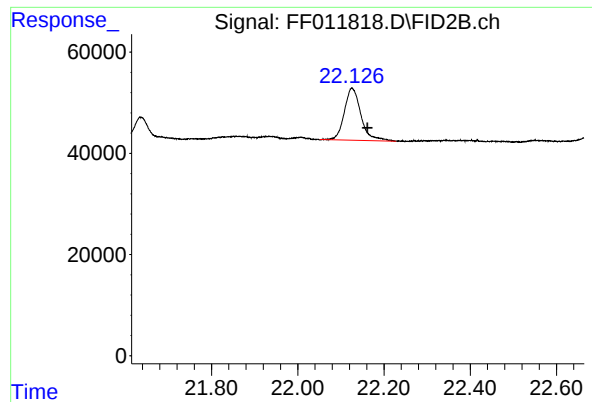

#18 N-TETRACONTANE

R.T.: 22.126 min
Delta R.T.: -0.036 min
Response: 275066
Conc: 2.11 ug/ml

Instrument :

FID_F

ClientSampleId :