

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121422\
Data File : FF011820.D
Signal(s) : FID2B.ch
Acq On : 14 Dec 2022 10:40
Operator : YP\AJ
Sample : PB149625BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 14 14:58:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.050	2278725	19.956 ug/ml
Target Compounds			
12) N-OCTACOSANE	17.223	57601	0.467 ug/ml
13) N-TRIACONTANE	18.110	91287	0.753 ug/ml
14) N-DOTRIACONTANE	18.941	105598	0.877 ug/ml
15) N-TETRATRIACONTANE	19.726	80500	0.679 ug/ml
16) N-HEXATRIACONTANE	20.467	47232	0.406 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121422\
Data File : FF011820.D
Signal(s) : FID2B.ch
Acq On : 14 Dec 2022 10:40
Operator : YP\AJ
Sample : PB149625BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 14 14:58:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

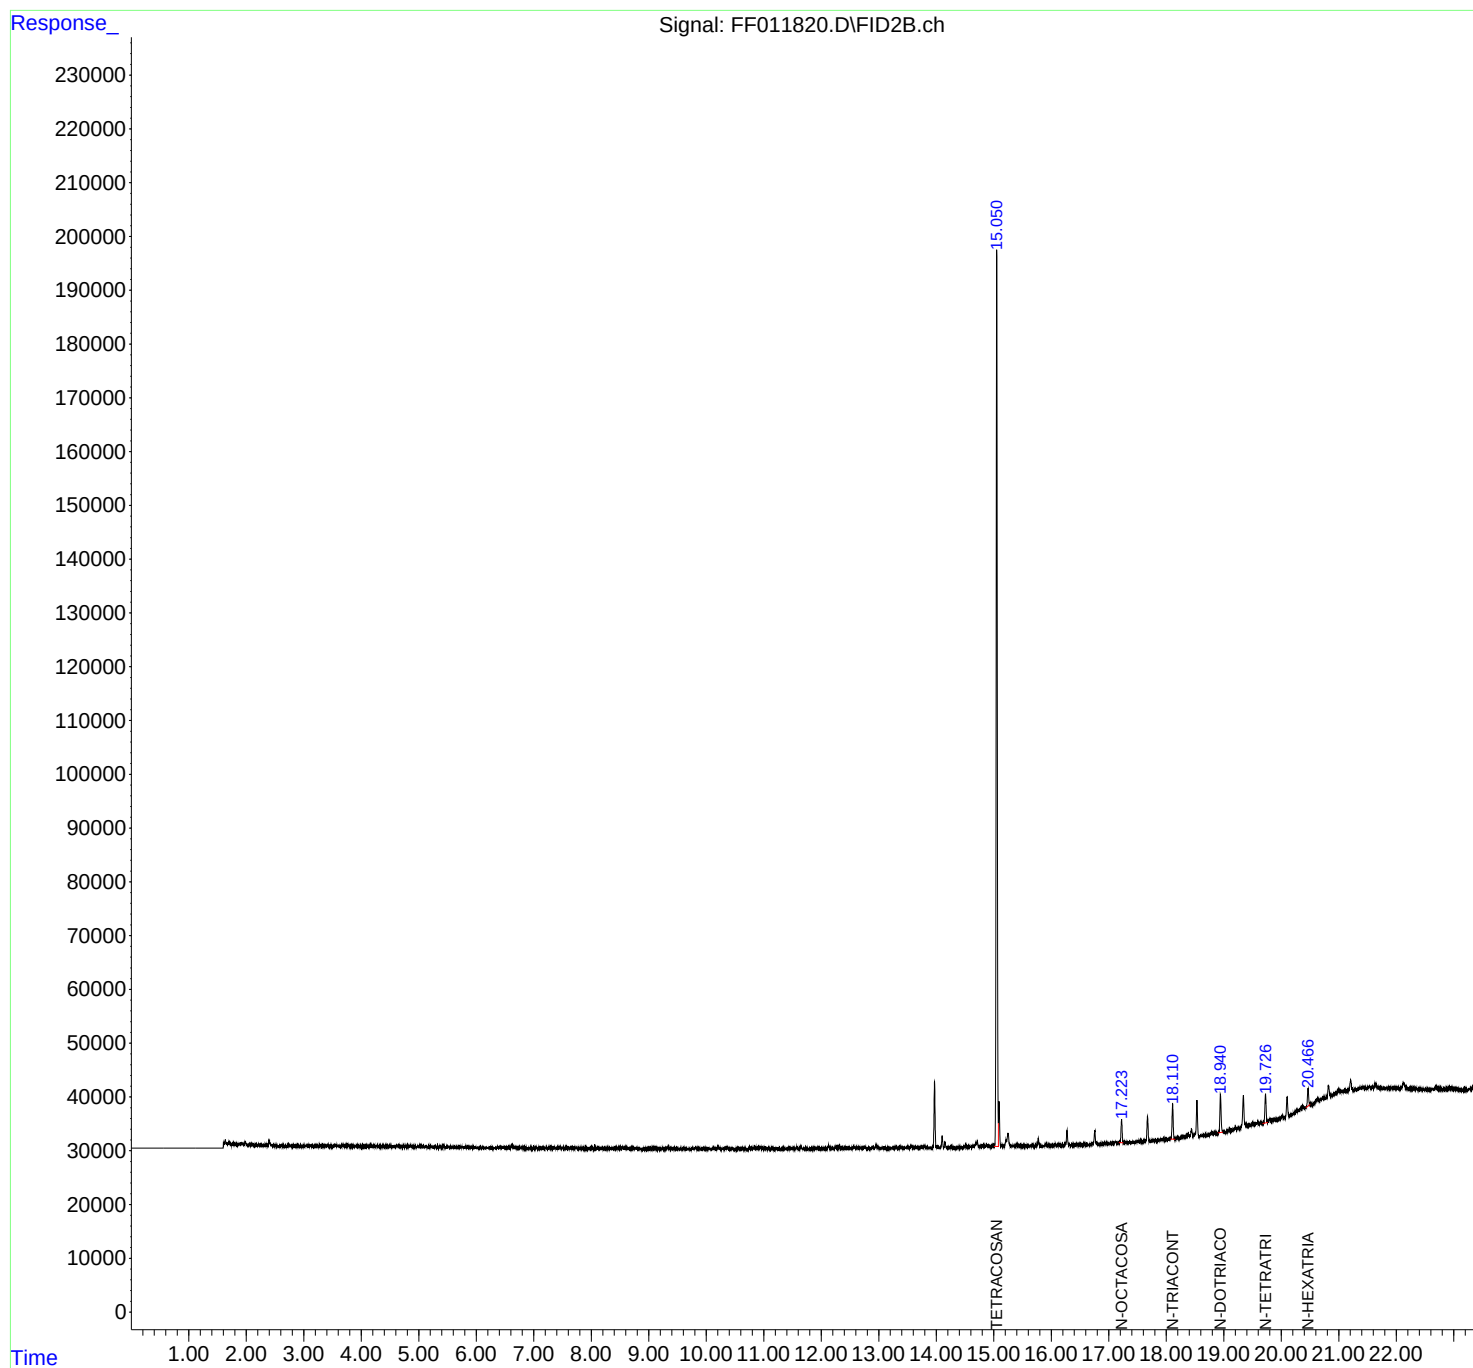


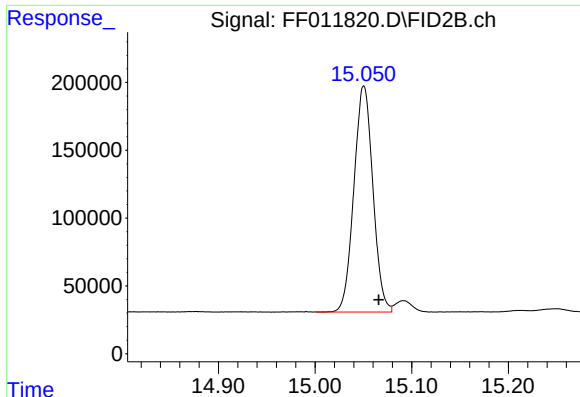

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.050 min
Delta R.T.: -0.016 min
Response: 2278725
Conc: 19.96 ug/ml

Instrument :
FID_F
ClientSampleId :

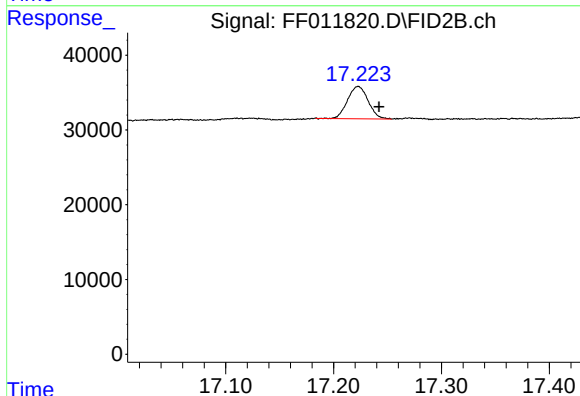


#12 N-OCTACOSANE

R.T.: 17.223 min
Delta R.T.: -0.019 min
Response: 57601
Conc: 0.47 ug/ml

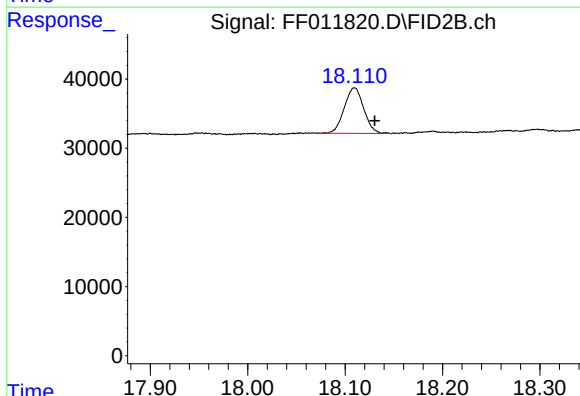


#13 N-TRIACONTANE

R.T.: 18.110 min
Delta R.T.: -0.021 min
Response: 91287
Conc: 0.75 ug/ml

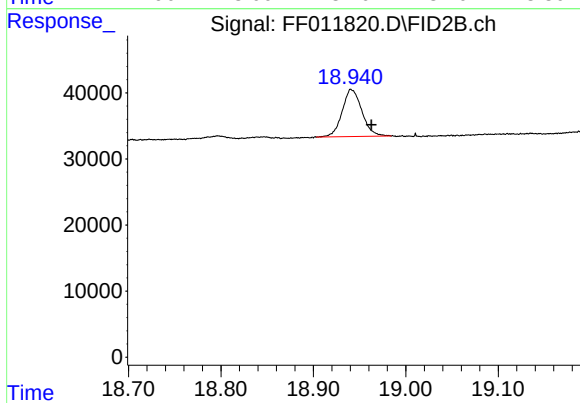

#14 N-DOTRIACONTANE


R.T.: 18.941 min
Delta R.T.: -0.022 min
Response: 105598
Conc: 0.88 ug/ml

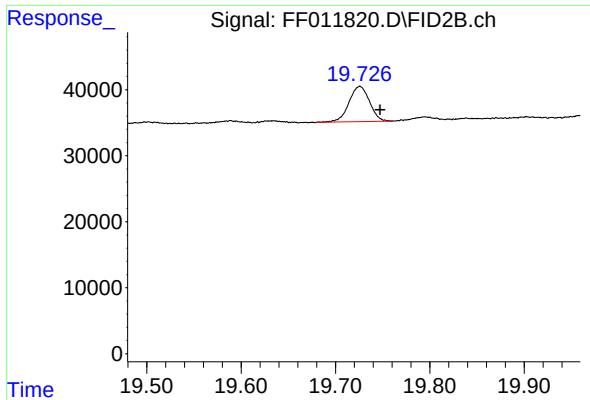

#15 N-TETRATRIACONTANE

R.T.: 19.726 min
Delta R.T.: -0.021 min
Response: 80500
Conc: 0.68 ug/ml

Instrument :
FID_F
ClientSampleId :

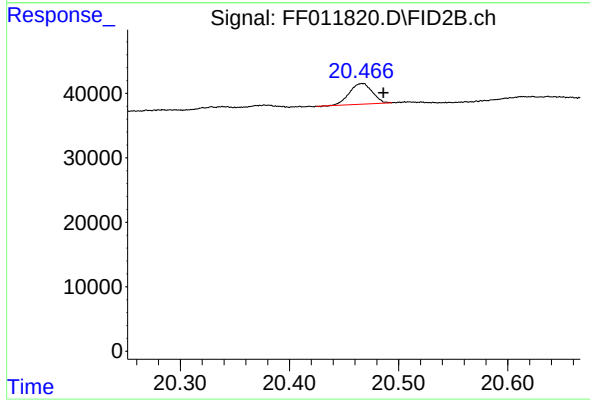

#16 N-HEXATRIACONTANE

R.T.: 20.467 min
Delta R.T.: -0.019 min
Response: 47232
Conc: 0.41 ug/ml