

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121422\
Data File : FF011819.D
Signal(s) : FID2B.ch
Acq On : 14 Dec 2022 10:11
Operator : YP\AJ
Sample : PB149624BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB149624BL

Integration File: autoint1.e
Quant Time: Dec 14 14:58:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.050	1888764	16.541 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121422\
Data File : FF011819.D
Signal(s) : FID2B.ch
Acq On : 14 Dec 2022 10:11
Operator : YP\AJ
Sample : PB149624BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB149624BL

Integration File: autoint1.e
Quant Time: Dec 14 14:58:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

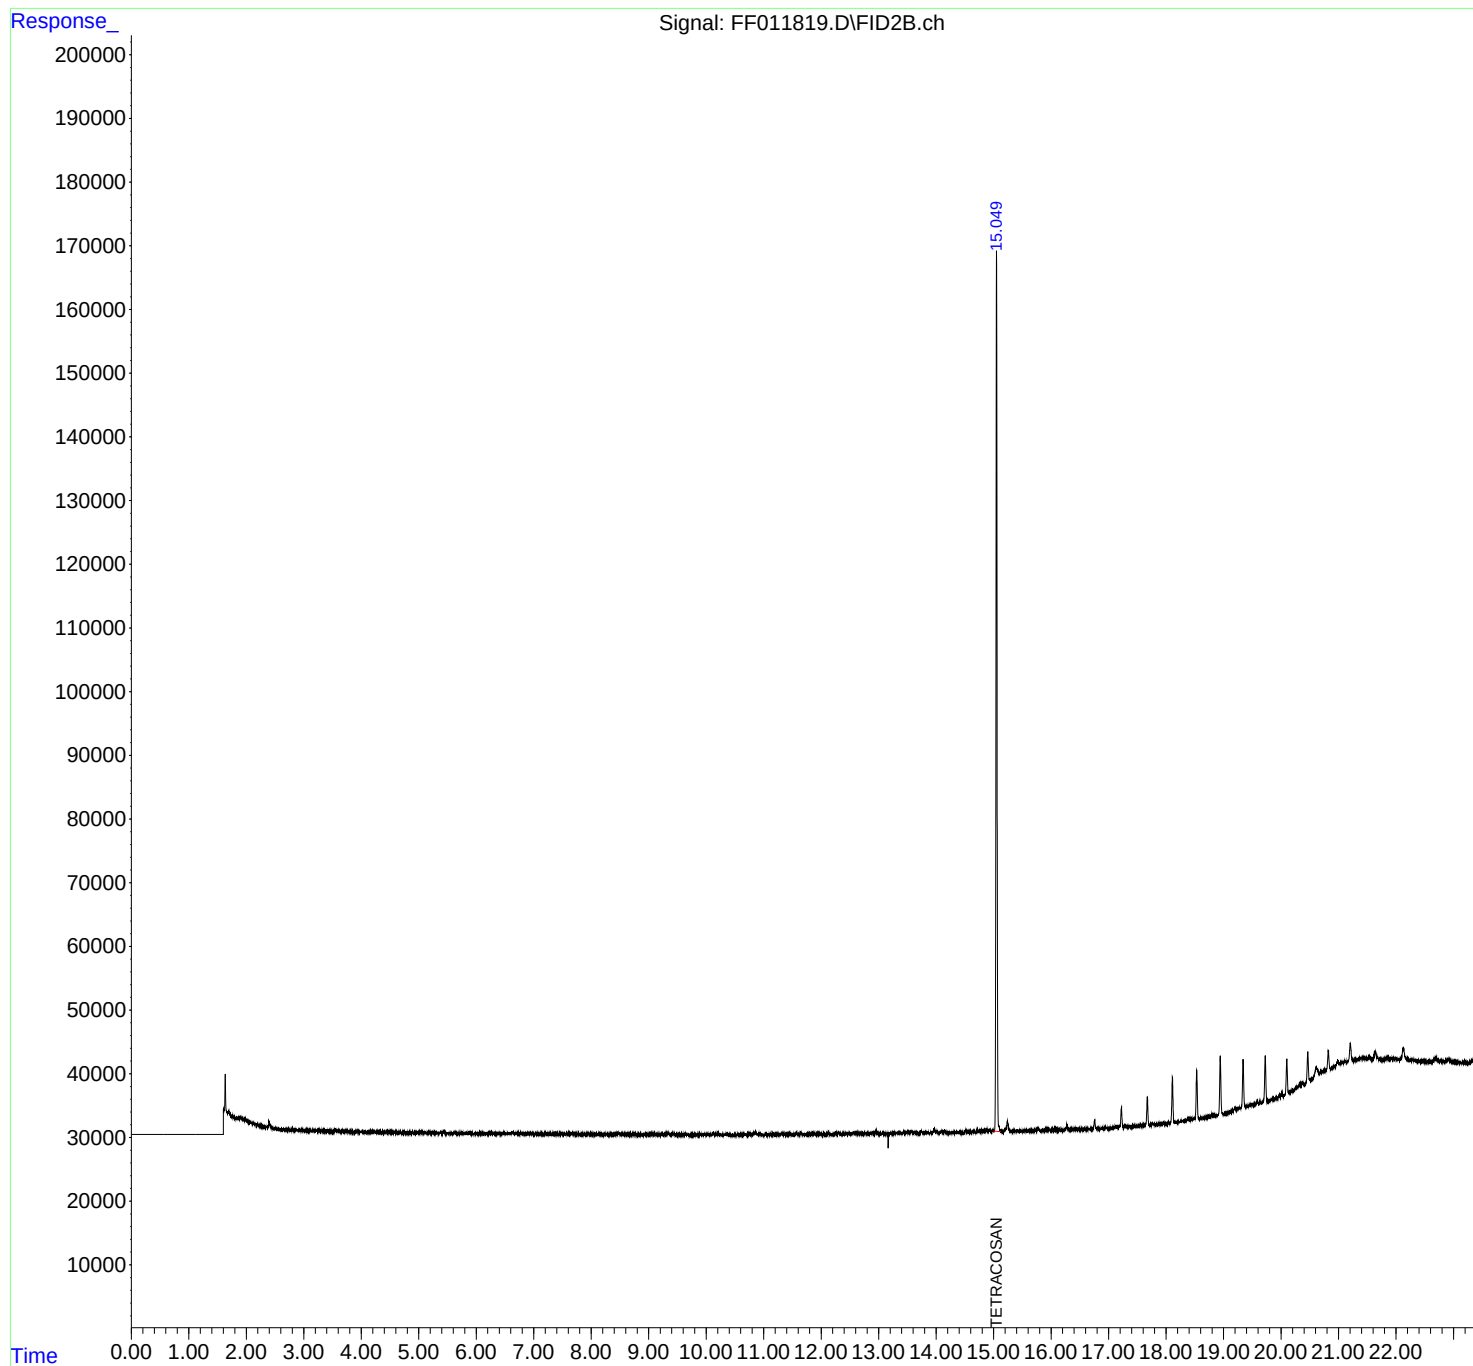

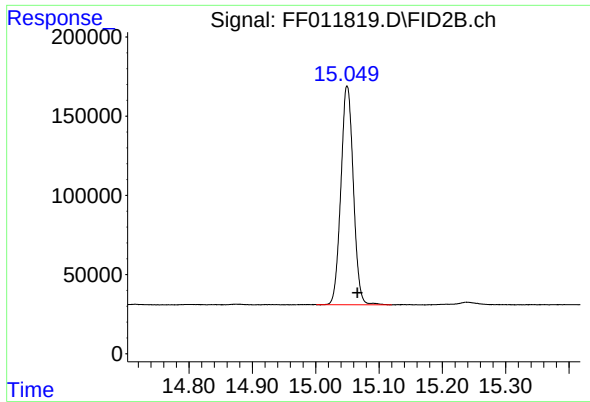

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.050 min
Delta R.T.: -0.016 min
Response: 1888764
Conc: 16.54 ug/ml

Instrument :
FID_F
ClientSampleId :
PB149624BL