

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121423\
Data File : FF013861.D
Signal(s) : FID2B.ch
Acq On : 14 Dec 2023 17:14
Operator : YP\AJ
Sample : PB157775BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 14 23:28:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120523.M
Quant Title :
QLast Update : Tue Dec 05 11:16:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.961	2072354	17.537 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.025	83832	0.714 ug/ml
14) N-DOTRIACONTANE	18.858	104359	0.920 ug/ml
15) N-TETRATRIACONTANE	19.640	75017	0.765 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121423\
Data File : FF013861.D
Signal(s) : FID2B.ch
Acq On : 14 Dec 2023 17:14
Operator : YP\AJ
Sample : PB157775BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 14 23:28:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120523.M
Quant Title :
QLast Update : Tue Dec 05 11:16:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

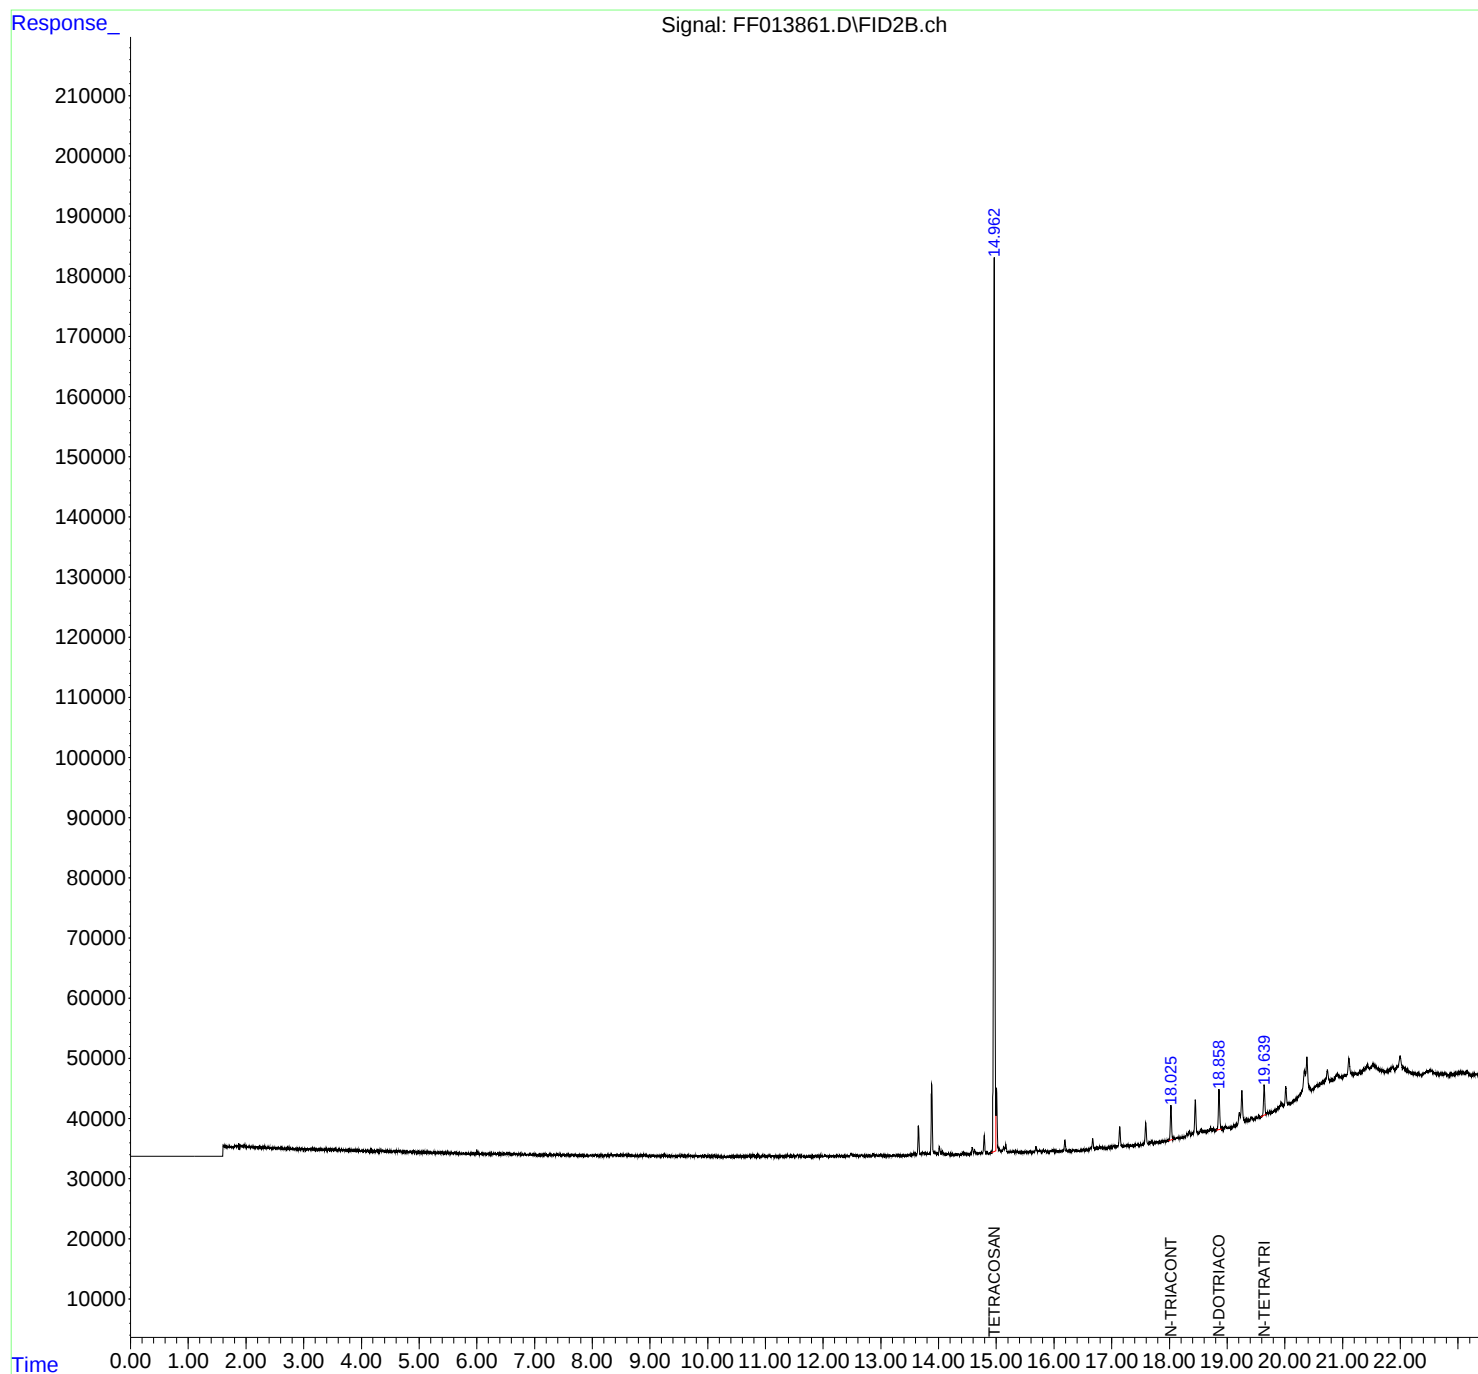


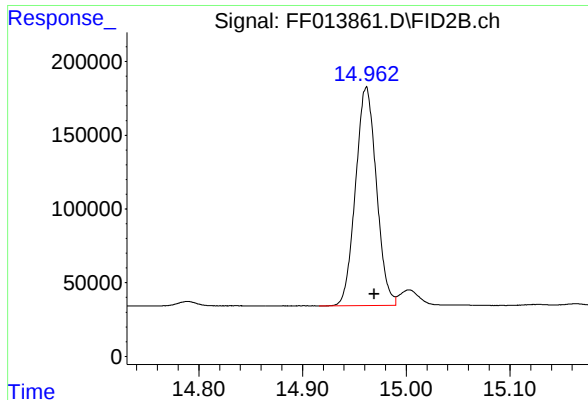

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.961 min
Delta R.T.: -0.008 min
Response: 2072354
Conc: 17.54 ug/ml

Instrument :
FID_F
ClientSampleId :

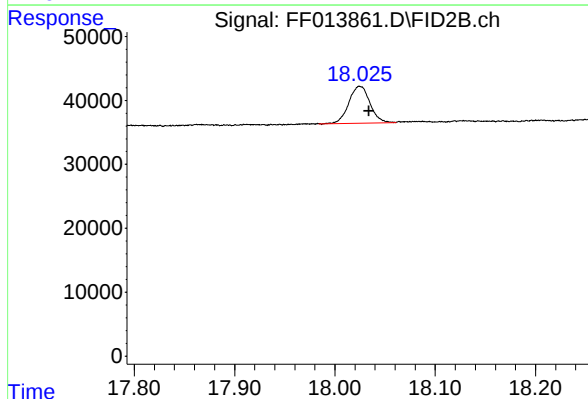


#13 N-TRIACONTANE

R.T.: 18.025 min
Delta R.T.: -0.009 min
Response: 83832
Conc: 0.71 ug/ml

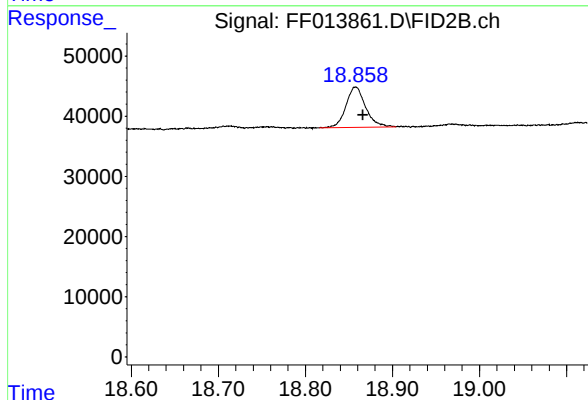

#14 N-DOTRIACONTANE

R.T.: 18.858 min
Delta R.T.: -0.008 min
Response: 104359
Conc: 0.92 ug/ml

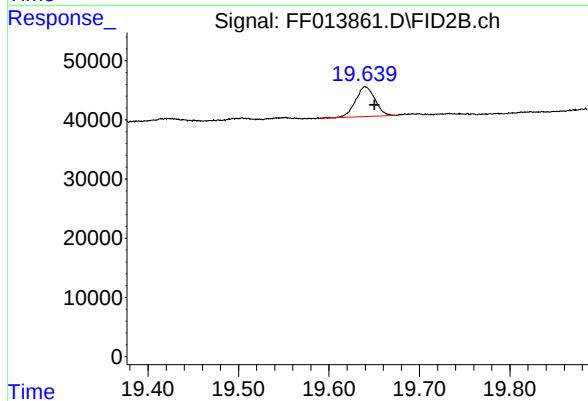

#15 N-TETRATRIACONTANE

R.T.: 19.640 min
Delta R.T.: -0.010 min
Response: 75017
Conc: 0.77 ug/ml