

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121423\
Data File : FF013856.D
Signal(s) : FID2B.ch
Acq On : 14 Dec 2023 14:19
Operator : YP\AJ
Sample : 05827-02
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT-SB-07-14-15

Integration File: autoint1.e
Quant Time: Dec 14 23:28:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120523.M
Quant Title :
QLast Update : Tue Dec 05 11:16:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.963	2359252	19.965 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121423\
Data File : FF013856.D
Signal(s) : FID2B.ch
Acq On : 14 Dec 2023 14:19
Operator : YP\AJ
Sample : 05827-02
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT-SB-07-14-15

Integration File: autoint1.e
Quant Time: Dec 14 23:28:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120523.M
Quant Title :
QLast Update : Tue Dec 05 11:16:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

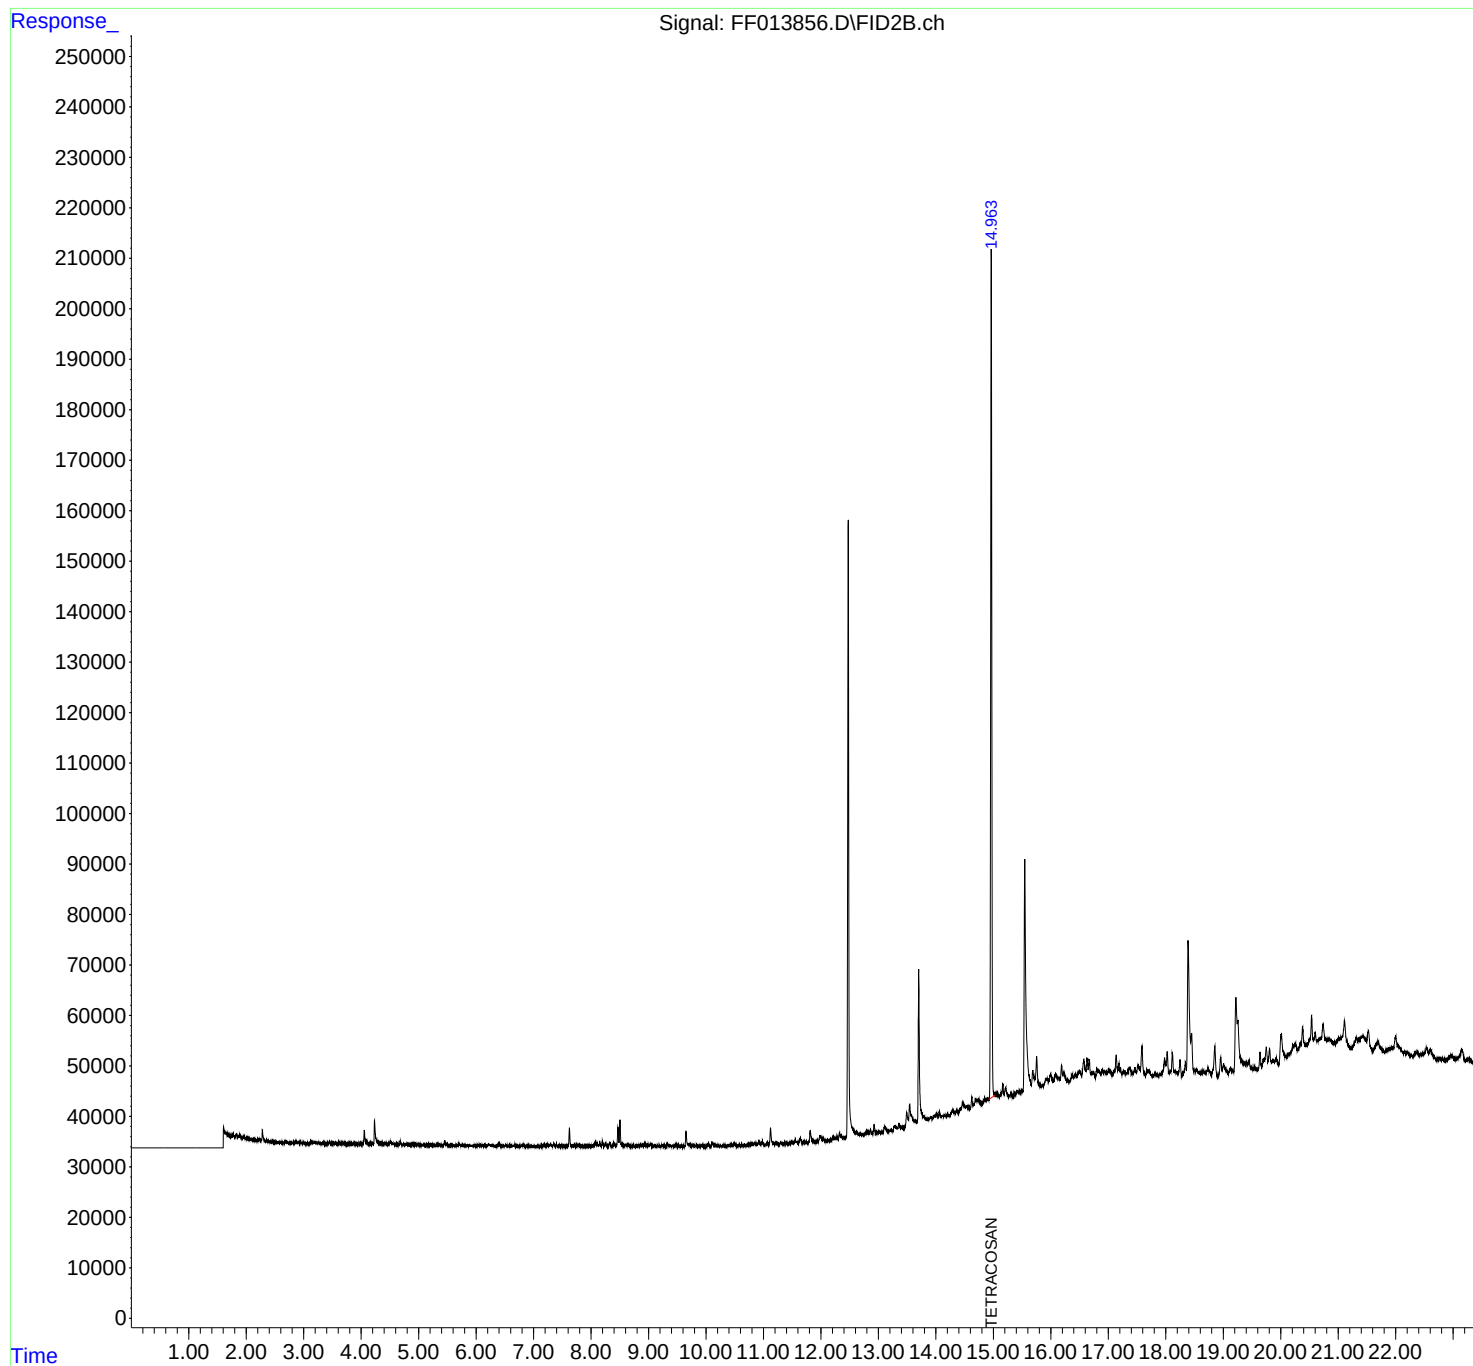

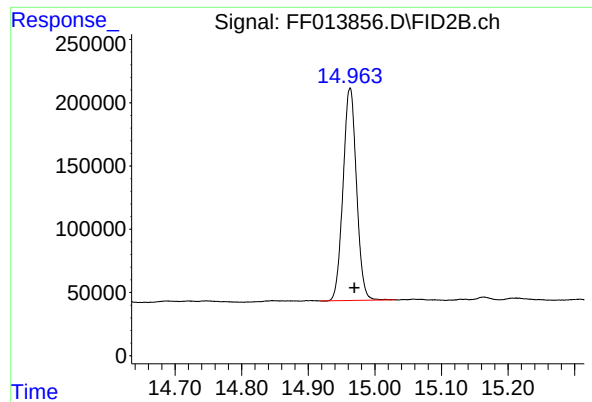

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.963 min
Delta R.T.: -0.007 min
Response: 2359252
Conc: 19.96 ug/ml

Instrument :
FID_F
ClientSampleId :
RT-SB-07-14-15