

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121423\
Data File : FF013857.D
Signal(s) : FID2B.ch
Acq On : 14 Dec 2023 14:48
Operator : YP\AJ
Sample : 05827-05
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT-SB-08-13.5-14.5

Integration File: autoint1.e
Quant Time: Dec 14 23:28:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120523.M
Quant Title :
QLast Update : Tue Dec 05 11:16:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.962	2753816	23.304 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121423\
Data File : FF013857.D
Signal(s) : FID2B.ch
Acq On : 14 Dec 2023 14:48
Operator : YP\AJ
Sample : 05827-05
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT-SB-08-13.5-14.5

Integration File: autoint1.e
Quant Time: Dec 14 23:28:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120523.M
Quant Title :
QLast Update : Tue Dec 05 11:16:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

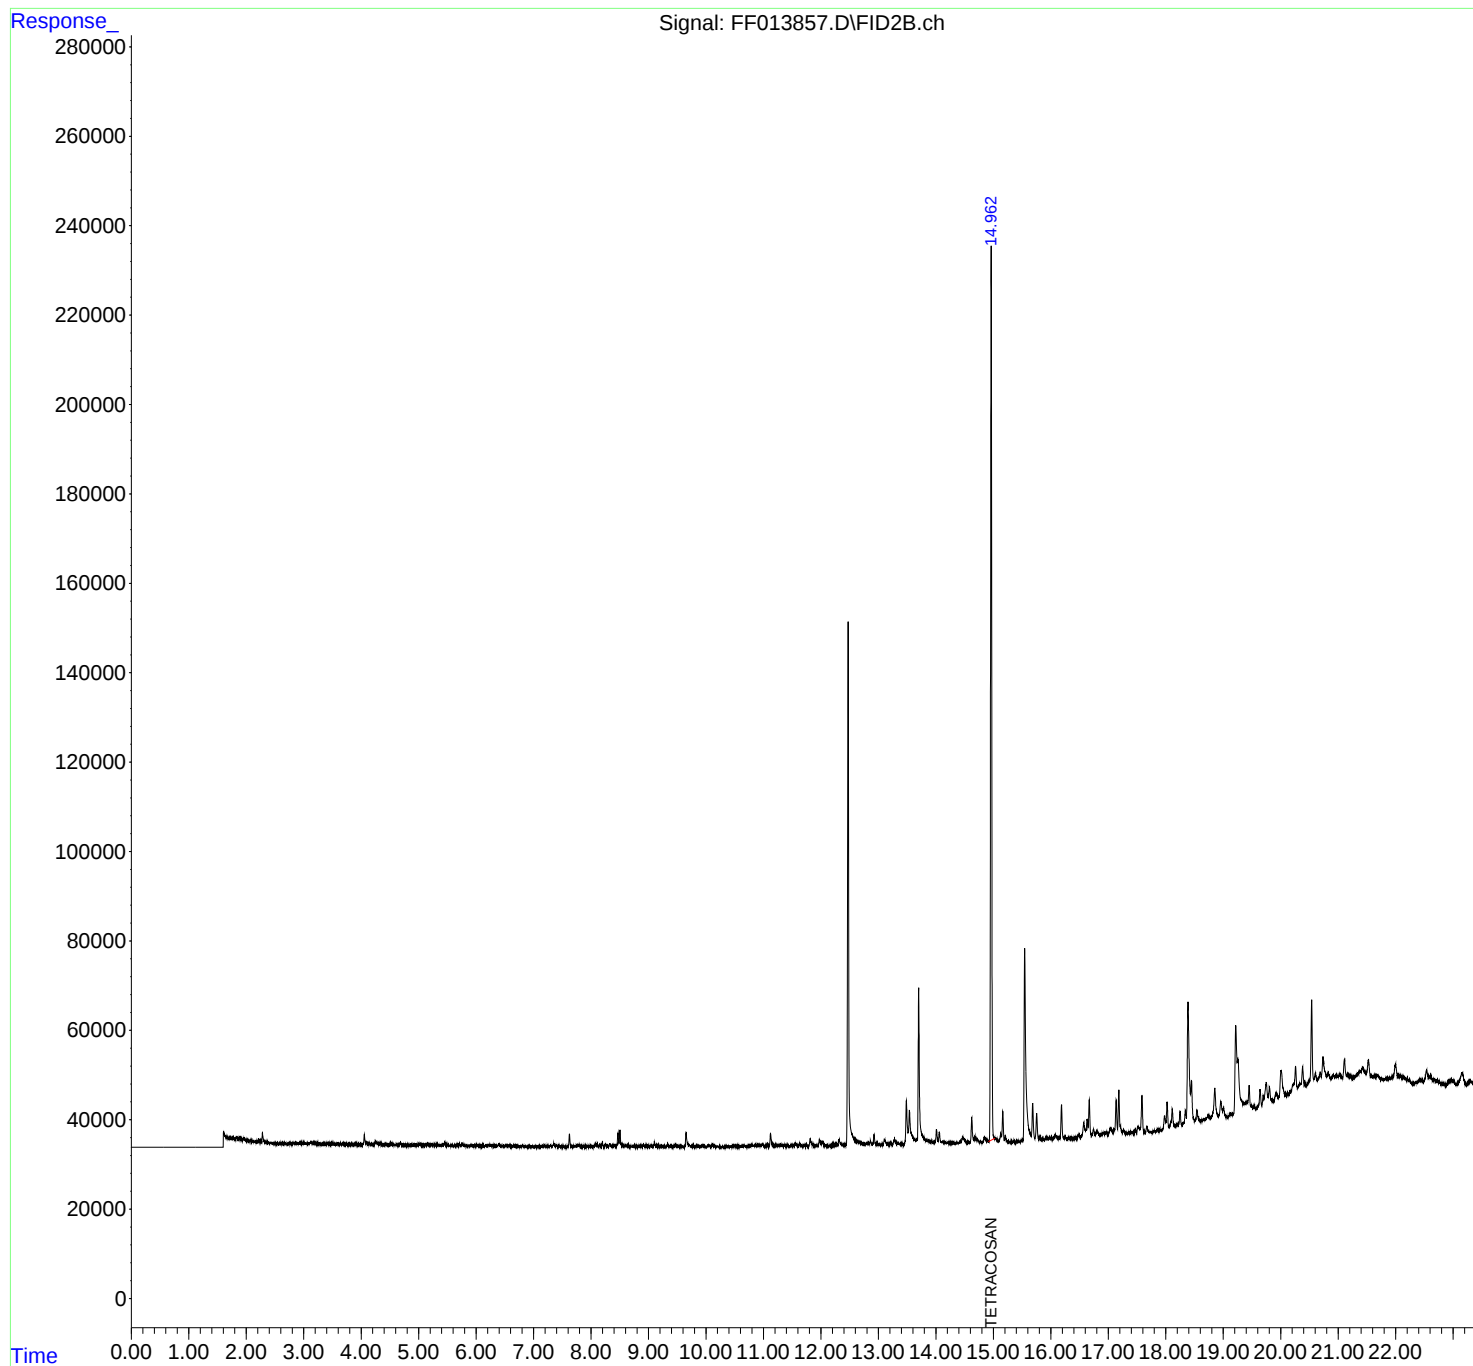

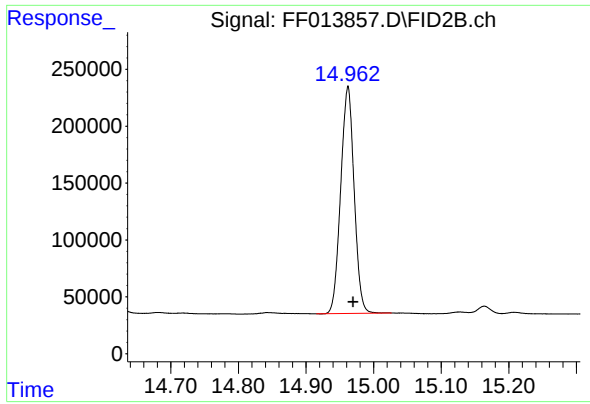

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.962 min
Delta R.T.: -0.007 min
Response: 2753816
Conc: 23.30 ug/ml

Instrument :
FID_F
ClientSampleId :
RT-SB-08-13.5-14.5