

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121520\
 Data File : FF008003.D
 Signal(s) : FID2B.ch
 Acq On : 15 Dec 2020 10:11
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Dec 16 00:53:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120220.M
 Quant Title :
 QLast Update : Thu Dec 03 09:08:10 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.440	4063779	28.218 ug/ml
12) N-OCTACOSANE	16.881	3556218	26.277 ug/ml
13) N-TRIACONTANE	17.768	194148	1.533 ug/ml
14) N-DOTRIACONTANE	18.605	314392	2.836 ug/ml
15) N-TETRATRIACONTANE	19.389	200370	2.335 ug/ml
16) N-HEXATRIACONTANE	20.134	165400	2.546 ug/ml
18) N-TETRACONTANE	21.851	346939	6.186 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121520\
Data File : FF008003.D
Signal(s) : FID2B.ch
Acq On : 15 Dec 2020 10:11
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Dec 16 00:53:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120220.M
Quant Title :
QLast Update : Thu Dec 03 09:08:10 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

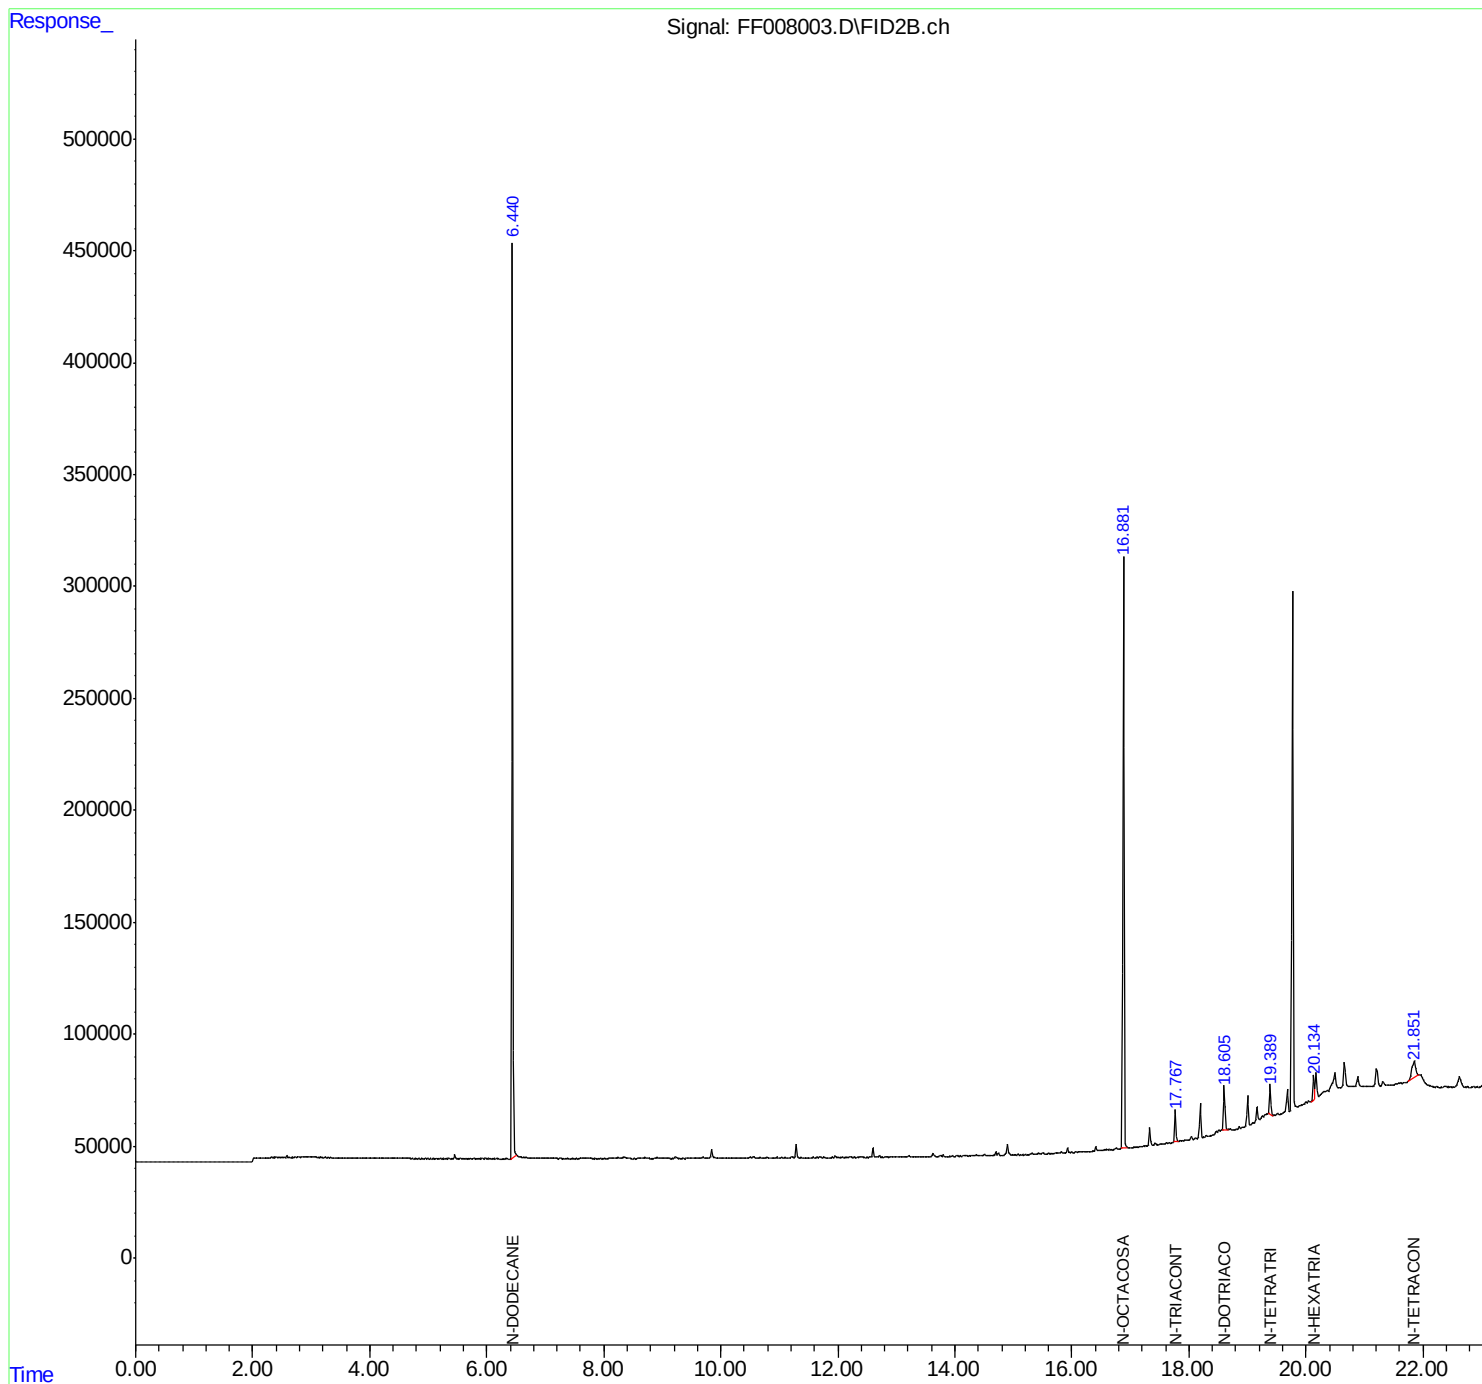


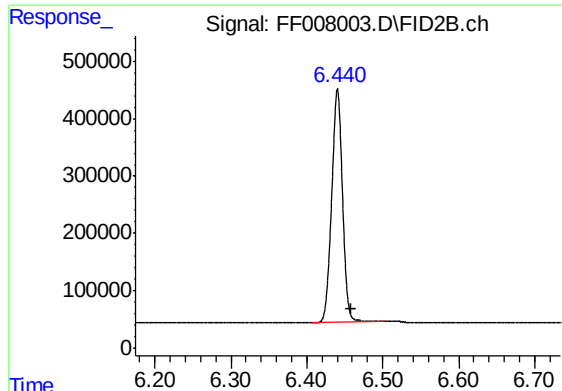

#3 N-DODECANE


R.T.: 6.440 min
Delta R.T.: -0.019 min
Response: 4063779
Conc: 28.22 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

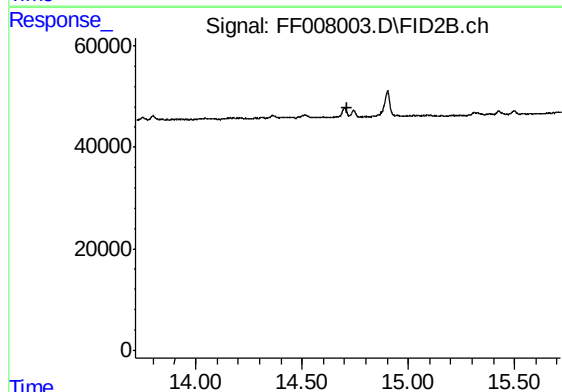


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.716 min
Response: 0
Conc: N.D.

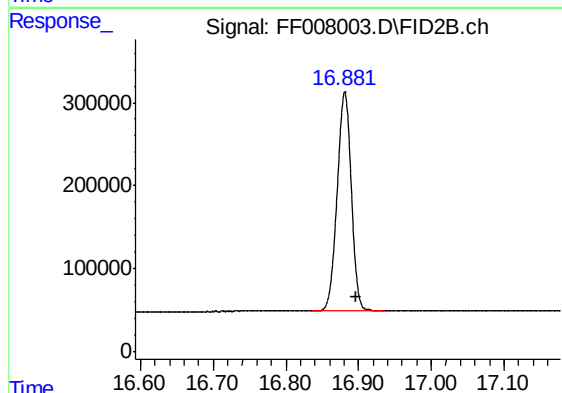


#12 N-OCTACOSANE

R.T.: 16.881 min
Delta R.T.: -0.016 min
Response: 3556218
Conc: 26.28 ug/ml

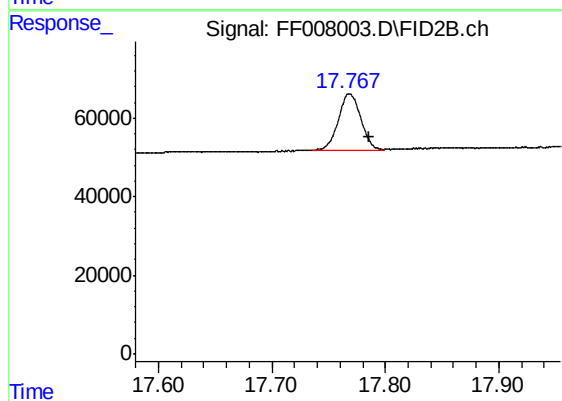

#13 N-TRIACONTANE


R.T.: 17.768 min
Delta R.T.: -0.018 min
Response: 194148
Conc: 1.53 ug/ml

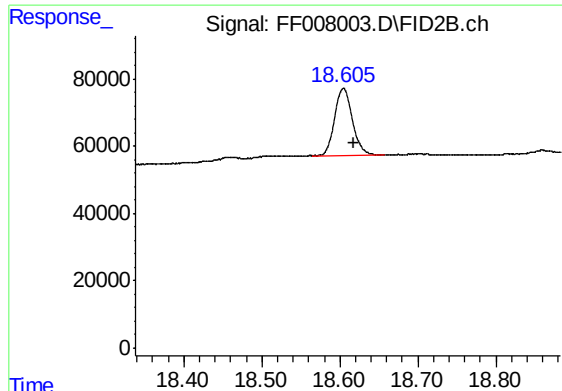

#14 N-DOTRIACONTANE


R.T.: 18.605 min
Delta R.T.: -0.014 min
Response: 314392
Conc: 2.84 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

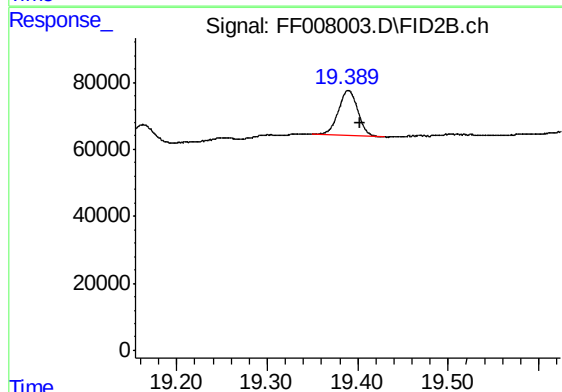


#15 N-TETRATRIACONTANE

R.T.: 19.389 min
Delta R.T.: -0.014 min
Response: 200370
Conc: 2.33 ug/ml

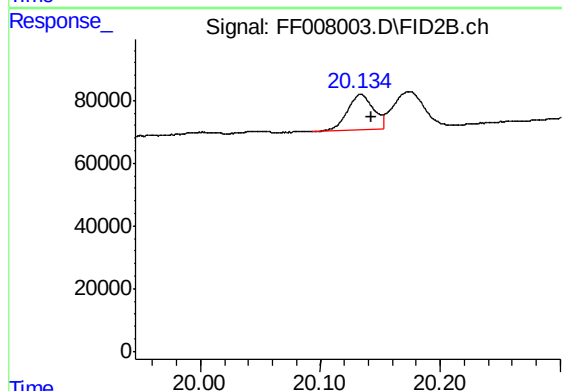

#16 N-HEXATRIACONTANE

R.T.: 20.134 min
Delta R.T.: -0.009 min
Response: 165400
Conc: 2.55 ug/ml

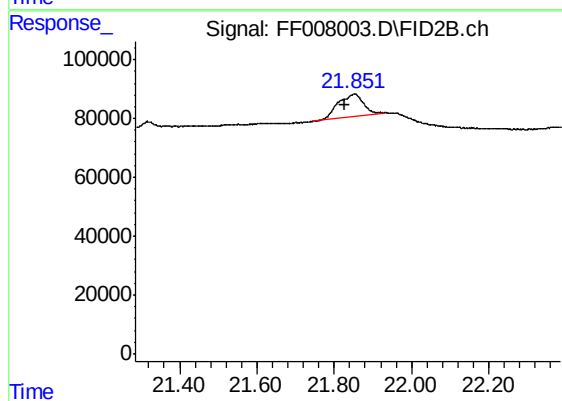

#18 N-TETRACONTANE

R.T.: 21.851 min
Delta R.T.: 0.024 min
Response: 346939
Conc: 6.19 ug/ml