

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121520\
Data File : FF008009.D
Signal(s) : FID2B.ch
Acq On : 15 Dec 2020 13:49
Operator : DD\AJ
Sample : L5066-04 200X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
JBD-BOLLARDS-0-6

Integration File: autoint1.e
Quant Time: Dec 16 00:54:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120220.M
Quant Title :
QLast Update : Thu Dec 03 09:08:10 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
4) N-TETRADECANE	8.288	184992	1.260 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121520\
Data File : FF008009.D
Signal(s) : FID2B.ch
Acq On : 15 Dec 2020 13:49
Operator : DD\AJ
Sample : L5066-04 200X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
JBD-BOLLARDS-0-6

Integration File: autoint1.e
Quant Time: Dec 16 00:54:23 2020
Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120220.M
Quant Title :
QLast Update : Thu Dec 03 09:08:10 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

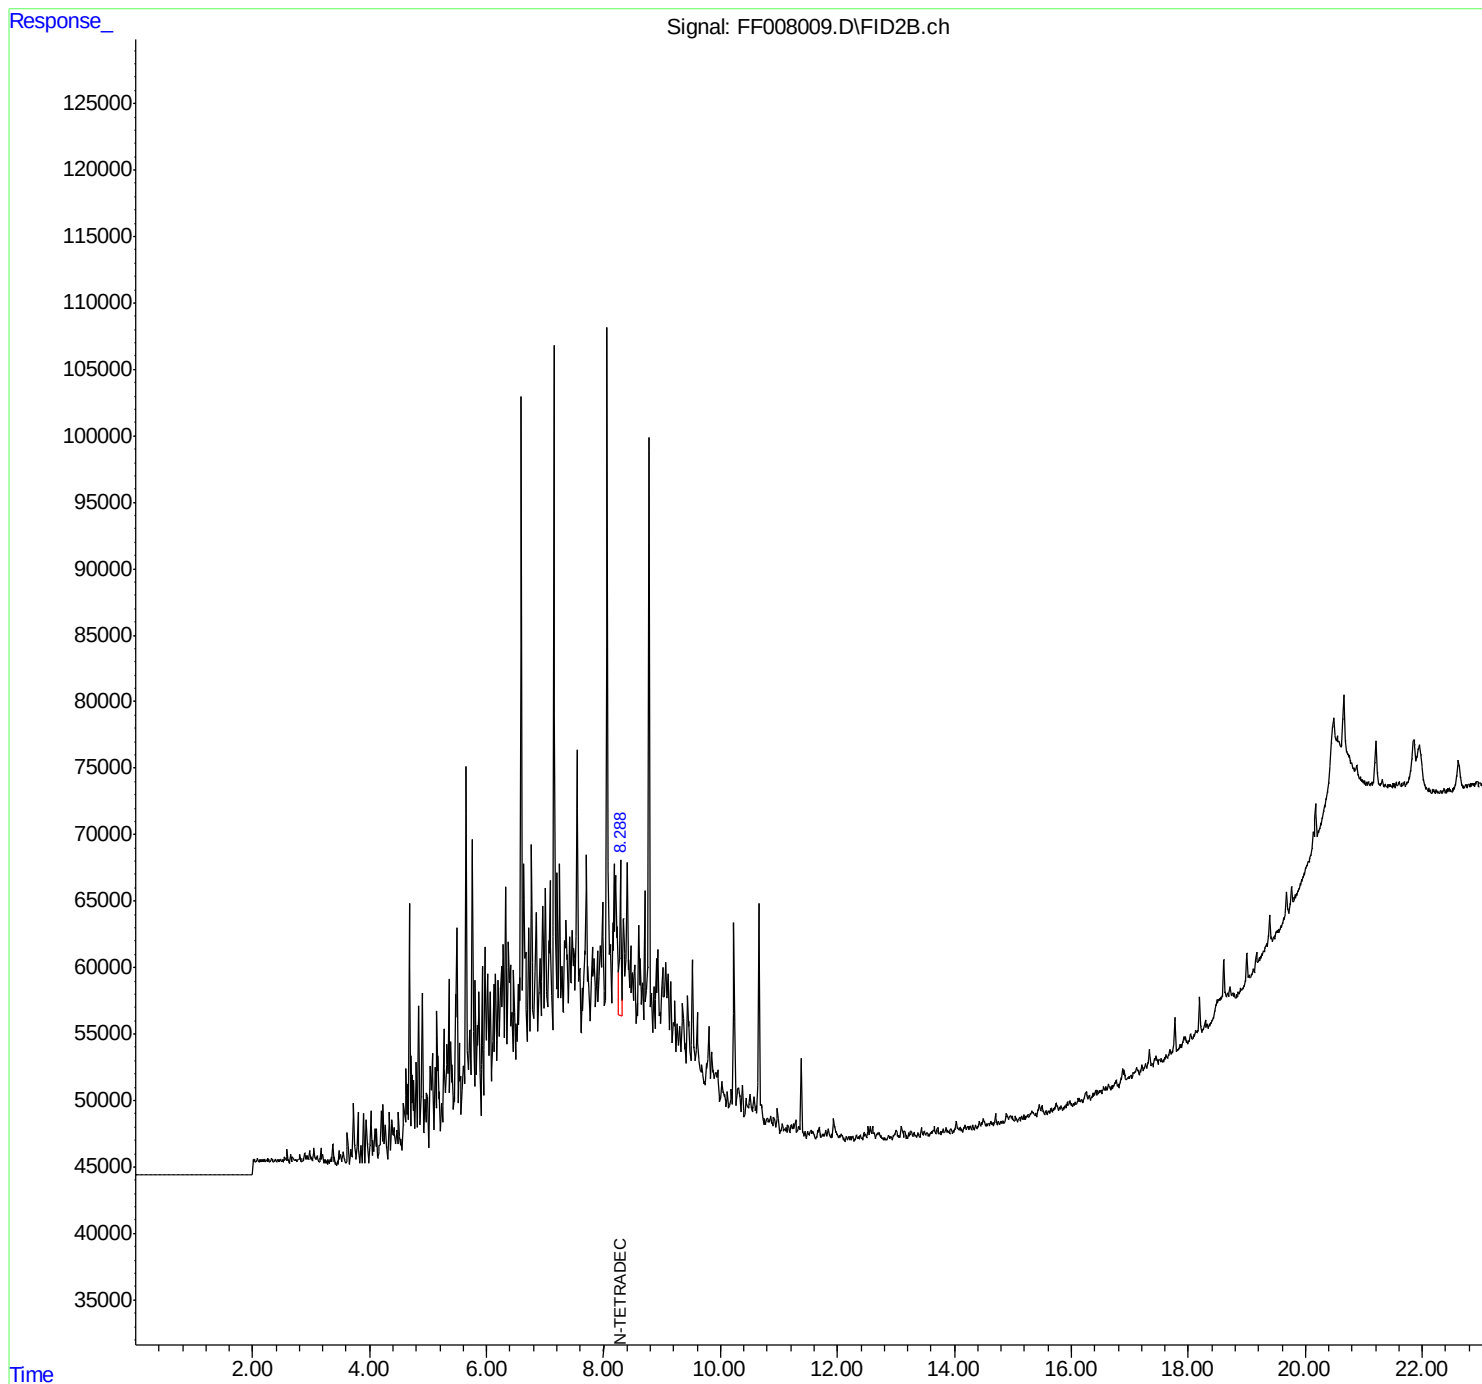


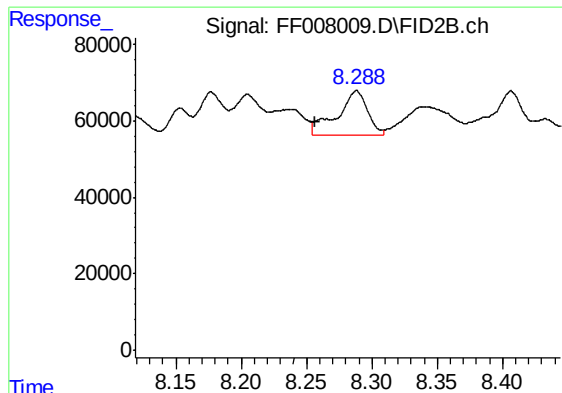

#4 N-TETRADECANE

R.T.: 8.288 min
Delta R.T.: 0.032 min
Response: 184992
Conc: 1.26 ug/ml

Instrument :
FID_F
ClientSampleId :
JBD-BOLLARDS-0-6

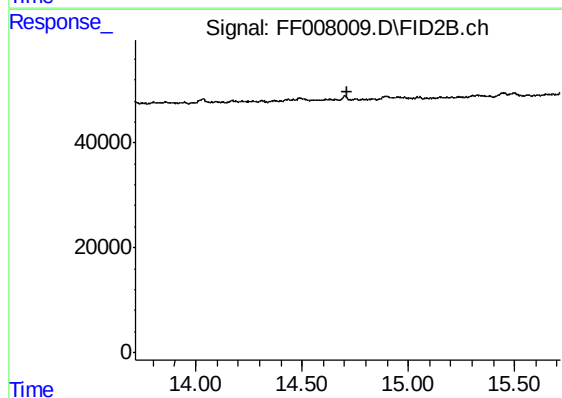

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.716 min
Response: 0
Conc: N.D.