

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121521\
Data File : FF009443.D
Signal(s) : FID2B.ch
Acq On : 15 Dec 2021 20:56
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 03:40:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.480	2305521	19.903 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.356	45996	0.421 ug/ml
15)	N-TETRATRIACONTANE	19.140	37880	0.358 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121521\
Data File : FF009443.D
Signal(s) : FID2B.ch
Acq On : 15 Dec 2021 20:56
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 03:40:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

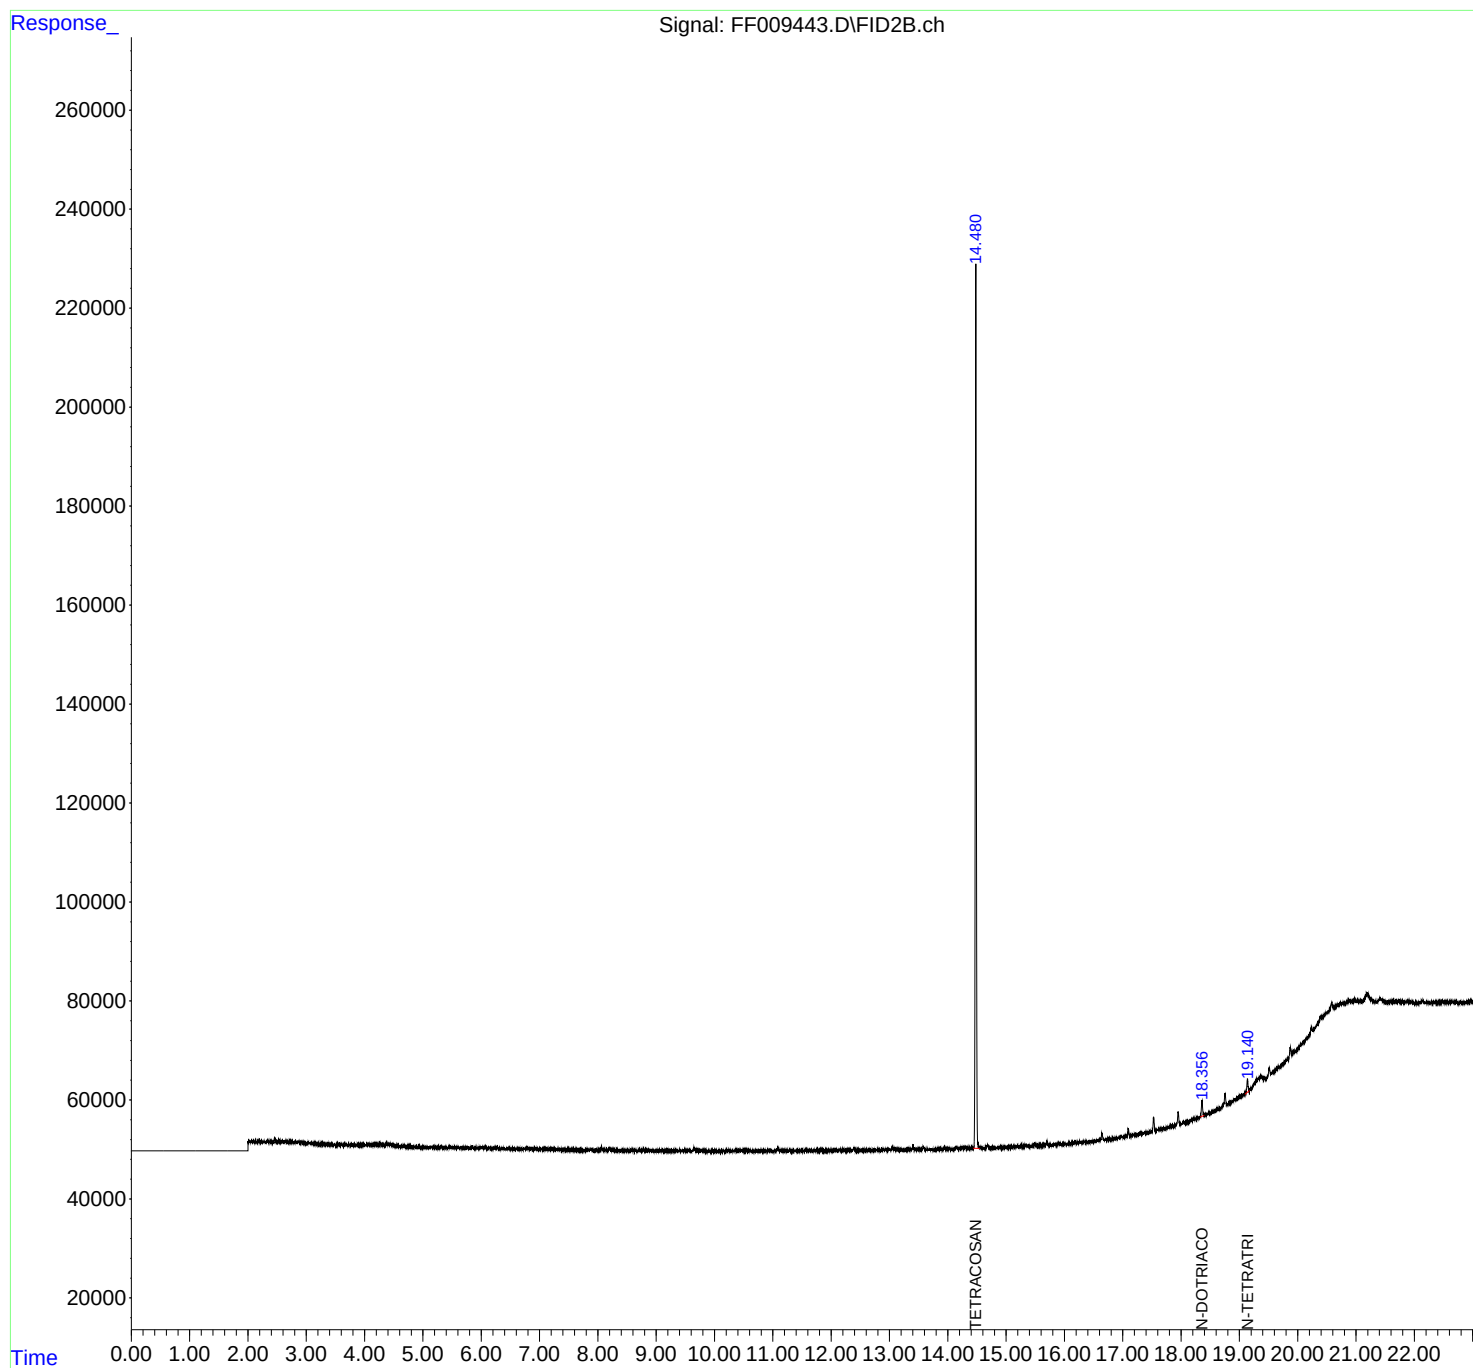


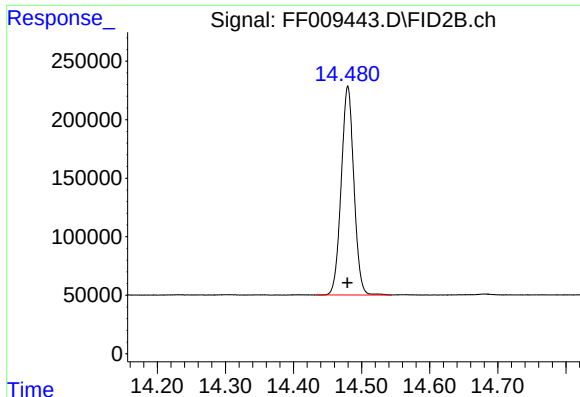

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.480 min
Delta R.T.: 0.000 min
Response: 2305521
Conc: 19.90 ug/ml

Instrument :
FID_F
ClientSampleId :

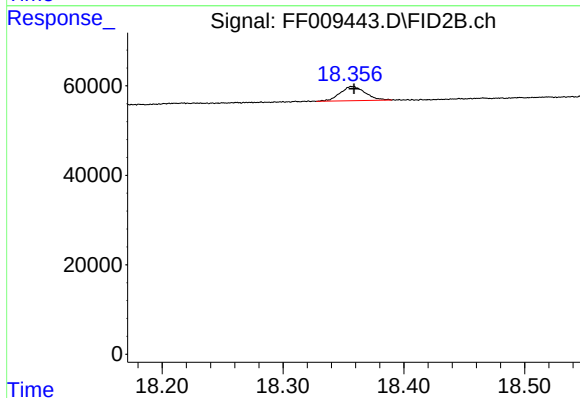

#14 N-DOTRIACONTANE

R.T.: 18.356 min
Delta R.T.: -0.003 min
Response: 45996
Conc: 0.42 ug/ml

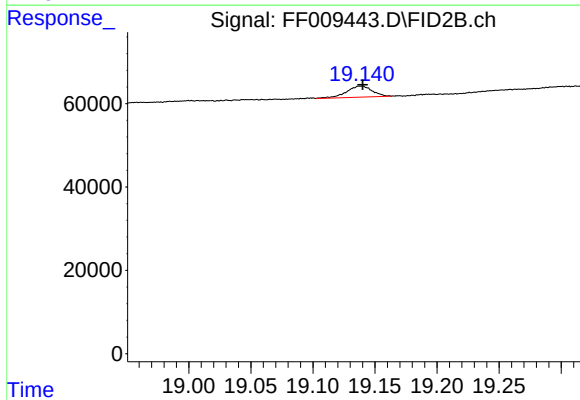

#15 N-TETRATRIACONTANE

R.T.: 19.140 min
Delta R.T.: 0.000 min
Response: 37880
Conc: 0.36 ug/ml